

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032619\
 Data File : VU030451.D
 Acq On : 26 Mar 2019 18:18
 Operator : JC/SP
 Sample : K2022-13 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C09D0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.183	24	29	34	rVB2	13794	12816	0.44%	0.074%
2	1.399	89	96	110	rBV	276282	279619	9.51%	1.613%
3	1.672	174	181	207	rVB	208587	281780	9.58%	1.625%
4	2.183	336	340	348	rVB5	6274	8124	0.28%	0.047%
5	2.270	356	367	381	rBV	413473	630515	21.44%	3.637%
6	2.367	394	397	402	rVB	1947	1657	0.06%	0.010%
7	2.441	413	420	422	rBV3	2263	2731	0.09%	0.016%
8	2.592	462	467	470	rBV	1073	1187	0.04%	0.007%
9	2.650	481	485	487	rBV2	1339	1226	0.04%	0.007%
10	2.756	513	518	521	rBV2	1213	1354	0.05%	0.008%
11	2.881	553	557	561	rBV	1373	1199	0.04%	0.007%
12	3.026	596	602	604	rBV	1013	1092	0.04%	0.006%
13	3.469	734	740	742	rBV	1344	1201	0.04%	0.007%
14	3.752	824	828	831	rBV	2033	1233	0.04%	0.007%
15	3.865	860	863	866	rBV	1451	1085	0.04%	0.006%
16	4.048	914	920	923	rBV2	1240	1626	0.06%	0.009%
17	4.174	946	959	992	rBV	209914	555539	18.89%	3.205%
18	4.518	1063	1066	1069	rBV	1739	1149	0.04%	0.007%
19	4.643	1089	1105	1135	rVV	304482	716384	24.36%	4.132%
20	4.994	1212	1214	1219	rVV	1171	1221	0.04%	0.007%
21	5.016	1219	1221	1226	rVV	1556	1198	0.04%	0.007%
22	5.064	1229	1236	1239	rBV	2059	2146	0.07%	0.012%
23	5.161	1262	1266	1272	rBV2	1037	1100	0.04%	0.006%
24	5.238	1283	1290	1293	rBV	1315	1856	0.06%	0.011%
25	5.338	1297	1321	1354	rBV2	622183	1907960	64.88%	11.006%
26	5.617	1401	1408	1413	rVB2	2088	2527	0.09%	0.015%
27	5.778	1455	1458	1461	rBV	1774	1189	0.04%	0.007%
28	5.884	1476	1491	1511	rBV	538268	1086746	36.95%	6.269%
29	6.190	1580	1586	1593	rVB	2103	2427	0.08%	0.014%
30	6.328	1615	1629	1655	rBV	425605	875271	29.76%	5.049%
31	6.566	1700	1703	1707	rVB	2154	1552	0.05%	0.009%
32	6.588	1707	1710	1712	rVB	1967	1133	0.04%	0.007%
33	6.611	1712	1717	1720	rBV	1309	1258	0.04%	0.007%
34	6.694	1740	1743	1747	rBV	2031	1717	0.06%	0.010%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032619\
 Data File : VU030451.D
 Acq On : 26 Mar 2019 18:18
 Operator : JC/SP
 Sample : K2022-13 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C09D0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

35	6.743	1754	1758	1762	rVB	2037	1833	0.06%	0.011%
36	6.772	1762	1767	1771	rBV	1333	1615	0.05%	0.009%
37	6.791	1771	1773	1785	rVB	2303	2962	0.10%	0.017%
38	6.865	1785	1796	1802	rBV	2287	4415	0.15%	0.025%
39	6.894	1802	1805	1809	rVV	1532	1463	0.05%	0.008%
40	6.926	1813	1815	1819	rVV	1579	1112	0.04%	0.006%
41	7.061	1854	1857	1862	rBV	1385	1130	0.04%	0.007%
42	7.090	1862	1866	1875	rVB	1669	2275	0.08%	0.013%
43	7.128	1875	1878	1884	rBV	1284	1444	0.05%	0.008%
44	7.225	1896	1908	1935	rBV	231429	435697	14.82%	2.513%
45	7.337	1941	1943	1947	rBV	2012	1396	0.05%	0.008%
46	7.434	1968	1973	1979	rBV	1555	1707	0.06%	0.010%
47	7.563	1998	2013	2042	rBV	792648	1418590	48.24%	8.183%
48	7.846	2089	2101	2119	rBV	159966	284899	9.69%	1.643%
49	7.971	2134	2140	2145	rBV	1780	2320	0.08%	0.013%
50	8.083	2172	2175	2180	rVV	1800	1449	0.05%	0.008%
51	8.141	2189	2193	2196	rBV	1484	1085	0.04%	0.006%
52	8.196	2207	2210	2218	rVB2	1529	1402	0.05%	0.008%
53	8.244	2222	2225	2230	rVB2	1999	1743	0.06%	0.010%
54	8.309	2234	2245	2280	rBV	635895	1174933	39.95%	6.778%
55	8.489	2295	2301	2305	rBV	1915	2264	0.08%	0.013%
56	8.591	2329	2333	2336	rBV	1882	1737	0.06%	0.010%
57	8.890	2423	2426	2431	rBV	1448	1329	0.05%	0.008%
58	8.968	2444	2450	2453	rBV	1364	1171	0.04%	0.007%
59	9.087	2475	2487	2492	rBV	826717	1417921	48.22%	8.179%
60	9.411	2585	2588	2592	rVB	1869	1353	0.05%	0.008%
61	9.627	2652	2655	2658	rVB	2142	1332	0.05%	0.008%
62	9.649	2658	2662	2667	rBV	1462	1709	0.06%	0.010%
63	9.852	2722	2725	2731	rVB	1431	1361	0.05%	0.008%
64	9.916	2741	2745	2749	rBV	1340	1470	0.05%	0.008%
65	9.977	2761	2764	2767	rVB	2280	1565	0.05%	0.009%
66	10.019	2772	2777	2780	rBV	1646	1561	0.05%	0.009%
67	10.064	2784	2791	2794	rBV	2107	2152	0.07%	0.012%
68	10.177	2820	2826	2828	rBV	1325	1265	0.04%	0.007%
69	10.427	2892	2904	2926	rBV	579266	948725	32.26%	5.473%
70	10.685	2976	2984	2988	rBV2	2398	3046	0.10%	0.018%
71	10.759	3002	3007	3009	rBV2	1087	1180	0.04%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032619\
 Data File : VU030451.D
 Acq On : 26 Mar 2019 18:18
 Operator : JC/SP
 Sample : K2022-13 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C09D0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

72	10.964	3065	3071	3073	rBV2	1768	2021	0.07%	0.012%
73	11.115	3115	3118	3121	rVV	1948	1280	0.04%	0.007%
74	11.135	3121	3124	3131	rVB	1523	1511	0.05%	0.009%
75	11.173	3131	3136	3139	rBV2	1290	1275	0.04%	0.007%
76	11.353	3189	3192	3197	rVB	1828	1331	0.05%	0.008%
77	11.414	3197	3211	3221	rBV3	59550	99614	3.39%	0.575%
78	11.482	3221	3232	3254	rVV2	719230	1537070	52.27%	8.867%
79	11.736	3305	3311	3316	rBV	1624	2002	0.07%	0.012%
80	11.791	3325	3328	3332	rVB2	2025	1437	0.05%	0.008%
81	11.871	3333	3353	3374	rBV2	1274425	2940766	100.00%	16.964%
82	12.064	3410	3413	3418	rBV2	1435	1285	0.04%	0.007%
83	12.437	3522	3529	3531	rBV	1600	1387	0.05%	0.008%
84	12.582	3572	3574	3581	rVB	1154	1077	0.04%	0.006%
85	12.656	3594	3597	3604	rVB	3593	4008	0.14%	0.023%
86	12.697	3604	3610	3614	rBV	1377	1657	0.06%	0.010%
87	12.910	3670	3676	3681	rBV	2023	2218	0.08%	0.013%
88	13.064	3722	3724	3730	rVB	1817	1369	0.05%	0.008%
89	13.138	3742	3747	3750	rBV	2051	1739	0.06%	0.010%
90	13.389	3822	3825	3829	rVB2	1509	1126	0.04%	0.006%
91	13.501	3849	3860	3886	rBV	271656	488395	16.61%	2.817%
92	13.987	3997	4011	4031	rBV5	48867	104132	3.54%	0.601%
93	14.205	4074	4079	4082	rBV	2307	2549	0.09%	0.015%
94	14.331	4116	4118	4122	rVB	2120	1258	0.04%	0.007%
95	14.353	4122	4125	4130	rBV	1861	1633	0.06%	0.009%
96	14.514	4173	4175	4180	rVB	1694	1119	0.04%	0.006%
97	14.565	4188	4191	4195	rVB	1888	1312	0.04%	0.008%
98	14.588	4195	4198	4205	rBV	2373	2150	0.07%	0.012%
99	14.852	4277	4280	4287	rBV2	1498	1655	0.06%	0.010%
100	15.559	4495	4500	4503	rBV	1686	1758	0.06%	0.010%


Sum of corrected areas: 17335563

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU032619\
Data File : VU030451.D
Acq On : 26 Mar 2019 18:18
Operator : JC/SP
Sample : K2022-13 50X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C09D0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

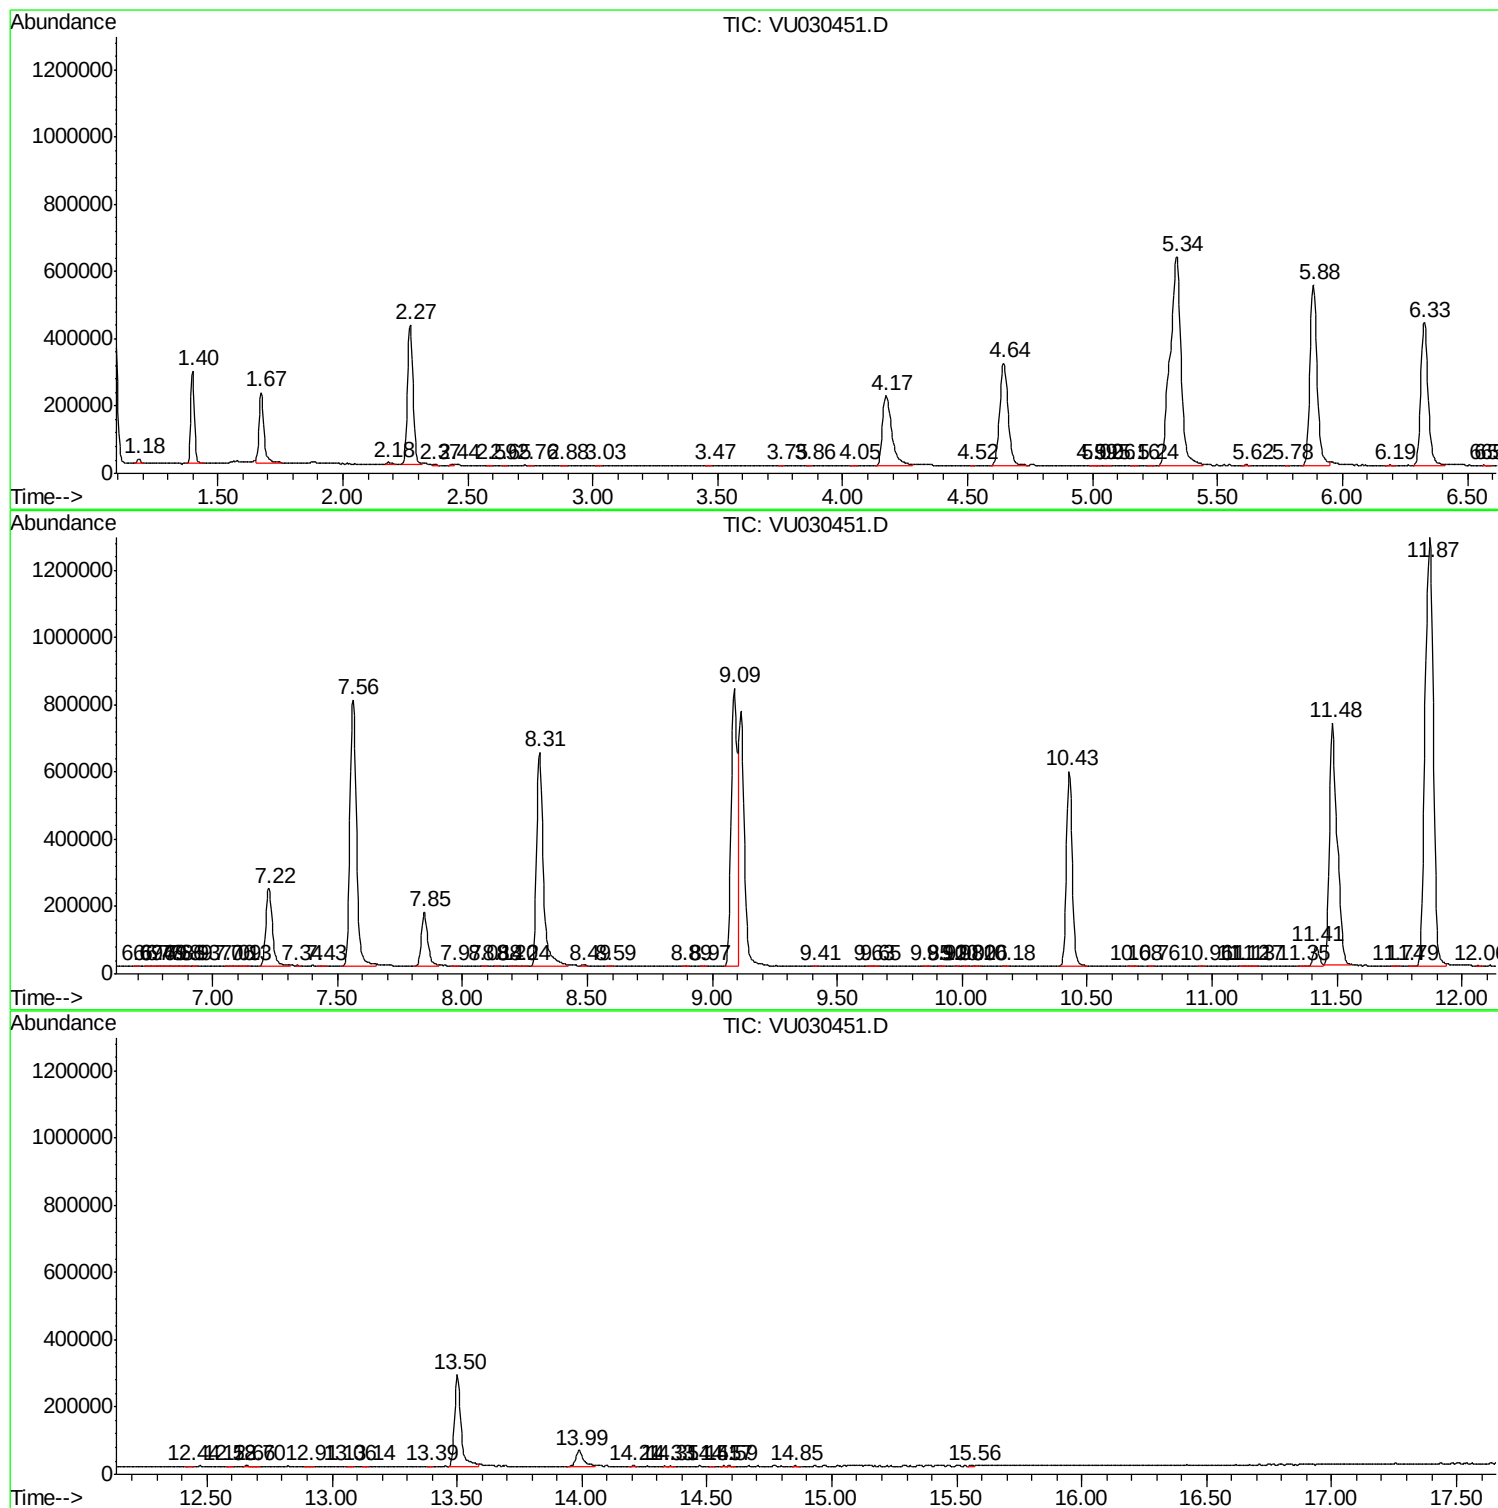

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032619\
Data File : VU030451.D
Acq On : 26 Mar 2019 18:18
Operator : JC/SP
Sample : K2022-13 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C09D0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032619\
Data File : VU030451.D
Acq On : 26 Mar 2019 18:18
Operator : JC/SP
Sample : K2022-13 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C09D0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc