

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032619\
 Data File : VU030453.D
 Acq On : 26 Mar 2019 19:05
 Operator : JC/SP
 Sample : K2022-15 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C09D9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.183	23	29	35	RBV3	14492	15722	0.04%	0.019%
2	1.399	89	96	107	RVB	269043	271549	0.78%	0.323%
3	1.672	173	181	196	RVB	211817	271822	0.78%	0.323%
4	2.154	329	331	333	RBV	1969	1134	0.00%	0.001%
5	2.267	356	366	379	RBV	407701	623104	1.78%	0.741%
6	2.376	397	400	405	RVB2	2366	1696	0.00%	0.002%
7	2.788	525	528	532	RBV	1960	1227	0.00%	0.001%
8	2.862	549	551	557	RVB	1855	1615	0.00%	0.002%
9	2.920	564	569	573	RBV	1377	1666	0.00%	0.002%
10	2.990	587	591	595	RBV	1320	1191	0.00%	0.001%
11	3.122	628	632	638	RVB	2135	2269	0.01%	0.003%
12	3.161	638	644	649	RBV2	1485	2462	0.01%	0.003%
13	3.482	741	744	747	RBV	1748	1135	0.00%	0.001%
14	3.582	767	775	777	RBV	1297	1647	0.00%	0.002%
15	3.694	807	810	814	RBV	2163	1579	0.00%	0.002%
16	3.842	852	856	860	RVB	2681	2212	0.01%	0.003%
17	3.965	892	894	903	RVB	1868	1961	0.01%	0.002%
18	4.077	921	929	931	RBV	3307	4492	0.01%	0.005%
19	4.174	947	959	989	RBV	209661	560484	1.60%	0.667%
20	4.553	1074	1077	1080	RBV	1667	1122	0.00%	0.001%
21	4.646	1089	1106	1131	RBV2	322933	836037	2.39%	0.994%
22	4.987	1209	1212	1215	RBV2	1669	1231	0.00%	0.001%
23	5.135	1243	1258	1271	RVB3	21713	50783	0.15%	0.060%
24	5.337	1295	1321	1325	RBV2	658112	1705842	4.88%	2.029%
25	5.386	1326	1336	1382	RVB	3944941	8457147	24.19%	10.057%
26	5.881	1472	1490	1515	RBV	558761	1127839	3.23%	1.341%
27	6.103	1553	1559	1561	RBV2	1488	1814	0.01%	0.002%
28	6.144	1569	1572	1577	RVB2	1544	1121	0.00%	0.001%
29	6.190	1580	1586	1591	RBV	1963	2627	0.01%	0.003%
30	6.328	1614	1629	1652	RBV	429212	877025	2.51%	1.043%
31	6.537	1691	1694	1703	RVB	1886	2100	0.01%	0.002%
32	6.627	1716	1722	1723	RBV	1836	1556	0.00%	0.002%
33	6.678	1731	1738	1741	RBV	1390	1511	0.00%	0.002%
34	6.749	1757	1760	1764	RVV	1529	1294	0.00%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032619\
 Data File : VU030453.D
 Acq On : 26 Mar 2019 19:05
 Operator : JC/SP
 Sample : K2022-15 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C09D9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

35	6.923	1805	1814	1818	rBV	2050	2342	0.01%	0.003%
36	7.026	1843	1846	1850	rVB	2154	1380	0.00%	0.002%
37	7.087	1862	1865	1869	rVB	1722	1214	0.00%	0.001%
38	7.225	1896	1908	1927	rBV	235310	432631	1.24%	0.514%
39	7.463	1978	1982	1985	rBV	1435	1239	0.00%	0.001%
40	7.562	2000	2013	2032	rBV	789512	1413009	4.04%	1.680%
41	7.845	2090	2101	2127	rBV	165091	296642	0.85%	0.353%
42	7.939	2127	2130	2134	rVV2	3073	2600	0.01%	0.003%
43	7.961	2134	2137	2142	rVB	2036	1536	0.00%	0.002%
44	8.013	2151	2153	2159	rVB2	1678	1413	0.00%	0.002%
45	8.061	2162	2168	2173	rBV	1802	2140	0.01%	0.003%
46	8.112	2177	2184	2189	rVB	1170	1581	0.00%	0.002%
47	8.231	2215	2221	2224	rVB2	1559	1243	0.00%	0.001%
48	8.254	2224	2228	2233	rBV	1853	2341	0.01%	0.003%
49	8.308	2234	2245	2283	rVV	660034	1198593	3.43%	1.425%
50	8.562	2321	2324	2331	rBV	1395	1462	0.00%	0.002%
51	8.730	2374	2376	2383	rVB	2376	2076	0.01%	0.002%
52	8.884	2421	2424	2433	rVB	2170	2795	0.01%	0.003%
53	8.929	2433	2438	2444	rBV	2469	2629	0.01%	0.003%
54	9.119	2470	2497	2540	rBV	20437409	34961413	100.00%	41.577%
55	9.530	2622	2625	2630	rBV2	1662	1773	0.01%	0.002%
56	9.636	2652	2658	2660	rBV	2528	2152	0.01%	0.003%
57	9.739	2687	2690	2697	rVB	1812	2014	0.01%	0.002%
58	9.794	2703	2707	2709	rBV	2332	2006	0.01%	0.002%
59	9.858	2724	2727	2732	rVB	2676	2151	0.01%	0.003%
60	10.038	2780	2783	2793	rVB	2168	3198	0.01%	0.004%
61	10.427	2891	2904	2925	rVV	588244	961499	2.75%	1.143%
62	10.566	2944	2947	2949	rBV	1894	1305	0.00%	0.002%
63	10.611	2958	2961	2964	rBV	1902	1212	0.00%	0.001%
64	10.630	2964	2967	2973	rVB	1517	1242	0.00%	0.001%
65	10.662	2973	2977	2980	rBV	1639	1526	0.00%	0.002%
66	10.710	2989	2992	2997	rBV2	1048	1223	0.00%	0.001%
67	10.951	3063	3067	3070	rBV	1938	1566	0.00%	0.002%
68	10.974	3070	3074	3078	rVB	1876	1618	0.00%	0.002%
69	11.000	3078	3082	3088	rVB	1930	1882	0.01%	0.002%
70	11.144	3121	3127	3130	rBV	1590	1521	0.00%	0.002%
71	11.202	3142	3145	3150	rBV	1684	1437	0.00%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032619\
 Data File : VU030453.D
 Acq On : 26 Mar 2019 19:05
 Operator : JC/SP
 Sample : K2022-15 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C09D9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

72	11.414	3196	3211	3222	rBV	699774	1106079	3.16%	1.315%
73	11.504	3222	3239	3271	rVB2	7087591	12246264	35.03%	14.564%
74	11.877	3334	3355	3379	rBV2	8586612	14745773	42.18%	17.536%
75	12.096	3420	3423	3427	rBV	1852	1402	0.00%	0.002%
76	12.205	3454	3457	3460	rBV3	1485	1262	0.00%	0.002%
77	12.286	3479	3482	3485	rVB	2092	1325	0.00%	0.002%
78	12.401	3509	3518	3521	rBV2	1901	2632	0.01%	0.003%
79	12.643	3584	3593	3596	rBV3	5182	6375	0.02%	0.008%
80	12.771	3631	3633	3640	rVB	2088	1547	0.00%	0.002%
81	12.842	3652	3655	3658	rBV	1638	1370	0.00%	0.002%
82	12.993	3691	3702	3711	rBV7	4323	8227	0.02%	0.010%
83	13.202	3761	3767	3772	rBV	1865	2227	0.01%	0.003%
84	13.273	3786	3789	3792	rBV	1679	1306	0.00%	0.002%
85	13.411	3825	3832	3835	rBV2	1184	1412	0.00%	0.002%
86	13.498	3846	3859	3888	rBV	837161	1391068	3.98%	1.654%
87	13.794	3949	3951	3957	rVB2	1732	1337	0.00%	0.002%
88	13.826	3957	3961	3965	rBV2	1702	1562	0.00%	0.002%
89	13.987	3996	4011	4031	rBV	210525	391191	1.12%	0.465%
90	14.128	4053	4055	4062	rVB4	1573	1573	0.00%	0.002%
91	14.186	4070	4073	4076	rBV	1765	1207	0.00%	0.001%
92	14.266	4096	4098	4106	rVB3	1483	1555	0.00%	0.002%
93	14.305	4106	4110	4113	rBV	1647	1259	0.00%	0.001%
94	14.382	4131	4134	4138	rBV	1605	1276	0.00%	0.002%
95	14.906	4290	4297	4303	rVB2	2249	3691	0.01%	0.004%
96	14.938	4303	4307	4310	rBV	3075	2572	0.01%	0.003%
97	15.086	4350	4353	4356	rBV	1666	1189	0.00%	0.001%
98	15.118	4360	4363	4366	rVB	1969	1113	0.00%	0.001%
99	15.157	4372	4375	4378	rVB	2196	1398	0.00%	0.002%
100	15.372	4439	4442	4446	rBV	1610	1339	0.00%	0.002%


Sum of corrected areas: 84088151

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU032619\
Data File : VU030453.D
Acq On : 26 Mar 2019 19:05
Operator : JC/SP
Sample : K2022-15 50X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C09D9

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

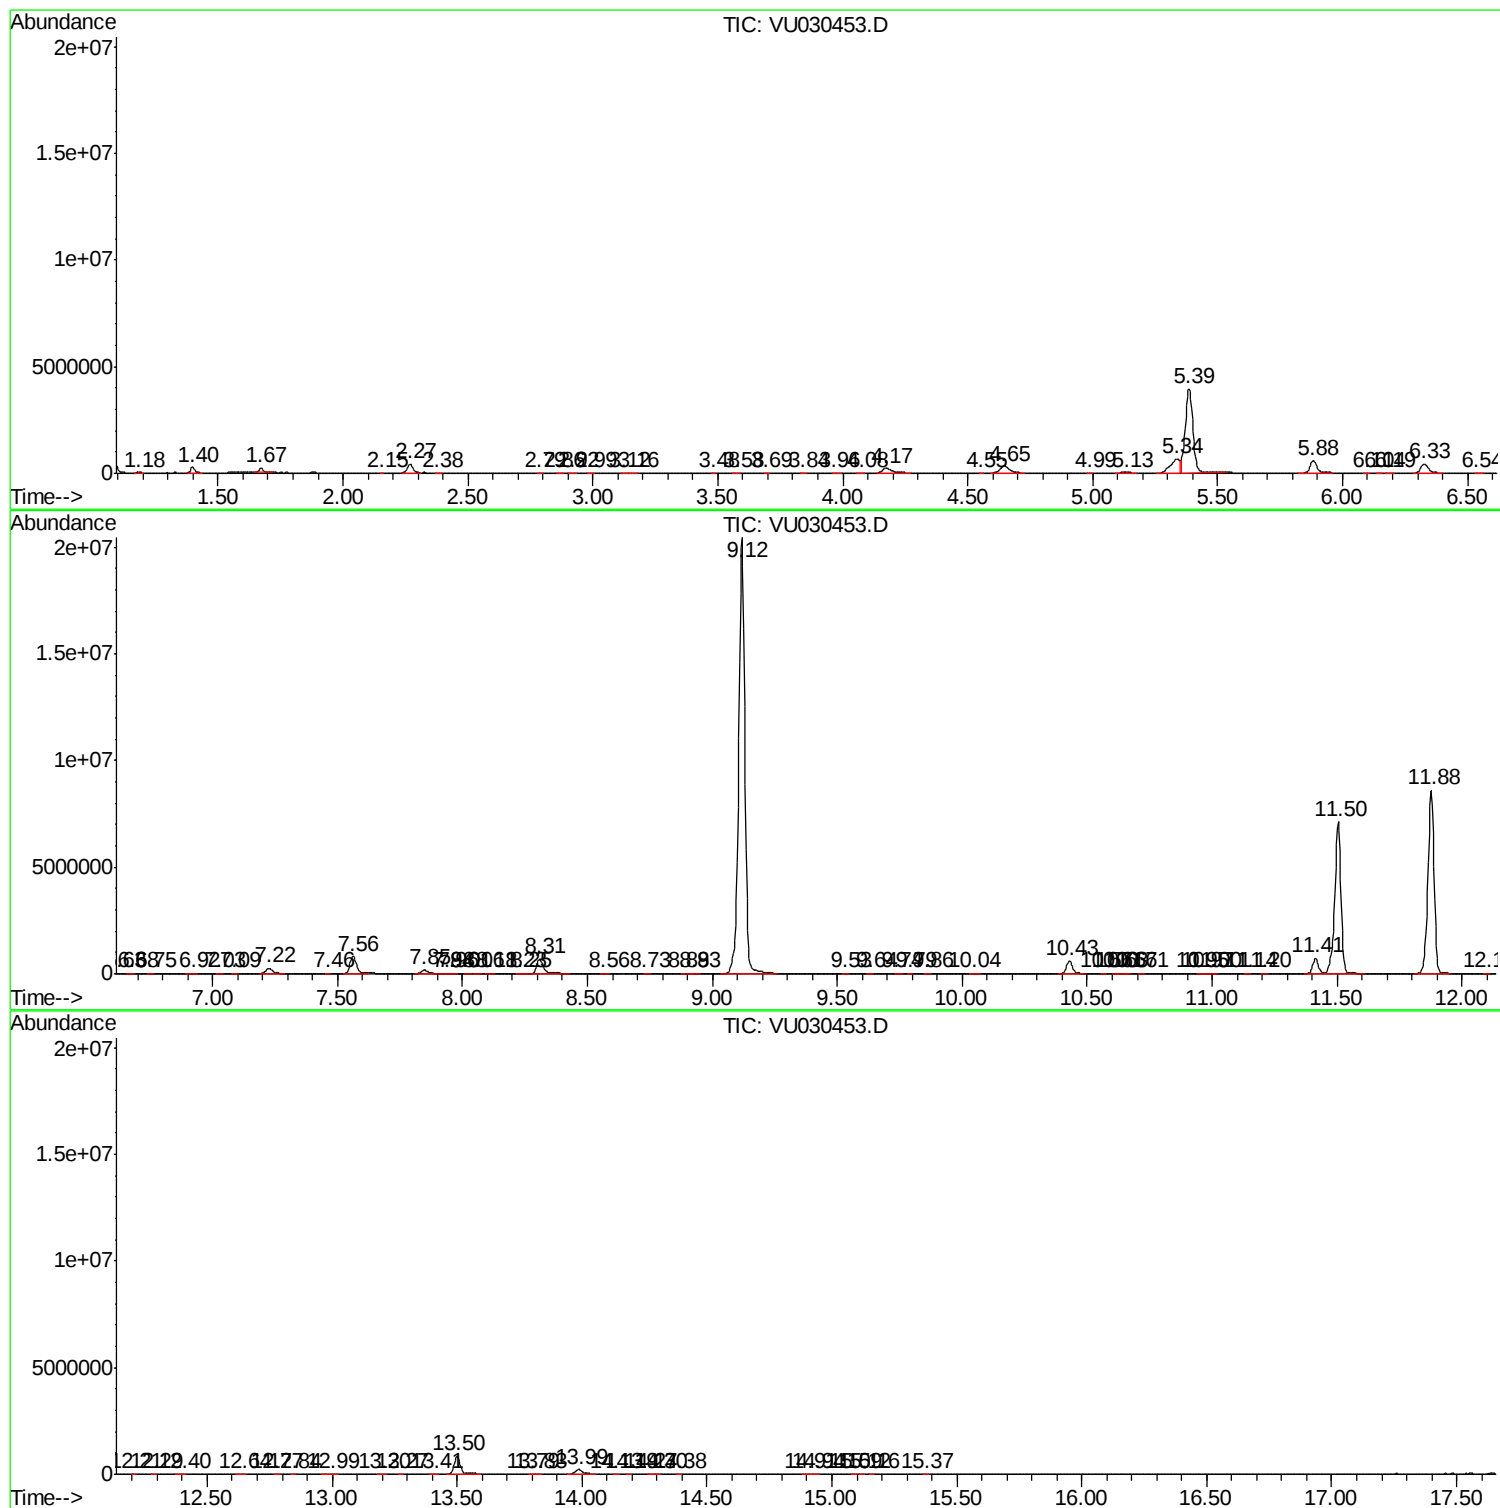

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032619\
Data File : VU030453.D
Acq On : 26 Mar 2019 19:05
Operator : JC/SP
Sample : K2022-15 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C09D9

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032619\
Data File : VU030453.D
Acq On : 26 Mar 2019 19:05
Operator : JC/SP
Sample : K2022-15 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C09D9

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc