

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032619\
 Data File : VU030454.D
 Acq On : 26 Mar 2019 19:29
 Operator : JC/SP
 Sample : K2022-16 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C09E4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.399	89	96	108	rVB	267556	267596	0.46%	0.256%
2	1.672	174	181	196	rVB	206279	258631	0.45%	0.247%
3	2.267	357	366	382	rVB	407025	618240	1.07%	0.591%
4	2.656	484	487	490	rBV	1497	908	0.00%	0.001%
5	2.785	522	527	531	rBV	1850	2243	0.00%	0.002%
6	2.862	549	551	553	rBV	1728	1097	0.00%	0.001%
7	2.913	563	567	571	rBV	1620	1429	0.00%	0.001%
8	3.035	601	605	610	rBV	2102	1884	0.00%	0.002%
9	3.100	622	625	628	rBV	1624	997	0.00%	0.001%
10	3.177	643	649	651	rBV	1306	1396	0.00%	0.001%
11	3.251	667	672	674	rBV	1946	1607	0.00%	0.002%
12	3.293	682	685	687	rBV	1736	1356	0.00%	0.001%
13	3.453	732	735	737	rBV	1327	813	0.00%	0.001%
14	3.646	792	795	799	rBV	2100	1629	0.00%	0.002%
15	3.666	799	801	805	rBV	1315	961	0.00%	0.001%
16	3.878	861	867	872	rBV	1646	2303	0.00%	0.002%
17	4.174	946	959	984	rBV	212737	551926	0.95%	0.528%
18	4.643	1090	1105	1130	rBV	303793	721687	1.24%	0.690%
19	5.080	1237	1241	1245	rBV	1095	1116	0.00%	0.001%
20	5.135	1245	1258	1270	rVV4	6513	14723	0.03%	0.014%
21	5.334	1297	1320	1331	rBV2	630251	1894746	3.27%	1.812%
22	5.746	1446	1448	1452	rVB	1551	1037	0.00%	0.001%
23	5.881	1478	1490	1510	rBV	544095	1090817	1.88%	1.043%
24	6.328	1615	1629	1652	rBV	430129	876823	1.51%	0.839%
25	6.653	1728	1730	1731	rBV	1054	506	0.00%	0.000%
26	6.720	1748	1751	1754	rBV	1559	958	0.00%	0.001%
27	6.820	1775	1782	1785	rBV2	1636	2481	0.00%	0.002%
28	6.900	1805	1807	1810	rVB	1933	944	0.00%	0.001%
29	6.920	1810	1813	1818	rVB	1921	1679	0.00%	0.002%
30	6.955	1818	1824	1827	rBV	1937	2020	0.00%	0.002%
31	7.157	1883	1887	1888	rBV	1215	917	0.00%	0.001%
32	7.225	1896	1908	1923	rBV	239558	430596	0.74%	0.412%
33	7.563	2001	2013	2043	rBV	793320	1427842	2.46%	1.365%
34	7.846	2091	2101	2120	rBV	161917	283421	0.49%	0.271%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032619\
 Data File : VU030454.D
 Acq On : 26 Mar 2019 19:29
 Operator : JC/SP
 Sample : K2022-16 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C09E4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

35	8.173	2200	2203	2209	rBV	1708	1444	0.00%	0.001%
36	8.309	2233	2245	2282	rBV	669597	1214556	2.09%	1.162%
37	8.691	2360	2364	2368	rBV	1602	1716	0.00%	0.002%
38	8.746	2377	2381	2385	rVB2	1322	1222	0.00%	0.001%
39	8.820	2401	2404	2405	rBV	1289	831	0.00%	0.001%
40	8.878	2415	2422	2423	rBV	1169	1368	0.00%	0.001%
41	8.929	2432	2438	2442	rBV	1639	1685	0.00%	0.002%
42	8.955	2442	2446	2449	rBV	1296	1127	0.00%	0.001%
43	9.122	2475	2498	2546	rBV2	34096067	58003123	100.00%	55.470%
44	9.553	2630	2632	2635	rBV2	1562	952	0.00%	0.001%
45	9.617	2649	2652	2653	rBV	925	438	0.00%	0.000%
46	9.665	2659	2667	2668	rBV2	1253	1444	0.00%	0.001%
47	9.726	2683	2686	2688	rBV	1595	975	0.00%	0.001%
48	9.788	2701	2705	2707	rBV2	1806	1531	0.00%	0.001%
49	9.816	2711	2714	2717	rVB	1355	786	0.00%	0.001%
50	9.903	2736	2741	2743	rBV2	1522	1264	0.00%	0.001%
51	9.968	2757	2761	2764	rBV	1644	1435	0.00%	0.001%
52	10.032	2777	2781	2784	rVB	1161	781	0.00%	0.001%
53	10.051	2784	2787	2788	rBV	912	514	0.00%	0.000%
54	10.206	2832	2835	2839	rBV	1321	1252	0.00%	0.001%
55	10.308	2864	2867	2870	rBV	2435	1309	0.00%	0.001%
56	10.328	2870	2873	2876	rVV	1336	1057	0.00%	0.001%
57	10.360	2880	2883	2887	rBV	1314	963	0.00%	0.001%
58	10.427	2891	2904	2928	rBV	584285	960473	1.66%	0.919%
59	10.617	2959	2963	2968	rVB	1349	1205	0.00%	0.001%
60	10.640	2968	2970	2972	rVB	1235	565	0.00%	0.001%
61	10.659	2972	2976	2979	rBV3	2084	1894	0.00%	0.002%
62	10.717	2990	2994	2997	rBV	945	657	0.00%	0.001%
63	10.733	2997	2999	3002	rBV	925	499	0.00%	0.000%
64	10.791	3013	3017	3020	rBV2	1373	1094	0.00%	0.001%
65	10.942	3060	3064	3067	rBV2	1057	1071	0.00%	0.001%
66	11.061	3095	3101	3104	rVB	1816	1639	0.00%	0.002%
67	11.087	3104	3109	3115	rBV	1436	1714	0.00%	0.002%
68	11.164	3129	3133	3137	rBV	1340	1093	0.00%	0.001%
69	11.186	3137	3140	3143	rBV2	1437	927	0.00%	0.001%
70	11.344	3186	3189	3193	rVB2	1180	815	0.00%	0.001%
71	11.411	3198	3210	3222	rVV	1654381	2582877	4.45%	2.470%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032619\
 Data File : VU030454.D
 Acq On : 26 Mar 2019 19:29
 Operator : JC/SP
 Sample : K2022-16 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C09E4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

72	11.505	3222	3239	3267	rVB2	6116129	10626425	18.32%	10.162%
73	11.878	3333	3355	3383	rBV	12920735	21513963	37.09%	20.575%
74	12.707	3607	3613	3616	rBV	1922	2166	0.00%	0.002%
75	12.922	3678	3680	3682	rBV	1083	681	0.00%	0.001%
76	13.061	3720	3723	3728	rBV2	1350	1227	0.00%	0.001%
77	13.112	3736	3739	3742	rVB	2292	1199	0.00%	0.001%
78	13.128	3742	3744	3748	rBV	2139	1612	0.00%	0.002%
79	13.196	3760	3765	3768	rBV	1569	1646	0.00%	0.002%
80	13.254	3780	3783	3785	rBV	1412	832	0.00%	0.001%
81	13.344	3808	3811	3816	rBV	2190	2381	0.00%	0.002%
82	13.498	3848	3859	3893	rBV	562588	972763	1.68%	0.930%
83	13.865	3967	3973	3975	rBV	2034	1910	0.00%	0.002%
84	13.932	3992	3994	3998	rVB	1331	734	0.00%	0.001%
85	13.987	3998	4011	4028	rBV2	84564	167842	0.29%	0.161%
86	14.122	4050	4053	4059	rBV	1852	2148	0.00%	0.002%
87	14.656	4216	4219	4223	rBV	2022	1753	0.00%	0.002%
88	14.858	4279	4282	4284	rBV	1597	899	0.00%	0.001%


Sum of corrected areas: 104565806

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU032619\
Data File : VU030454.D
Acq On : 26 Mar 2019 19:29
Operator : JC/SP
Sample : K2022-16 50X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C09E4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

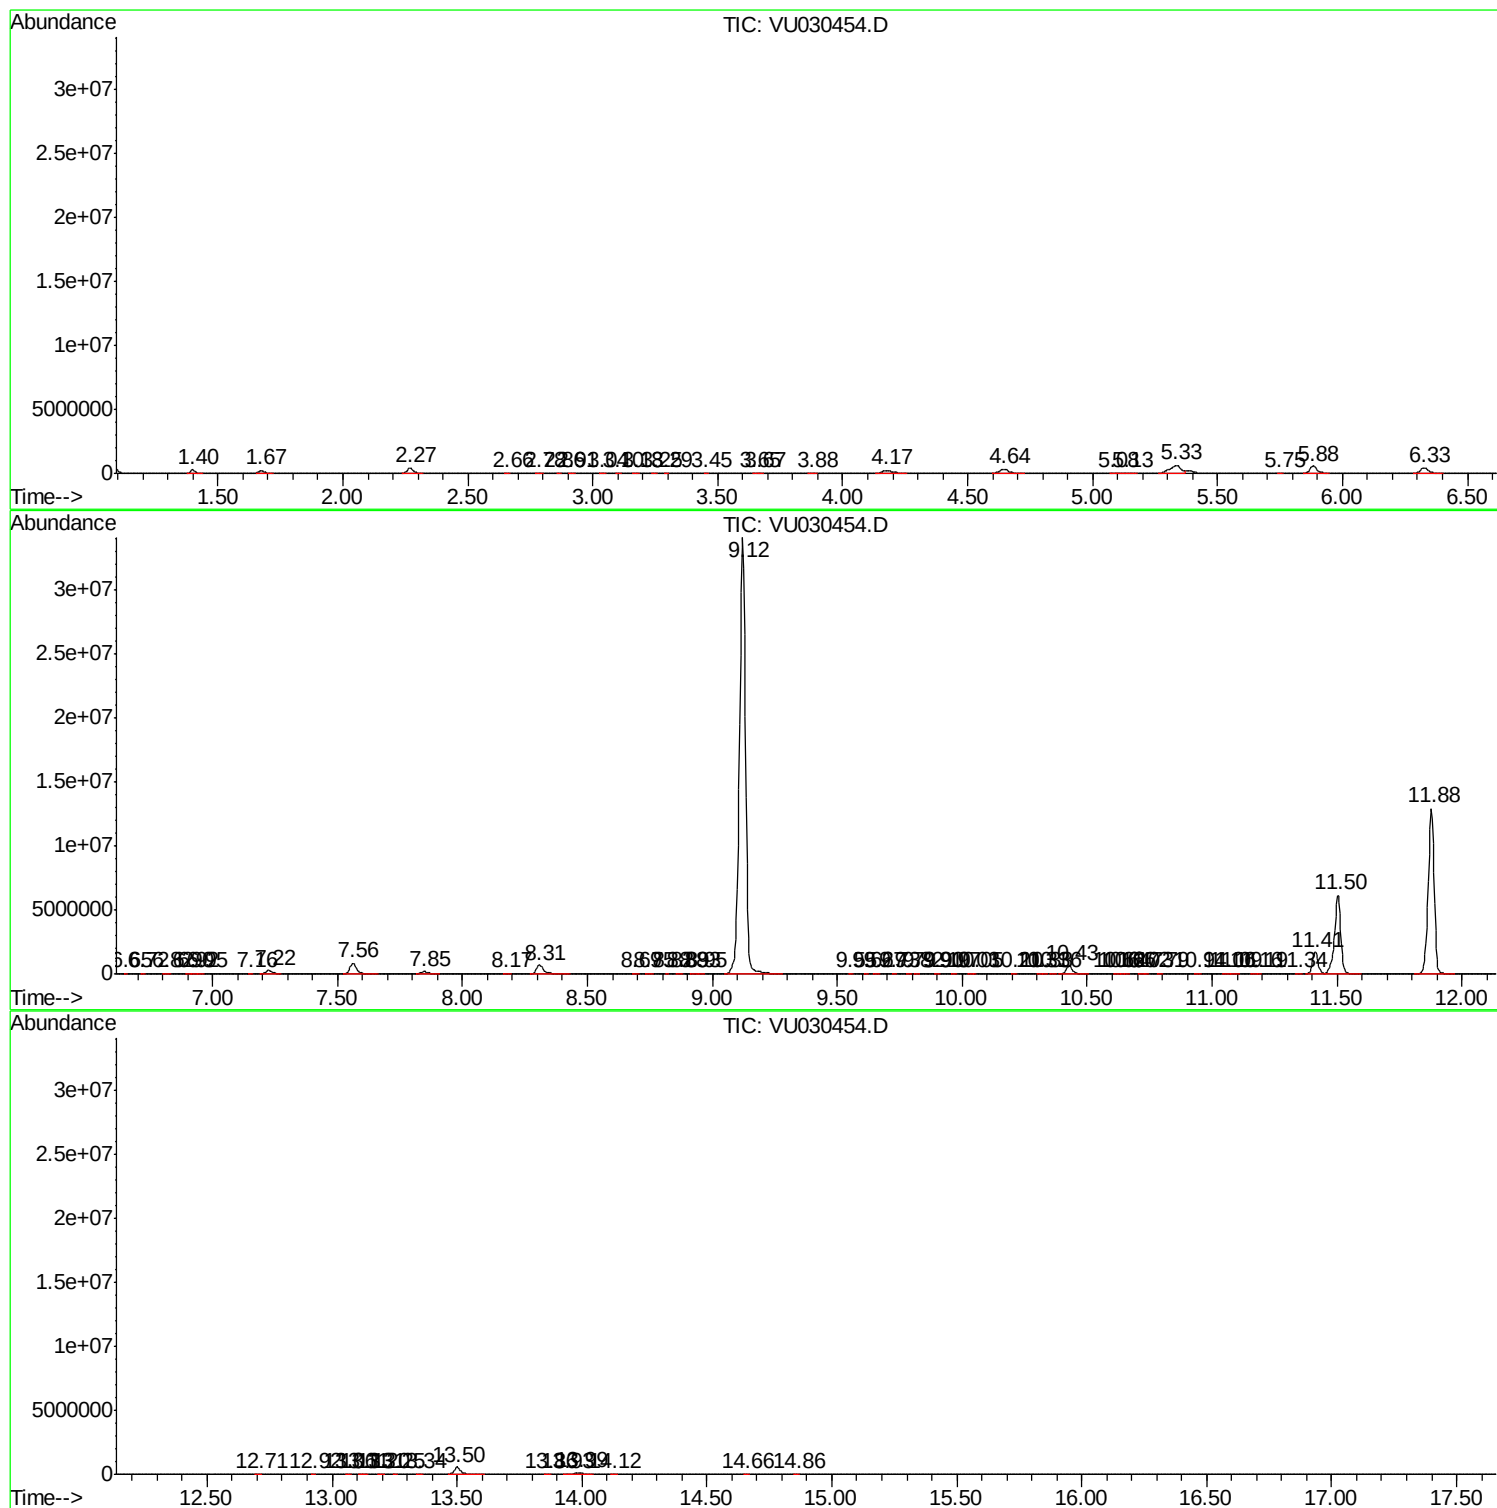

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032619\
Data File : VU030454.D
Acq On : 26 Mar 2019 19:29
Operator : JC/SP
Sample : K2022-16 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C09E4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032619\
Data File : VU030454.D
Acq On : 26 Mar 2019 19:29
Operator : JC/SP
Sample : K2022-16 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C09E4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc