

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032619\
 Data File : VU030455.D
 Acq On : 26 Mar 2019 19:53
 Operator : JC/SP
 Sample : K2022-17 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C09F2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.183	25	29	37	rVB2	13532	13081	0.50%	0.077%
2	1.399	89	96	110	rVB	276444	274531	10.40%	1.616%
3	1.672	173	181	206	rVB	200933	274070	10.38%	1.613%
4	2.270	356	367	379	rBV	413621	633125	23.98%	3.726%
5	2.457	422	425	427	rBV	1623	1146	0.04%	0.007%
6	2.569	457	460	463	rBV	1237	964	0.04%	0.006%
7	2.608	469	472	478	rVB	1426	1267	0.05%	0.007%
8	2.797	527	531	534	rBV	1686	1326	0.05%	0.008%
9	2.887	556	559	564	rVB	1605	1424	0.05%	0.008%
10	2.920	564	569	577	rBV	1863	3122	0.12%	0.018%
11	3.206	655	658	661	rBV	1900	1373	0.05%	0.008%
12	3.424	723	726	731	rVB	1051	1005	0.04%	0.006%
13	3.450	731	734	744	rVB2	878	1205	0.05%	0.007%
14	3.575	770	773	775	rBV2	1691	1240	0.05%	0.007%
15	3.707	812	814	818	rVB	1259	957	0.04%	0.006%
16	3.772	831	834	840	rVB	2828	2494	0.09%	0.015%
17	3.836	851	854	859	rBV	1353	1272	0.05%	0.007%
18	3.862	859	862	866	rBV	1151	980	0.04%	0.006%
19	3.929	881	883	887	rVB	1439	942	0.04%	0.006%
20	4.029	909	914	918	rBV	1343	1334	0.05%	0.008%
21	4.071	923	927	932	rBV	1636	1306	0.05%	0.008%
22	4.174	947	959	994	rBV	214044	562973	21.33%	3.314%
23	4.495	1055	1059	1065	rBV	1564	1583	0.06%	0.009%
24	4.643	1090	1105	1123	rBV	307544	715149	27.09%	4.209%
25	4.923	1189	1192	1197	rBV	1279	1379	0.05%	0.008%
26	5.055	1230	1233	1239	rVB	1890	1906	0.07%	0.011%
27	5.087	1239	1243	1247	rBV	2037	1942	0.07%	0.011%
28	5.119	1247	1253	1256	rVB	1249	1096	0.04%	0.006%
29	5.193	1271	1276	1281	rVB	1894	2136	0.08%	0.013%
30	5.228	1281	1287	1289	rBV	1762	1825	0.07%	0.011%
31	5.337	1295	1321	1357	rBV2	632819	1914321	72.52%	11.267%
32	5.881	1477	1490	1514	rBV	538964	1094593	41.47%	6.443%
33	6.132	1564	1568	1571	rBV	1951	1744	0.07%	0.010%
34	6.328	1609	1629	1653	rBV	434585	890174	33.72%	5.239%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032619\
 Data File : VU030455.D
 Acq On : 26 Mar 2019 19:53
 Operator : JC/SP
 Sample : K2022-17 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C09F2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

35	6.466	1670	1672	1674	rBV	1791	984	0.04%	0.006%
36	6.775	1765	1768	1772	rBV	1399	995	0.04%	0.006%
37	6.833	1783	1786	1790	rBV	1636	1673	0.06%	0.010%
38	6.884	1798	1802	1808	rVB	1370	1256	0.05%	0.007%
39	7.144	1880	1883	1887	rVB	1644	1134	0.04%	0.007%
40	7.170	1887	1891	1893	rBV	1578	1449	0.05%	0.009%
41	7.225	1897	1908	1930	rVV	235651	424309	16.07%	2.497%
42	7.562	2000	2013	2035	rBV	795369	1413473	53.55%	8.319%
43	7.743	2066	2069	2076	rVB	2994	3540	0.13%	0.021%
44	7.781	2076	2081	2084	rBV	1755	2075	0.08%	0.012%
45	7.845	2091	2101	2123	rBV	161107	290192	10.99%	1.708%
46	8.025	2153	2157	2160	rBV	1160	943	0.04%	0.006%
47	8.096	2174	2179	2182	rVV2	1521	1577	0.06%	0.009%
48	8.308	2234	2245	2275	rBV	670506	1219726	46.21%	7.179%
49	8.582	2326	2330	2334	rBV	2016	1719	0.07%	0.010%
50	8.614	2338	2340	2348	rVB2	1941	1926	0.07%	0.011%
51	8.746	2378	2381	2386	rVB	2638	2354	0.09%	0.014%
52	8.771	2386	2389	2396	rBV	2495	3122	0.12%	0.018%
53	9.025	2464	2468	2471	rBV	1305	1050	0.04%	0.006%
54	9.086	2475	2487	2530	rBV2	818044	1983993	75.16%	11.677%
55	9.279	2544	2547	2550	rBV3	1358	1269	0.05%	0.007%
56	9.366	2570	2574	2580	rVV	1987	1368	0.05%	0.008%
57	9.395	2580	2583	2587	rVB	1377	1022	0.04%	0.006%
58	9.456	2596	2602	2605	rVB	1442	1335	0.05%	0.008%
59	9.582	2637	2641	2647	rVB2	1391	1764	0.07%	0.010%
60	9.668	2663	2668	2670	rVB	1235	925	0.04%	0.005%
61	9.768	2696	2699	2702	rVB	1664	1043	0.04%	0.006%
62	9.829	2714	2718	2723	rBV	1354	1416	0.05%	0.008%
63	9.913	2735	2744	2746	rBV2	1472	2159	0.08%	0.013%
64	9.948	2752	2755	2758	rVB	1573	964	0.04%	0.006%
65	10.045	2780	2785	2788	rBV	1193	936	0.04%	0.006%
66	10.193	2825	2831	2834	rVV	1632	1679	0.06%	0.010%
67	10.250	2846	2849	2852	rBV2	1567	1113	0.04%	0.007%
68	10.279	2855	2858	2862	rBV	1750	1406	0.05%	0.008%
69	10.302	2862	2865	2870	rVB	1649	1181	0.04%	0.007%
70	10.337	2871	2876	2879	rBV2	1649	1893	0.07%	0.011%
71	10.427	2887	2904	2926	rBV	594545	963875	36.51%	5.673%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032619\
 Data File : VU030455.D
 Acq On : 26 Mar 2019 19:53
 Operator : JC/SP
 Sample : K2022-17 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C09F2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

72	10.662	2973	2977	2980	rBV	1501	1056	0.04%	0.006%
73	10.681	2980	2983	2987	rBV	1116	1013	0.04%	0.006%
74	10.720	2992	2995	3000	rVV2	1306	1240	0.05%	0.007%
75	10.803	3017	3021	3027	rVB	2077	2112	0.08%	0.012%
76	10.842	3031	3033	3037	rVB	1470	967	0.04%	0.006%
77	10.884	3043	3046	3050	rBV2	1788	1596	0.06%	0.009%
78	10.932	3056	3061	3063	rBV	1458	1290	0.05%	0.008%
79	11.025	3088	3090	3094	rVB	1549	978	0.04%	0.006%
80	11.083	3105	3108	3113	rBV	2222	1824	0.07%	0.011%
81	11.109	3113	3116	3119	rBV	1169	1023	0.04%	0.006%
82	11.215	3146	3149	3154	rVB	1358	1150	0.04%	0.007%
83	11.418	3202	3212	3220	rBV2	32598	54777	2.08%	0.322%
84	11.482	3221	3232	3257	rVB2	690552	1314813	49.81%	7.739%
85	11.668	3287	3290	3292	rBV3	2017	1429	0.05%	0.008%
86	11.710	3300	3303	3306	rBV2	1493	1327	0.05%	0.008%
87	11.871	3334	3353	3381	rBV2	1094345	2639676	100.00%	15.537%
88	12.215	3458	3460	3464	rVB	1499	933	0.04%	0.005%
89	12.340	3496	3499	3504	rBV	1791	1714	0.06%	0.010%
90	12.492	3542	3546	3549	rBV	1201	1278	0.05%	0.008%
91	12.562	3564	3568	3569	rBV	1195	938	0.04%	0.006%
92	12.697	3606	3610	3613	rBV	1470	1344	0.05%	0.008%
93	12.916	3674	3678	3681	rBV3	1941	1737	0.07%	0.010%
94	12.990	3698	3701	3704	rBV	1498	1142	0.04%	0.007%
95	13.504	3849	3861	3876	rBV3	82060	167912	6.36%	0.988%
96	13.993	4005	4013	4022	rBV4	13951	27687	1.05%	0.163%
97	14.196	4073	4076	4078	rBV	2190	1436	0.05%	0.008%
98	14.652	4214	4218	4220	rBV	2277	1808	0.07%	0.011%
99	14.691	4226	4230	4232	rBV	1617	1340	0.05%	0.008%
100	15.569	4500	4503	4512	rVB	2345	2650	0.10%	0.016%


Sum of corrected areas: 16990013

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU032619\
Data File : VU030455.D
Acq On : 26 Mar 2019 19:53
Operator : JC/SP
Sample : K2022-17 50X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C09F2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

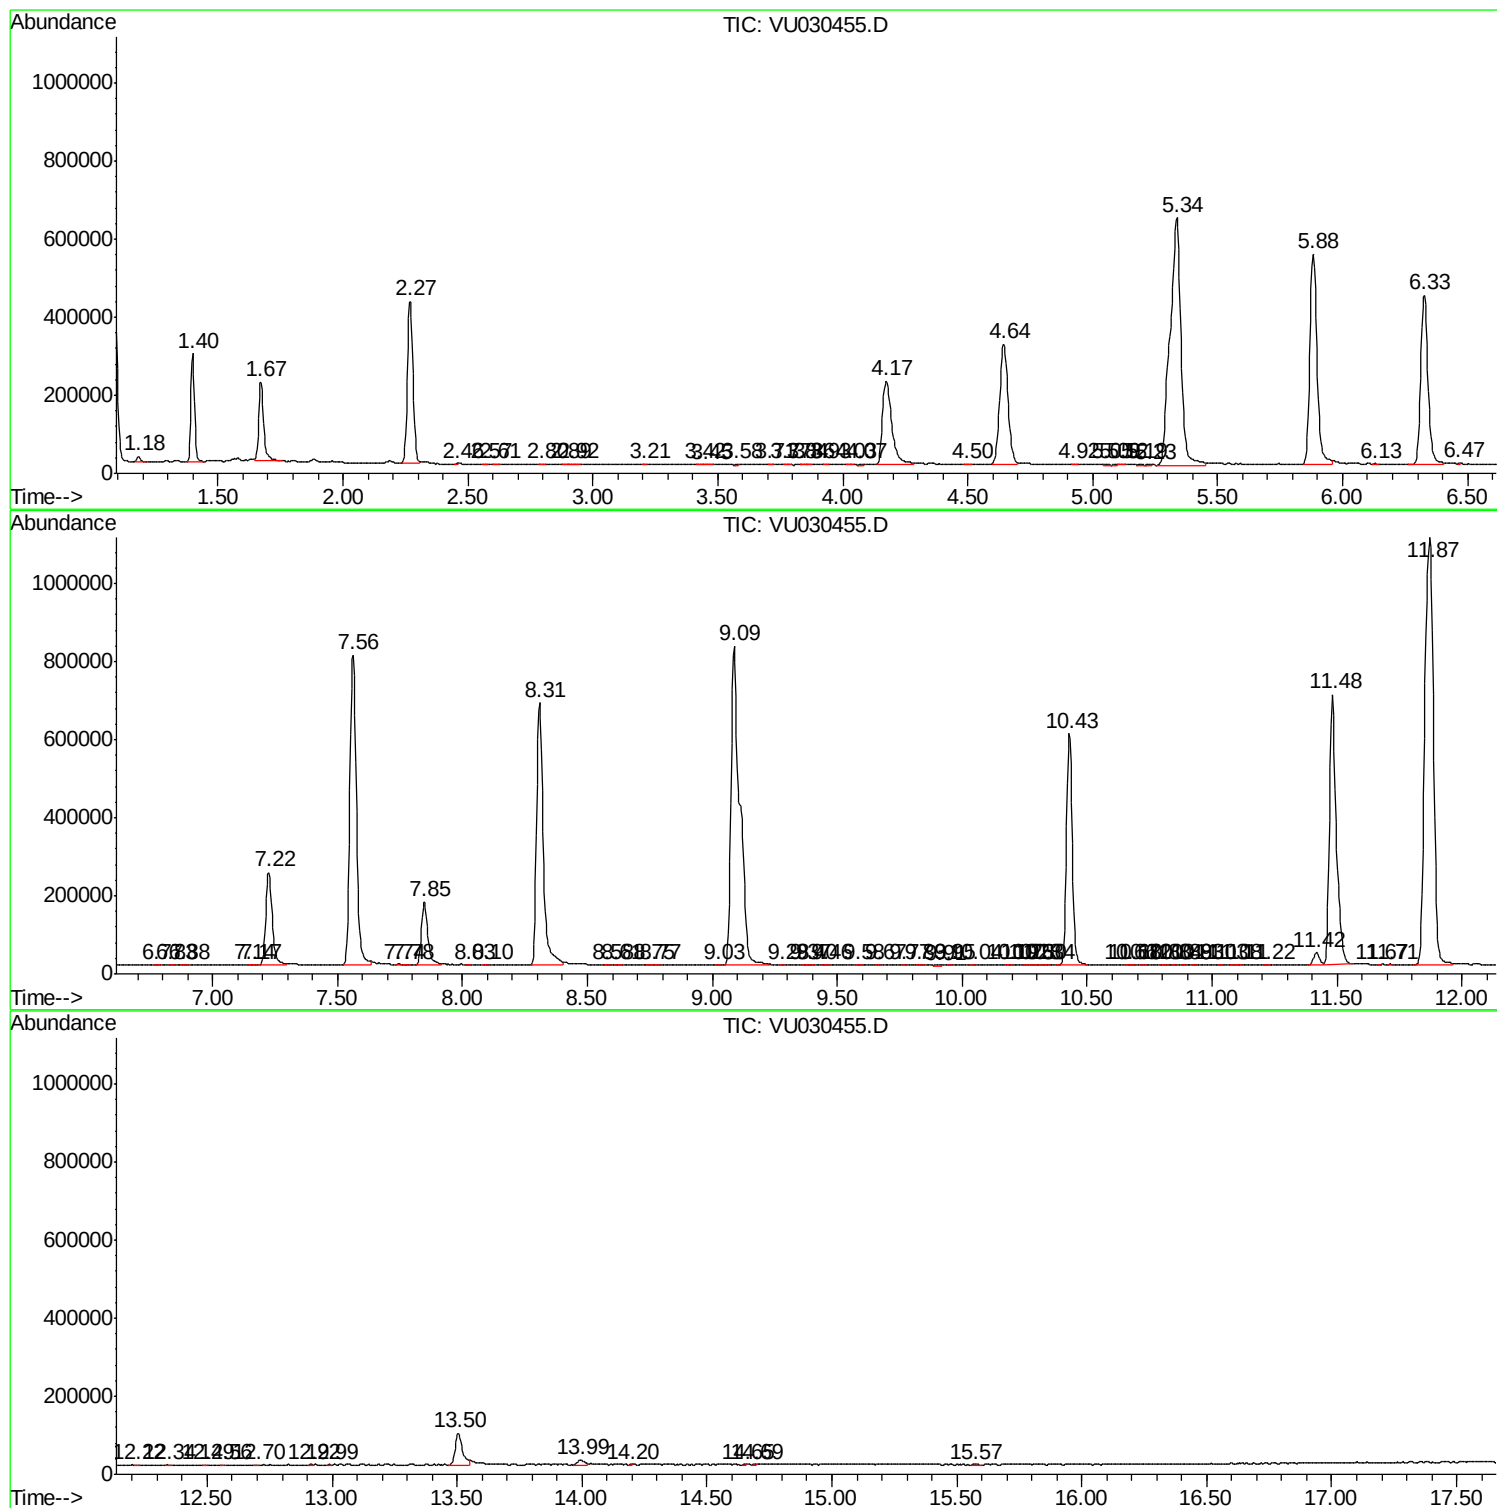

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032619\
Data File : VU030455.D
Acq On : 26 Mar 2019 19:53
Operator : JC/SP
Sample : K2022-17 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C09F2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032619\
Data File : VU030455.D
Acq On : 26 Mar 2019 19:53
Operator : JC/SP
Sample : K2022-17 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C09F2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc