

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032619\
 Data File : VU030457.D
 Acq On : 26 Mar 2019 20:40
 Operator : JC/SP
 Sample : K2022-19 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C09F4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.399	89	96	108	rBV	264656	268876	14.58%	1.916%
2	1.672	174	181	198	rVB	195487	261476	14.18%	1.863%
3	2.270	356	367	380	rBV	401517	611115	33.14%	4.354%
4	2.453	417	424	431	rBV2	4875	7641	0.41%	0.054%
5	2.559	453	457	459	rBV2	656	557	0.03%	0.004%
6	2.675	490	493	496	rBV	1196	940	0.05%	0.007%
7	2.746	512	515	521	rBV	1569	1538	0.08%	0.011%
8	2.775	521	524	526	rBV2	1090	509	0.03%	0.004%
9	2.791	526	529	533	rVB	1034	735	0.04%	0.005%
10	2.820	533	538	543	rBV	1814	2251	0.12%	0.016%
11	2.887	553	559	562	rVB	1672	1509	0.08%	0.011%
12	2.910	562	566	567	rBV2	1343	838	0.05%	0.006%
13	2.955	577	580	582	rBV	821	571	0.03%	0.004%
14	3.029	597	603	607	rBV	1856	1829	0.10%	0.013%
15	3.090	616	622	625	rBV2	1230	1387	0.08%	0.010%
16	3.222	660	663	664	rBV2	671	386	0.02%	0.003%
17	3.231	664	666	669	rVV2	1131	673	0.04%	0.005%
18	3.389	709	715	718	rBV	1944	2075	0.11%	0.015%
19	3.437	726	730	734	rBV	1471	1017	0.06%	0.007%
20	3.473	734	741	743	rBV2	1261	1602	0.09%	0.011%
21	3.498	744	749	752	rVV	2020	1756	0.10%	0.013%
22	3.518	752	755	760	rVB	1587	1520	0.08%	0.011%
23	3.553	760	766	769	rBV	1550	1414	0.08%	0.010%
24	3.878	865	867	869	rBV	1162	715	0.04%	0.005%
25	4.039	914	917	918	rBV	648	332	0.02%	0.002%
26	4.051	918	921	923	rBV	1398	921	0.05%	0.007%
27	4.119	938	942	946	rBV	1646	1756	0.10%	0.013%
28	4.174	947	959	990	rBV	211858	551637	29.91%	3.930%
29	4.643	1091	1105	1123	rBV	297031	694587	37.66%	4.948%
30	4.829	1161	1163	1164	rBV	1752	760	0.04%	0.005%
31	4.955	1199	1202	1204	rBV	1882	1209	0.07%	0.009%
32	5.154	1260	1264	1269	rBV	2071	1963	0.11%	0.014%
33	5.337	1299	1321	1344	rBV2	620585	1844189	100.00%	13.138%
34	5.800	1462	1465	1467	rBV2	1134	670	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032619\
 Data File : VU030457.D
 Acq On : 26 Mar 2019 20:40
 Operator : JC/SP
 Sample : K2022-19 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C09F4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

35	5.884	1478	1491	1524	rBV	533073	1069686	58.00%	7.621%
36	6.151	1570	1574	1579	rBV	1887	2092	0.11%	0.015%
37	6.267	1606	1610	1614	rBV	1566	1319	0.07%	0.009%
38	6.328	1614	1629	1653	rBV	424828	864728	46.89%	6.160%
39	6.559	1698	1701	1704	rBV	1449	1001	0.05%	0.007%
40	6.630	1718	1723	1726	rBV	1721	1556	0.08%	0.011%
41	6.659	1729	1732	1733	rBV	1308	619	0.03%	0.004%
42	6.739	1754	1757	1759	rBV	1827	1214	0.07%	0.009%
43	6.778	1767	1769	1772	rVB	906	473	0.03%	0.003%
44	6.794	1772	1774	1777	rVB	983	479	0.03%	0.003%
45	6.810	1777	1779	1781	rBV	502	266	0.01%	0.002%
46	6.833	1781	1786	1788	rBV	860	841	0.05%	0.006%
47	6.862	1792	1795	1798	rBV	1138	870	0.05%	0.006%
48	6.968	1825	1828	1830	rBV2	959	613	0.03%	0.004%
49	7.013	1835	1842	1846	rBV	1253	1694	0.09%	0.012%
50	7.090	1863	1866	1867	rBV2	671	333	0.02%	0.002%
51	7.138	1877	1881	1883	rBV	1160	756	0.04%	0.005%
52	7.154	1883	1886	1888	rBV	763	404	0.02%	0.003%
53	7.167	1888	1890	1892	rBV	1013	452	0.02%	0.003%
54	7.180	1892	1894	1896	rBV	891	473	0.03%	0.003%
55	7.225	1896	1908	1935	rBV	227429	422379	22.90%	3.009%
56	7.489	1987	1990	1994	rVB	1858	1428	0.08%	0.010%
57	7.514	1994	1998	2000	rBV	1655	1226	0.07%	0.009%
58	7.562	2001	2013	2037	rBV	777284	1380306	74.85%	9.834%
59	7.849	2091	2102	2123	rBV	152374	279598	15.16%	1.992%
60	8.103	2179	2181	2183	rBV	713	425	0.02%	0.003%
61	8.116	2183	2185	2188	rVB	1481	777	0.04%	0.006%
62	8.308	2234	2245	2277	rBV	644181	1187107	64.37%	8.457%
63	8.665	2353	2356	2358	rBV	1589	982	0.05%	0.007%
64	8.810	2397	2401	2402	rBV	1717	1152	0.06%	0.008%
65	8.855	2412	2415	2419	rBV	1445	1014	0.05%	0.007%
66	8.923	2434	2436	2438	rBV	1115	641	0.03%	0.005%
67	9.000	2454	2460	2463	rBV	1898	2433	0.13%	0.017%
68	9.087	2475	2487	2517	rBV	773346	1341372	72.74%	9.556%
69	9.456	2599	2602	2605	rBV	955	569	0.03%	0.004%
70	9.514	2618	2620	2621	rBV2	634	263	0.01%	0.002%
71	9.530	2621	2625	2629	rVV	2048	1676	0.09%	0.012%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032619\
 Data File : VU030457.D
 Acq On : 26 Mar 2019 20:40
 Operator : JC/SP
 Sample : K2022-19 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C09F4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

72	9.649	2660	2662	2664	rBV	1191	541	0.03%	0.004%
73	9.836	2714	2720	2726	rBV	1693	2302	0.12%	0.016%
74	9.874	2730	2732	2735	rBV	1039	774	0.04%	0.006%
75	9.916	2741	2745	2748	rBV	1719	1609	0.09%	0.011%
76	10.025	2774	2779	2782	rBV2	1168	1065	0.06%	0.008%
77	10.048	2782	2786	2791	rBV2	1241	1523	0.08%	0.011%
78	10.228	2835	2842	2844	rBV2	1486	1574	0.09%	0.011%
79	10.427	2891	2904	2926	rBV	578997	949870	51.51%	6.767%
80	10.556	2939	2944	2946	rBV	1453	1573	0.09%	0.011%
81	11.228	3148	3153	3159	rBV2	2730	3205	0.17%	0.023%
82	11.279	3166	3169	3172	rBV	1818	1255	0.07%	0.009%
83	11.482	3220	3232	3257	rBV	640049	1075562	58.32%	7.663%
84	11.726	3305	3308	3312	rBV	2404	1843	0.10%	0.013%
85	11.858	3337	3349	3372	rBV	662501	1146265	62.16%	8.166%
86	13.212	3768	3770	3773	rBV	1277	723	0.04%	0.005%
87	13.344	3808	3811	3813	rBV2	1457	997	0.05%	0.007%
88	14.164	4062	4066	4068	rBV2	2157	1805	0.10%	0.013%


Sum of corrected areas: 14036657

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU032619\
Data File : VU030457.D
Acq On : 26 Mar 2019 20:40
Operator : JC/SP
Sample : K2022-19 50X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C09F4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

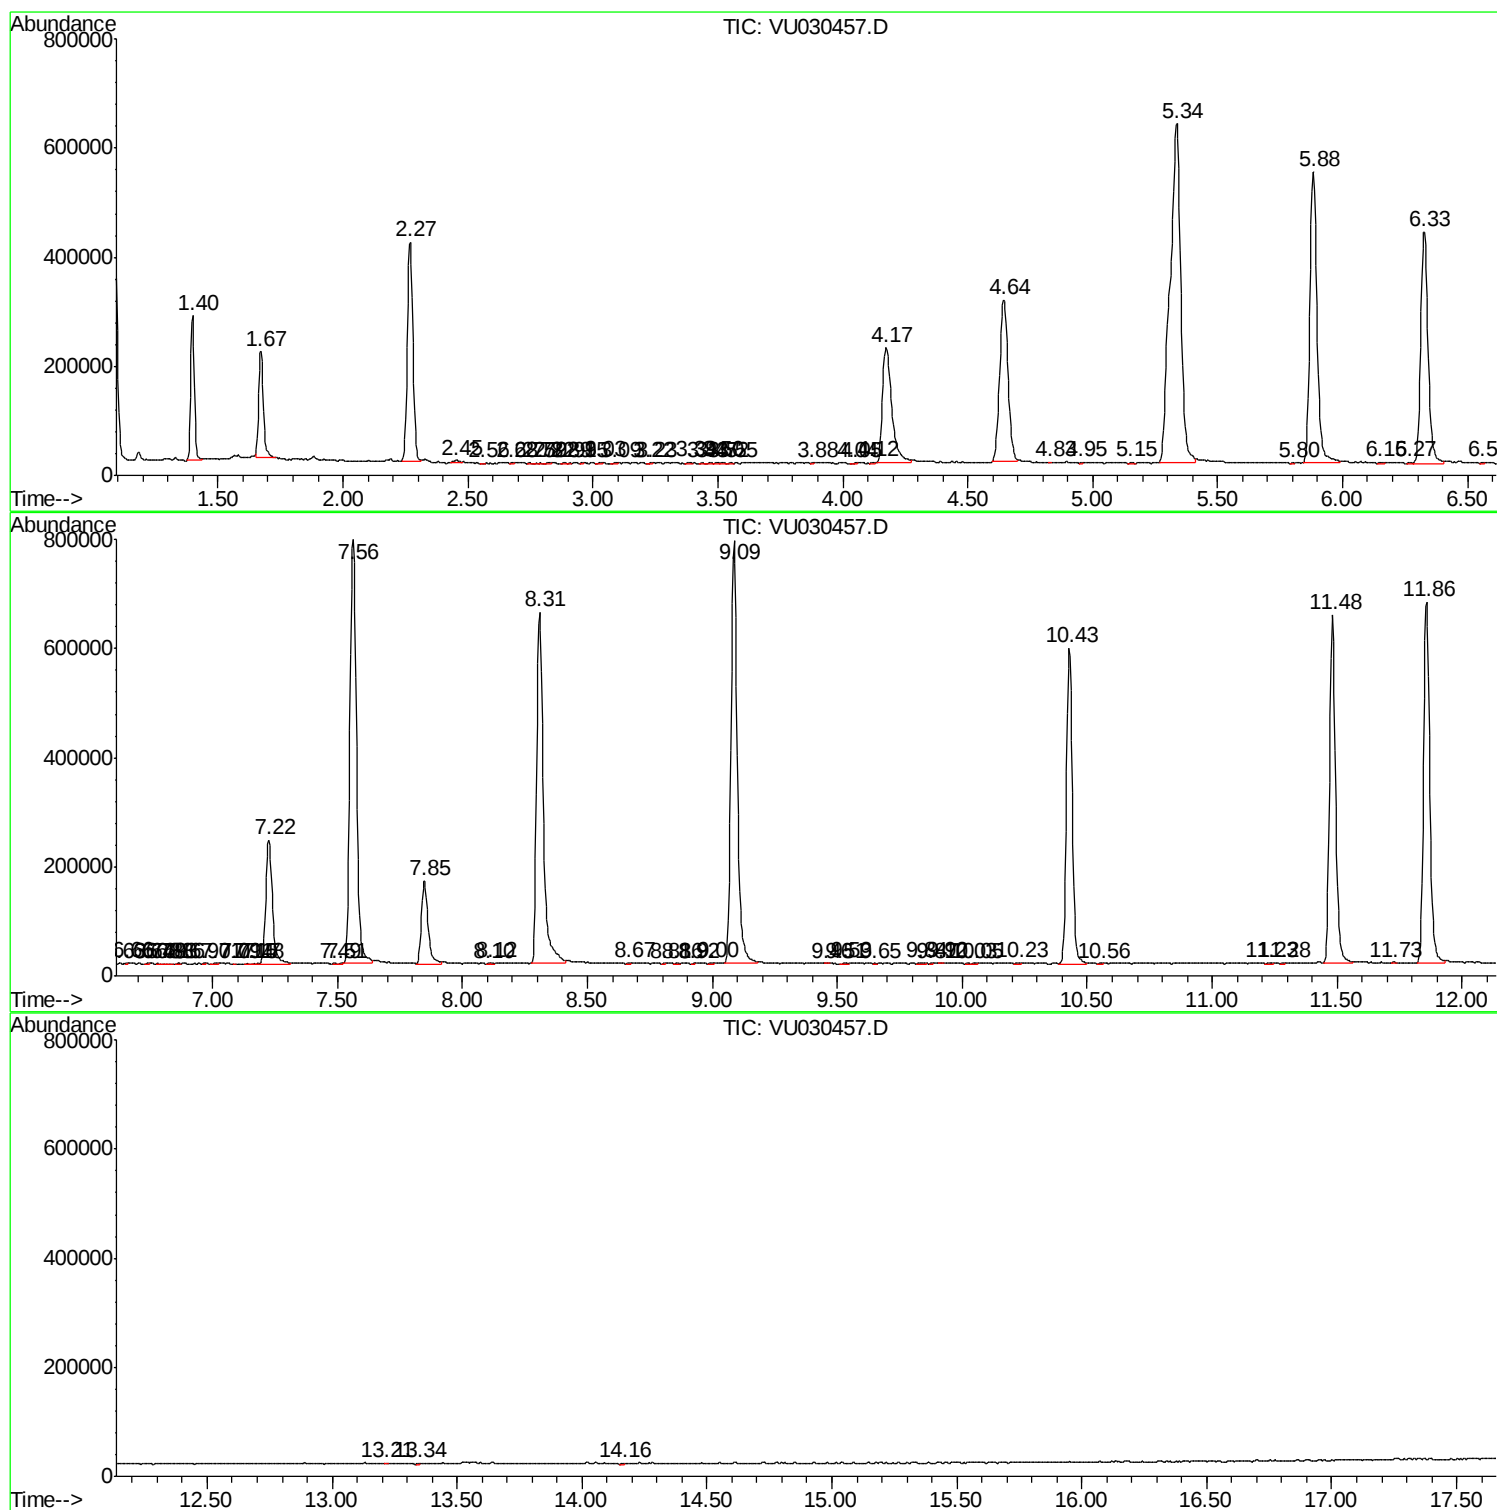

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032619\
Data File : VU030457.D
Acq On : 26 Mar 2019 20:40
Operator : JC/SP
Sample : K2022-19 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C09F4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU032619\
Data File : VU030457.D
Acq On : 26 Mar 2019 20:40
Operator : JC/SP
Sample : K2022-19 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C09F4

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc