

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032619\
 Data File : VU030466.D
 Acq On : 27 Mar 2019 00:12
 Operator : JC/SP
 Sample : K2063-13 100X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB6S0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	24	28	35	rVB2	14534	14147	0.73%	0.096%
2	1.399	89	96	106	rBV	285611	282308	14.64%	1.925%
3	1.665	171	179	198	rVB	219282	280750	14.55%	1.915%
4	2.267	355	366	380	rBV	425703	647853	33.59%	4.418%
5	2.534	446	449	453	rVB	2128	1381	0.07%	0.009%
6	2.563	453	458	463	rBV	1861	2105	0.11%	0.014%
7	2.694	493	499	502	rBV3	2380	2669	0.14%	0.018%
8	2.990	586	591	594	rBV2	1759	1760	0.09%	0.012%
9	3.048	603	609	613	rBV	1381	1876	0.10%	0.013%
10	3.090	619	622	628	rVB2	1159	1317	0.07%	0.009%
11	3.170	643	647	653	rVB2	1217	1661	0.09%	0.011%
12	3.424	723	726	729	rBV	1593	1133	0.06%	0.008%
13	3.569	769	771	778	rVB	2396	2338	0.12%	0.016%
14	3.608	778	783	788	rBV	2594	3777	0.20%	0.026%
15	3.778	833	836	841	rVV	1569	1397	0.07%	0.010%
16	3.823	846	850	852	rBV	1557	1101	0.06%	0.008%
17	3.874	860	866	869	rBV	1913	2039	0.11%	0.014%
18	3.964	890	894	900	rVB	2024	2229	0.12%	0.015%
19	4.009	900	908	911	rBV	1937	2817	0.15%	0.019%
20	4.096	932	935	938	rVB	1852	1251	0.06%	0.009%
21	4.116	938	941	944	rBV	2685	2167	0.11%	0.015%
22	4.173	947	959	991	rVV	215524	570084	29.55%	3.888%
23	4.476	1050	1053	1058	rVB	1817	1394	0.07%	0.010%
24	4.501	1058	1061	1064	rVB	1917	1089	0.06%	0.007%
25	4.521	1064	1067	1071	rBV	1374	1122	0.06%	0.008%
26	4.553	1071	1077	1082	rBV2	1261	1748	0.09%	0.012%
27	4.643	1089	1105	1125	rBV	309393	726639	37.67%	4.956%
28	4.935	1193	1196	1199	rBV	1852	1288	0.07%	0.009%
29	4.955	1199	1202	1206	rVV	1496	1242	0.06%	0.008%
30	5.334	1298	1320	1352	rVV2	643260	1928961	100.00%	13.155%
31	5.511	1372	1375	1378	rVB	2410	1496	0.08%	0.010%
32	5.669	1421	1424	1427	rVB	2064	1415	0.07%	0.010%
33	5.697	1427	1433	1434	rBV	1562	1364	0.07%	0.009%
34	5.714	1435	1438	1447	rVB	1438	2007	0.10%	0.014%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032619\
 Data File : VU030466.D
 Acq On : 27 Mar 2019 00:12
 Operator : JC/SP
 Sample : K2063-13 100X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB6S0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

35	5.807	1464	1467	1470	rBV	1319	1079	0.06%	0.007%
36	5.881	1478	1490	1519	rBV	556510	1112384	57.67%	7.586%
37	6.096	1554	1557	1564	rVB	1942	2237	0.12%	0.015%
38	6.324	1615	1628	1663	rBV	439214	895313	46.41%	6.106%
39	6.453	1665	1668	1671	rBV3	1940	1713	0.09%	0.012%
40	6.530	1689	1692	1697	rVB2	1538	1267	0.07%	0.009%
41	6.556	1697	1700	1706	rBV	1253	1200	0.06%	0.008%
42	6.784	1766	1771	1777	rVV	914	1246	0.06%	0.008%
43	6.836	1783	1787	1791	rVV	1861	1583	0.08%	0.011%
44	6.926	1812	1815	1819	rVB	2051	1489	0.08%	0.010%
45	7.167	1887	1890	1893	rVB	2284	1480	0.08%	0.010%
46	7.225	1893	1908	1933	rBV	235411	441588	22.89%	3.012%
47	7.495	1986	1992	1995	rBV2	1382	1643	0.09%	0.011%
48	7.562	2000	2013	2030	rBV	821334	1444051	74.86%	9.848%
49	7.803	2085	2088	2091	rBV	1683	1104	0.06%	0.008%
50	7.845	2091	2101	2122	rBV2	162562	286576	14.86%	1.954%
51	7.990	2144	2146	2150	rVB	2100	1396	0.07%	0.010%
52	8.012	2150	2153	2159	rBV2	1824	1915	0.10%	0.013%
53	8.064	2164	2169	2177	rVB	1596	2391	0.12%	0.016%
54	8.099	2177	2180	2185	rBV2	1178	1258	0.07%	0.009%
55	8.128	2185	2189	2192	rBV	1135	1118	0.06%	0.008%
56	8.308	2232	2245	2279	rBV	682746	1244372	64.51%	8.486%
57	8.611	2334	2339	2341	rBV	2203	1811	0.09%	0.012%
58	8.762	2381	2386	2387	rBV	2367	2056	0.11%	0.014%
59	8.932	2437	2439	2447	rVB2	1707	1502	0.08%	0.010%
60	9.086	2473	2487	2519	rBV	801123	1370056	71.03%	9.343%
61	9.379	2569	2578	2590	rVB3	10020	18502	0.96%	0.126%
62	9.450	2593	2600	2604	rBV3	1650	1824	0.09%	0.012%
63	9.781	2694	2703	2713	rBV3	4813	8597	0.45%	0.059%
64	9.852	2721	2725	2730	rBV	2034	2047	0.11%	0.014%
65	9.893	2731	2738	2744	rVV	2378	3303	0.17%	0.023%
66	10.122	2804	2809	2815	rVV	2266	2779	0.14%	0.019%
67	10.164	2819	2822	2828	rVV	1482	1290	0.07%	0.009%
68	10.209	2833	2836	2839	rVB	1887	1086	0.06%	0.007%
69	10.324	2868	2872	2875	rBV2	1634	1443	0.07%	0.010%
70	10.427	2887	2904	2925	rBV	600384	974680	50.53%	6.647%
71	10.762	3005	3008	3013	rVB	1711	1493	0.08%	0.010%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032619\
 Data File : VU030466.D
 Acq On : 27 Mar 2019 00:12
 Operator : JC/SP
 Sample : K2063-13 100X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB6S0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

72	11.147	3122	3128	3137	rVB4	5009	7484	0.39%	0.051%
73	11.299	3168	3175	3177	rVV2	1134	1402	0.07%	0.010%
74	11.315	3177	3180	3182	rVV	1535	1124	0.06%	0.008%
75	11.347	3186	3190	3194	rBV	1764	1415	0.07%	0.010%
76	11.405	3203	3208	3214	rVB	2189	2311	0.12%	0.016%
77	11.482	3220	3232	3251	rBV	672028	1110405	57.56%	7.573%
78	11.665	3287	3289	3295	rVB	1947	1212	0.06%	0.008%
79	11.858	3336	3349	3368	rBV	694612	1165304	60.41%	7.947%
80	12.115	3427	3429	3434	rVB2	1528	1162	0.06%	0.008%
81	12.308	3484	3489	3493	rBV2	1378	1373	0.07%	0.009%
82	12.459	3532	3536	3540	rBV	1324	1683	0.09%	0.011%
83	12.572	3568	3571	3574	rBV	1315	1087	0.06%	0.007%
84	12.823	3645	3649	3654	rBV	2416	2527	0.13%	0.017%
85	12.913	3674	3677	3683	rBV2	1503	1588	0.08%	0.011%
86	13.006	3702	3706	3711	rBV2	1371	1428	0.07%	0.010%
87	13.089	3729	3732	3737	rVB	1537	1186	0.06%	0.008%
88	13.337	3805	3809	3811	rBV	1699	1216	0.06%	0.008%
89	13.392	3823	3826	3829	rBV	1564	1268	0.07%	0.009%
90	13.411	3830	3832	3836	rVB	1950	1163	0.06%	0.008%
91	13.433	3836	3839	3844	rBV	1899	1745	0.09%	0.012%
92	13.549	3870	3875	3878	rBV2	2165	2142	0.11%	0.015%
93	13.935	3989	3995	3998	rBV	2382	3013	0.16%	0.021%
94	14.183	4069	4072	4075	rBV	1673	1130	0.06%	0.008%
95	14.208	4076	4080	4084	rVB	1918	1937	0.10%	0.013%
96	14.388	4133	4136	4138	rBV	1933	1182	0.06%	0.008%
97	14.639	4211	4214	4219	rBV	1393	1427	0.07%	0.010%
98	15.112	4358	4361	4363	rBV	1464	1097	0.06%	0.007%
99	15.822	4577	4582	4583	rBV3	1988	1736	0.09%	0.012%
100	16.408	4759	4764	4766	rBV2	2699	2701	0.14%	0.018%


Sum of corrected areas: 14663245

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU032619\
Data File : VU030466.D
Acq On : 27 Mar 2019 00:12
Operator : JC/SP
Sample : K2063-13 100X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampled :
DB6S0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

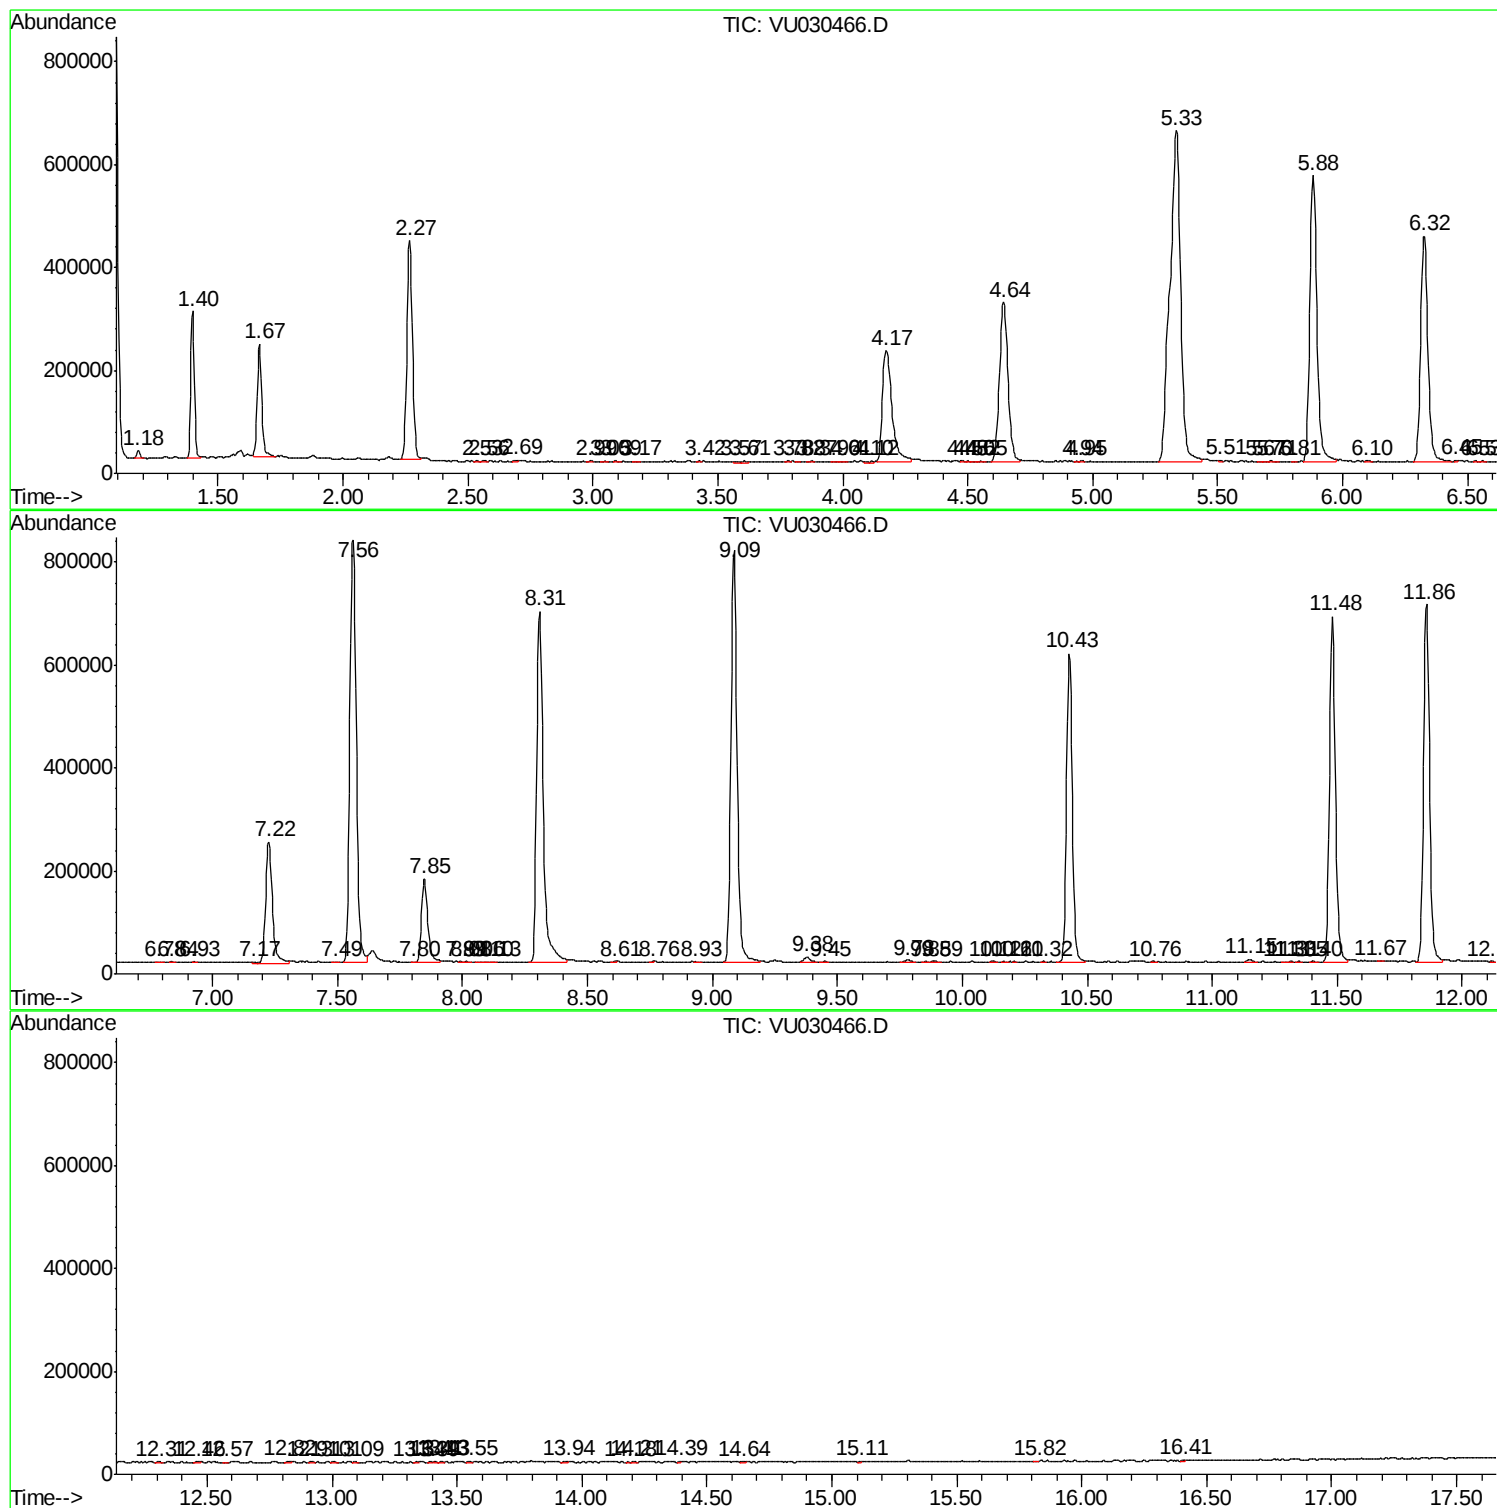

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032619\
Data File : VU030466.D
Acq On : 27 Mar 2019 00:12
Operator : JC/SP
Sample : K2063-13 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB6S0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU032619\
Data File : VU030466.D
Acq On : 27 Mar 2019 00:12
Operator : JC/SP
Sample : K2063-13 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB6S0

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc