

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032619\
 Data File : VU030467.D
 Acq On : 27 Mar 2019 00:36
 Operator : JC/SP
 Sample : K2063-14 100X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB6S1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.183	24	29	34	rBV	15544	13961	0.71%	0.095%
2	1.399	89	96	111	rVB	284962	285175	14.55%	1.950%
3	1.669	173	180	197	rVB	205276	271478	13.85%	1.857%
4	2.267	356	366	380	rBV	425951	640192	32.66%	4.378%
5	2.566	453	459	464	rBV	1710	2197	0.11%	0.015%
6	2.598	466	469	473	rVB	1761	1178	0.06%	0.008%
7	2.701	492	501	506	rBV4	4652	7272	0.37%	0.050%
8	2.987	586	590	592	rBV2	1982	1651	0.08%	0.011%
9	3.344	697	701	704	rBV2	1414	1256	0.06%	0.009%
10	3.376	709	711	718	rVB2	1713	1605	0.08%	0.011%
11	3.469	735	740	743	rBV	1637	1789	0.09%	0.012%
12	3.524	751	757	763	rBV	2317	3243	0.17%	0.022%
13	3.576	767	773	777	rBV2	1723	1894	0.10%	0.013%
14	3.630	785	790	794	rBV	1555	2037	0.10%	0.014%
15	3.788	836	839	844	rVB	1832	1504	0.08%	0.010%
16	3.813	844	847	855	rBV	1822	2349	0.12%	0.016%
17	3.945	881	888	892	rBV	1073	1618	0.08%	0.011%
18	4.093	925	934	943	rBV5	3757	6455	0.33%	0.044%
19	4.174	947	959	990	rBV	207871	558566	28.49%	3.820%
20	4.643	1090	1105	1135	rVB2	306330	730771	37.28%	4.998%
21	4.788	1146	1150	1153	rBV	1688	1527	0.08%	0.010%
22	4.990	1210	1213	1218	rVB3	1690	1458	0.07%	0.010%
23	5.193	1273	1276	1279	rBV	1571	1293	0.07%	0.009%
24	5.334	1297	1320	1357	rBV2	635241	1960397	100.00%	13.408%
25	5.881	1477	1490	1515	rBV	546272	1096248	55.92%	7.498%
26	6.180	1578	1583	1584	rBV	2242	1987	0.10%	0.014%
27	6.228	1593	1598	1604	rVB	2225	2175	0.11%	0.015%
28	6.328	1615	1629	1652	rBV	431928	884010	45.09%	6.046%
29	6.434	1660	1662	1668	rVV	1993	1681	0.09%	0.011%
30	6.463	1668	1671	1678	rVB3	2686	3102	0.16%	0.021%
31	6.588	1706	1710	1715	rVB	1595	1488	0.08%	0.010%
32	6.675	1734	1737	1742	rBV	1366	1258	0.06%	0.009%
33	6.820	1776	1782	1784	rBV	1167	1255	0.06%	0.009%
34	6.903	1801	1808	1814	rBV2	1143	1479	0.08%	0.010%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032619\
 Data File : VU030467.D
 Acq On : 27 Mar 2019 00:36
 Operator : JC/SP
 Sample : K2063-14 100X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB6S1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

35	7.016	1834	1843	1845	rBV	1392	1841	0.09%	0.013%
36	7.161	1883	1888	1891	rBV	1353	1405	0.07%	0.010%
37	7.225	1896	1908	1933	rVV	233175	429782	21.92%	2.939%
38	7.563	1998	2013	2028	rVV	808788	1414289	72.14%	9.673%
39	7.636	2029	2036	2055	rVB	51780	103803	5.29%	0.710%
40	7.794	2082	2085	2091	rBV	1274	1150	0.06%	0.008%
41	7.845	2091	2101	2118	rBV	160608	285391	14.56%	1.952%
42	7.955	2131	2135	2137	rBV2	1745	1442	0.07%	0.010%
43	8.087	2172	2176	2181	rVB	2024	1659	0.08%	0.011%
44	8.167	2197	2201	2205	rVB3	1943	1398	0.07%	0.010%
45	8.212	2210	2215	2219	rBV	1486	1563	0.08%	0.011%
46	8.251	2223	2227	2232	rVB	1284	1176	0.06%	0.008%
47	8.308	2232	2245	2281	rBV	661094	1214717	61.96%	8.308%
48	8.505	2303	2306	2309	rVB	1970	1270	0.06%	0.009%
49	8.968	2444	2450	2452	rBV2	1090	1269	0.06%	0.009%
50	9.087	2474	2487	2517	rBV	789751	1341719	68.44%	9.176%
51	9.254	2532	2539	2544	rBV4	8494	11507	0.59%	0.079%
52	9.376	2566	2577	2590	rVB3	21804	39385	2.01%	0.269%
53	9.527	2619	2624	2627	rVB	1431	1214	0.06%	0.008%
54	9.550	2627	2631	2635	rBV	1942	1703	0.09%	0.012%
55	9.640	2656	2659	2665	rVB	1672	1906	0.10%	0.013%
56	9.781	2695	2703	2717	rVB2	10835	20399	1.04%	0.140%
57	9.974	2758	2763	2766	rBV	1671	1451	0.07%	0.010%
58	10.151	2814	2818	2822	rBV2	1107	1288	0.07%	0.009%
59	10.231	2840	2843	2847	rVB	1863	1363	0.07%	0.009%
60	10.260	2847	2852	2858	rBV	2385	2641	0.13%	0.018%
61	10.315	2867	2869	2874	rVB2	1605	1225	0.06%	0.008%
62	10.376	2884	2888	2890	rBV	2131	1658	0.08%	0.011%
63	10.427	2893	2904	2923	rVV	585776	950951	48.51%	6.504%
64	10.611	2957	2961	2965	rBV	1346	1451	0.07%	0.010%
65	10.659	2972	2976	2978	rBV2	1418	1185	0.06%	0.008%
66	10.678	2979	2982	2984	rVV3	2109	1359	0.07%	0.009%
67	10.691	2984	2986	2990	rVB	2159	1456	0.07%	0.010%
68	10.765	3001	3009	3011	rBV3	1856	2483	0.13%	0.017%
69	10.826	3021	3028	3031	rBV	2101	2383	0.12%	0.016%
70	10.884	3043	3046	3048	rBV	1666	1253	0.06%	0.009%
71	10.977	3065	3075	3079	rBV2	2867	4136	0.21%	0.028%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032619\
 Data File : VU030467.D
 Acq On : 27 Mar 2019 00:36
 Operator : JC/SP
 Sample : K2063-14 100X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DB6S1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

72	11.074	3102	3105	3110	rBV	1637	1381	0.07%	0.009%
73	11.144	3120	3127	3133	rBV4	3535	5749	0.29%	0.039%
74	11.427	3211	3215	3220	rBV	1766	1644	0.08%	0.011%
75	11.479	3220	3231	3255	rBV	659065	1078406	55.01%	7.376%
76	11.855	3335	3348	3372	rBV	678178	1139950	58.15%	7.796%
77	12.218	3457	3461	3465	rBV3	1554	1615	0.08%	0.011%
78	12.347	3497	3501	3505	rBV	1927	1886	0.10%	0.013%
79	12.437	3522	3529	3532	rBV2	1313	1768	0.09%	0.012%
80	12.514	3550	3553	3558	rBV2	1432	1468	0.07%	0.010%
81	12.639	3587	3592	3595	rBV	1755	1771	0.09%	0.012%
82	12.778	3631	3635	3641	rVB2	1683	1658	0.08%	0.011%
83	12.848	3650	3657	3660	rBV2	2121	2512	0.13%	0.017%
84	13.009	3705	3707	3711	rVB	1904	1167	0.06%	0.008%
85	13.045	3711	3718	3723	rBV2	1753	2490	0.13%	0.017%
86	13.263	3783	3786	3791	rVB	1788	1501	0.08%	0.010%
87	13.302	3791	3798	3803	rVB2	1816	2420	0.12%	0.017%
88	13.395	3822	3827	3831	rBV	1466	1618	0.08%	0.011%
89	13.707	3920	3924	3930	rBV	1773	1907	0.10%	0.013%
90	13.938	3992	3996	3999	rVB	1670	1234	0.06%	0.008%
91	14.028	4017	4024	4026	rBV2	1843	1804	0.09%	0.012%
92	14.090	4040	4043	4045	rBV	2114	1528	0.08%	0.010%
93	14.122	4050	4053	4056	rVV	1734	1281	0.07%	0.009%
94	14.173	4060	4069	4072	rBV	2403	3042	0.16%	0.021%
95	14.215	4079	4082	4087	rBV	1345	1233	0.06%	0.008%
96	14.392	4133	4137	4141	rBV2	1655	1801	0.09%	0.012%
97	14.848	4276	4279	4281	rBV3	1558	1149	0.06%	0.008%
98	15.138	4366	4369	4375	rBV2	1620	1613	0.08%	0.011%
99	15.463	4467	4470	4473	rBV	1792	1719	0.09%	0.012%
100	16.154	4682	4685	4691	rBV2	2109	2194	0.11%	0.015%


Sum of corrected areas: 14621329

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU032619\
Data File : VU030467.D
Acq On : 27 Mar 2019 00:36
Operator : JC/SP
Sample : K2063-14 100X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB6S1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

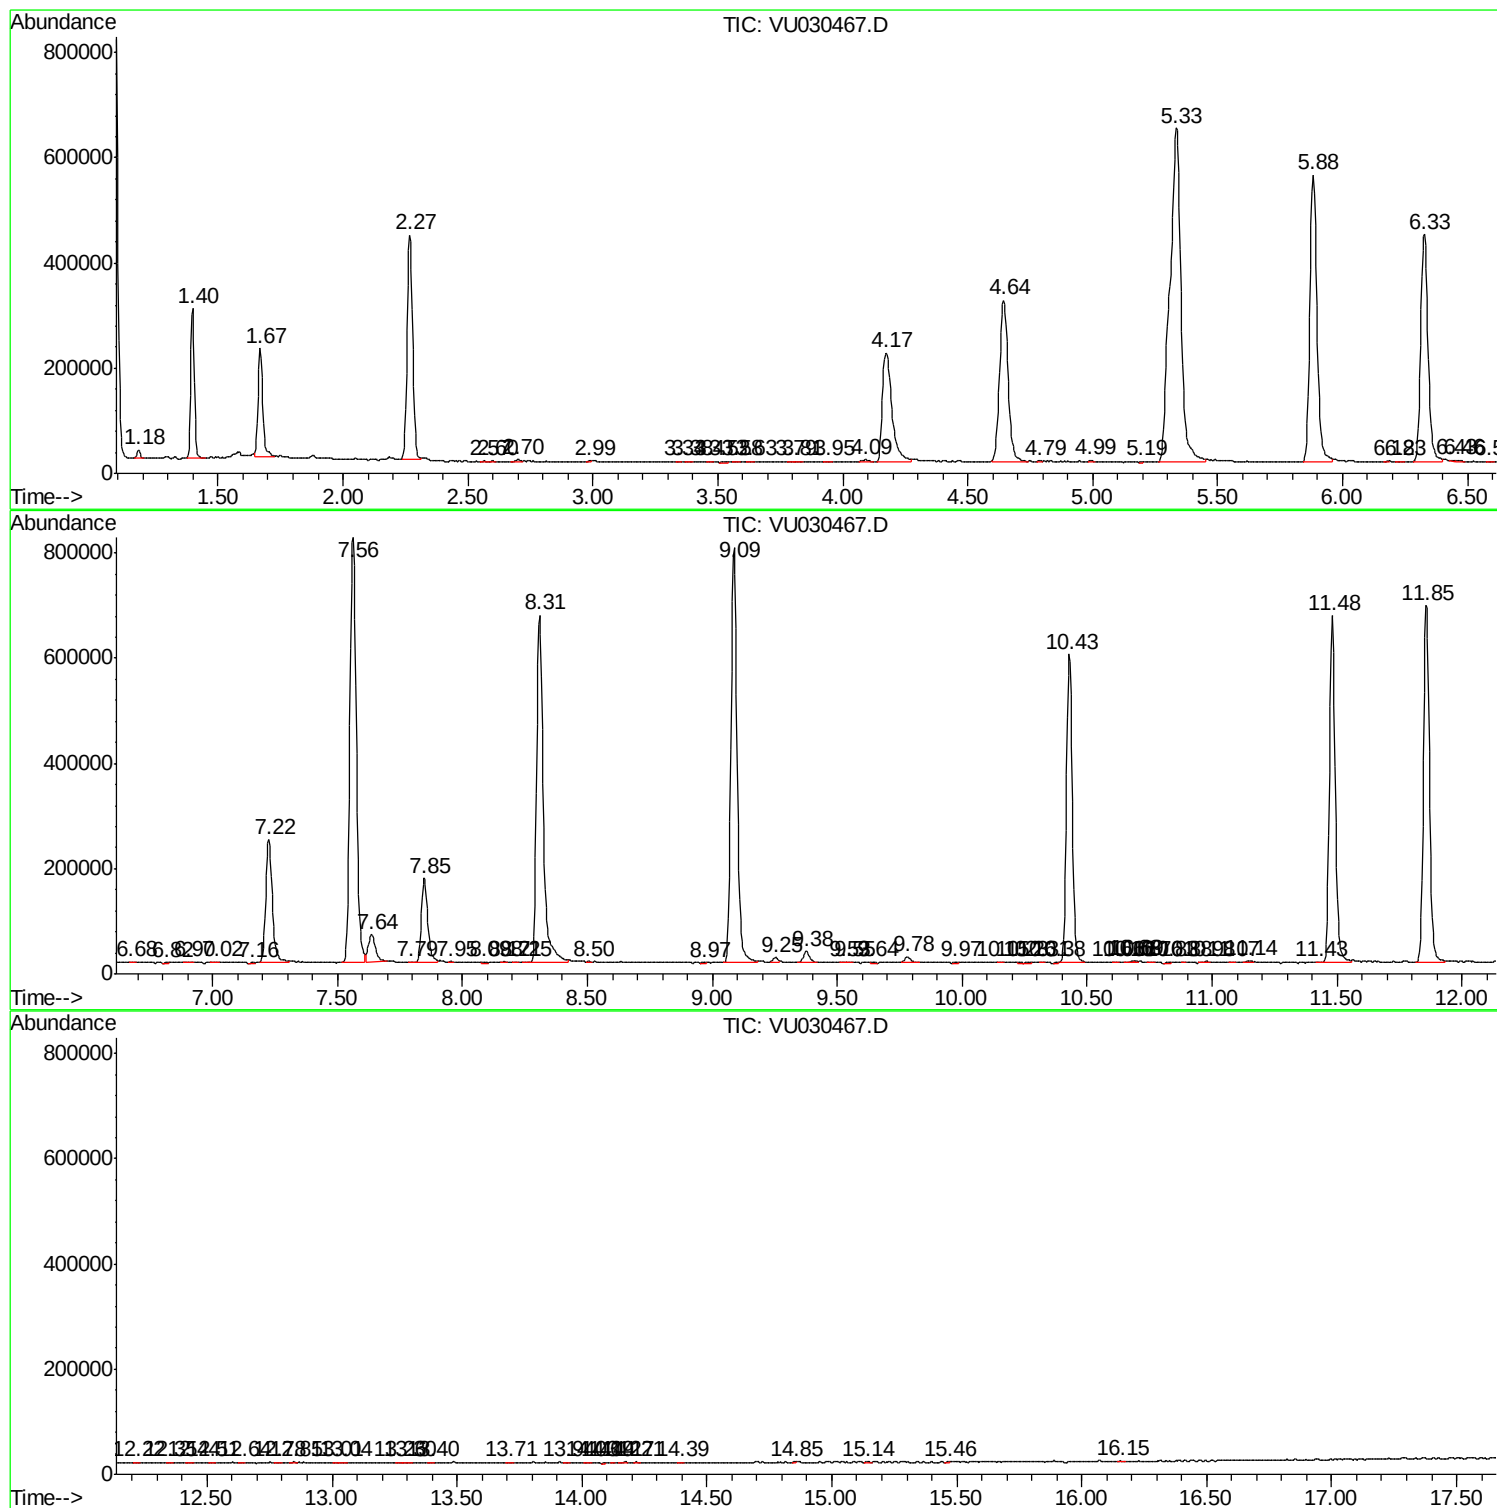

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032619\
Data File : VU030467.D
Acq On : 27 Mar 2019 00:36
Operator : JC/SP
Sample : K2063-14 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB6S1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032619\
Data File : VU030467.D
Acq On : 27 Mar 2019 00:36
Operator : JC/SP
Sample : K2063-14 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DB6S1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc