


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032619\
 Data File : VU030428.D
 Acq On : 26 Mar 2019 08:42
 Operator : JC/SP
 Sample : BFB44
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB44

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis
 Last Update : Thu Mar 28 01:25:46 2019

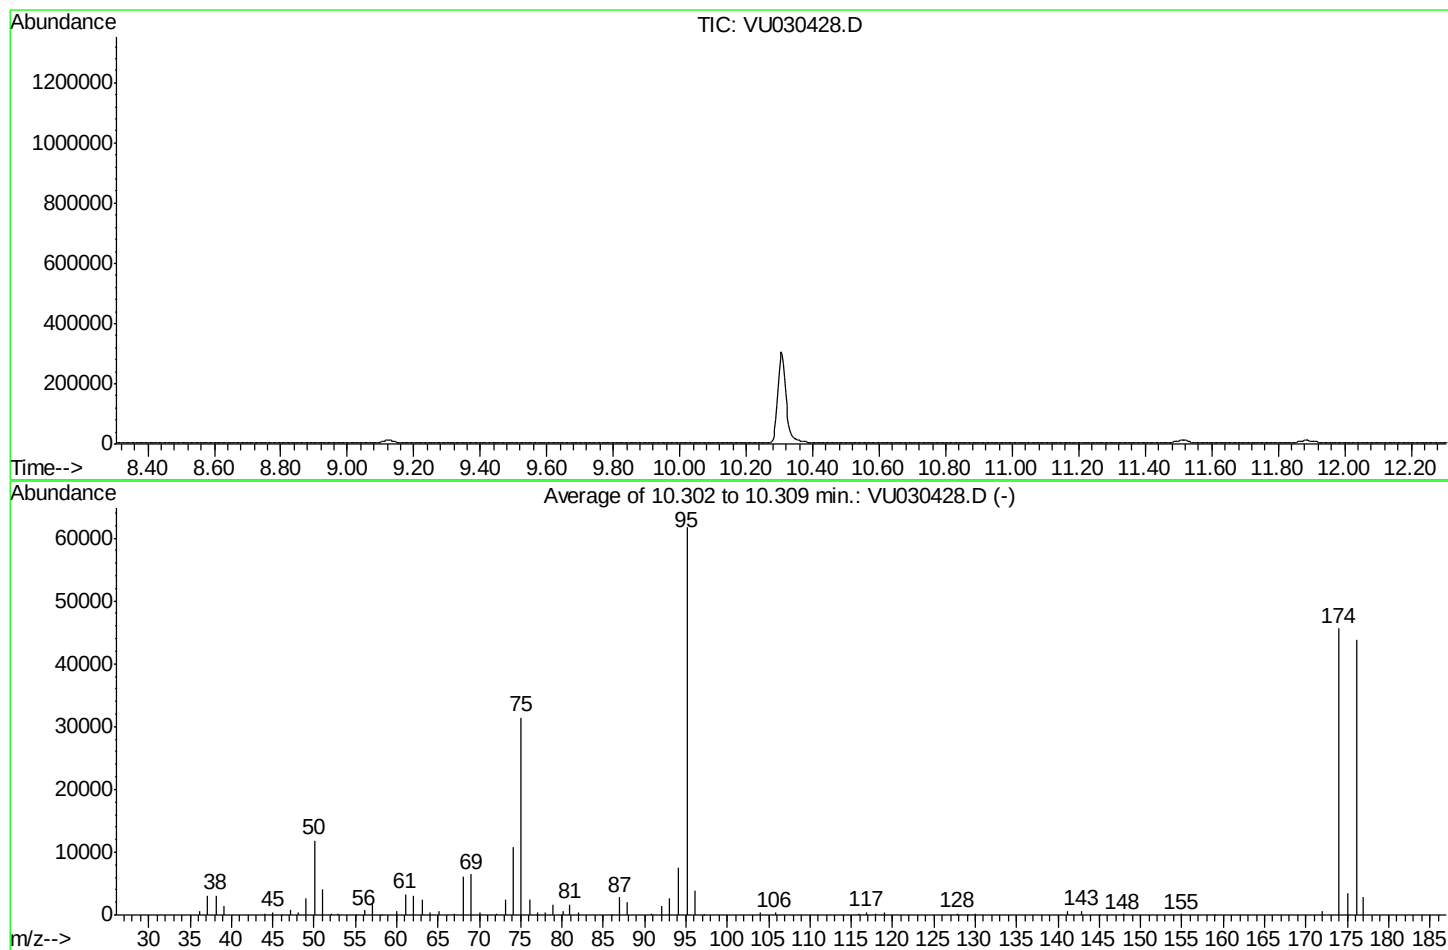

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2854

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.2	11829	PASS
75	95	30	80	51.0	31458	PASS
95	95	100	100	100.0	61714	PASS
96	95	5	9	6.4	3932	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	73.9	45626	PASS
175	174	5	9	7.6	3484	PASS
176	174	95	101	96.0	43789	PASS
177	176	5	9	6.7	2937	PASS

Scan 2854 (10.267 min): VU030428.D
BFB44

m/z	Abundance
40.00	3864.0
44.00	601.0
207.00	121.0

Instrument :
MSVOA_U
ClientSampleId :
BFB44

m/z	Abundance
36.10	765.0
37.00	3090.0
38.10	3132.0
39.10	1282.0
40.00	3729.0
44.00	722.0
45.00	518.0
47.10	838.0
48.10	346.0
49.00	2547.0
50.00	11481.0
51.10	3990.0
52.00	117.0
52.90	200.0
56.10	739.0
57.00	1693.0
58.10	132.0
60.00	624.0
61.00	2992.0
62.10	3205.0
63.10	2378.0
64.10	295.0
65.10	616.0
67.00	170.0
68.00	5775.0
69.10	6448.0
70.00	399.0
72.10	221.0
73.10	2372.0
74.10	10171.0
75.10	30808.0
76.10	2463.0
77.10	407.0
77.90	311.0
79.00	1587.0
80.10	493.0
80.90	1710.0
81.90	348.0
87.00	2714.0
88.00	2107.0
90.90	144.0
92.10	1240.0
93.00	2618.0
94.10	7254.0
95.10	60224.0
96.10	4036.0
97.10	137.0
104.00	306.0
105.80	334.0
115.90	132.0
116.80	393.0
117.90	234.0
119.00	336.0
127.90	259.0
129.00	122.0
129.90	204.0
141.10	552.0
142.90	660.0
145.00	153.0
147.90	206.0
155.00	178.0
172.00	615.0
174.00	42592.0
175.10	3451.0
176.10	40880.0
177.00	2785.0
207.10	119.0

Instrument :
MSVOA_U
ClientSampleId :
BFB44

m/z	Abundance
36.10	753.0
37.10	3142.0
38.10	3201.0
39.10	1559.0
40.00	3718.0
44.00	746.0
45.00	510.0
46.00	101.0
47.10	935.0
48.00	436.0
49.00	2663.0
50.00	12019.0
51.10	4152.0
52.10	123.0
52.90	168.0
55.20	119.0
56.10	817.0
57.00	1845.0
58.10	117.0
60.00	582.0
61.10	3375.0
62.10	3114.0
63.10	2574.0
64.00	318.0
65.00	717.0
67.00	203.0
68.10	6361.0
69.00	6693.0
70.00	437.0
72.10	279.0
73.10	2554.0
74.10	11290.0
75.10	32456.0
76.10	2569.0
77.10	470.0
78.00	370.0
79.00	1737.0
80.10	624.0
80.90	1690.0
82.00	333.0
87.00	2840.0
88.00	2203.0
90.90	150.0
92.10	1437.0
93.00	2744.0
94.10	7980.0
95.10	63616.0
96.10	4023.0
97.10	124.0
104.00	326.0
105.90	373.0
115.80	131.0
116.90	449.0
117.90	232.0
119.00	359.0
127.90	236.0
129.00	118.0
129.90	235.0
141.10	621.0
142.90	695.0
147.90	181.0
155.00	205.0
172.00	726.0
174.00	47072.0
175.00	3591.0
176.10	45280.0
177.00	3037.0
207.10	101.0

Instrument :
MSVOA_U
ClientSampleId :
BFB44

m/z	Abundance
36.10	611.0
37.10	3041.0
38.10	2964.0
39.10	1481.0
40.00	3711.0
44.10	779.0
45.10	476.0
47.10	848.0
48.00	473.0
49.00	2474.0
50.10	11988.0
51.10	4040.0
52.20	117.0
55.00	136.0
56.10	836.0
57.00	1844.0
60.00	542.0
61.10	3421.0
62.00	2781.0
63.00	2500.0
64.00	356.0
65.10	788.0
67.00	189.0
68.10	6422.0
69.00	6237.0
70.00	456.0
72.10	343.0
73.10	2636.0
74.10	11101.0
75.10	31112.0
76.10	2473.0
77.10	456.0
78.00	386.0
78.90	1733.0
80.10	702.0
81.00	1549.0
82.00	372.0
86.10	112.0
87.00	2838.0
87.90	2121.0
90.90	136.0
92.10	1589.0
93.00	2496.0
94.10	7595.0
95.10	61304.0
96.10	3738.0
103.90	333.0
105.90	365.0
115.90	166.0
116.90	444.0
118.00	226.0
118.90	326.0
127.90	180.0
130.00	228.0
141.10	625.0
142.90	634.0
147.90	105.0
155.00	180.0
159.00	102.0
172.00	712.0
174.00	47216.0
175.00	3412.0
176.10	45208.0
177.00	2991.0

Instrument :
MSVOA_U
ClientSampleId :
BFB44