
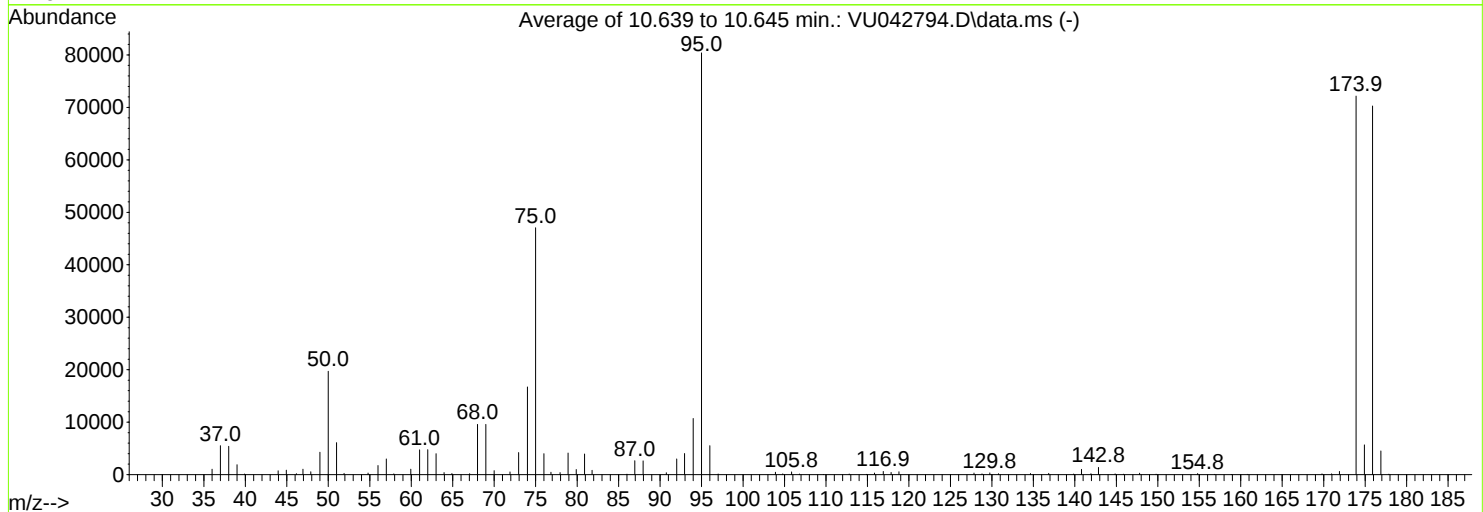


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032621\
Data File : VU042794.D
Acq On : 26 Mar 2021 09:27
Operator : SY/MD
Sample : BFB28
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB28

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M
Title : TRACE VOA SOM01.0
Last Update : Wed Mar 31 02:07:34 2021

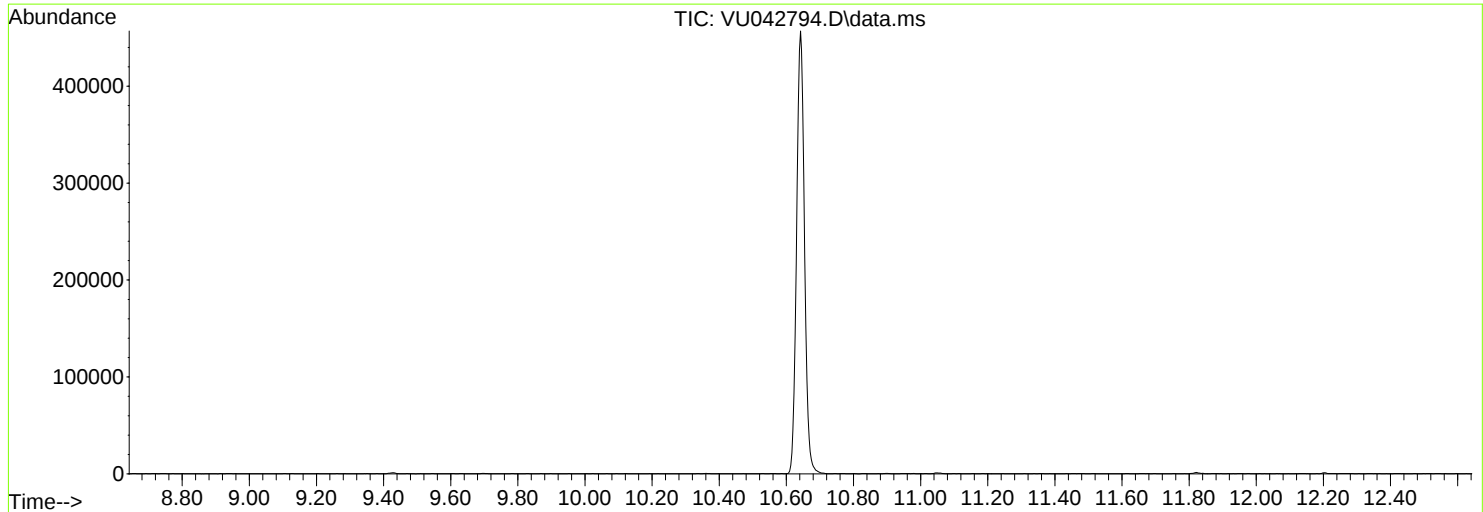

AutoFind: Scans 2892, 2893, 2894; Background Corrected with Scan 2879

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.5	19712	PASS
75	95	30	80	58.5	47061	PASS
95	95	100	100	100.0	80397	PASS
96	95	5	9	6.9	5519	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	89.7	72155	PASS
175	174	5	9	7.9	5688	PASS
176	174	95	101	97.4	70280	PASS
177	176	5	9	6.4	4507	PASS

m/z	Abundance
43.90	249.0

Instrument :
MSVOA_U
ClientSampleId :
BFB28

m/z	Abundance
36.00	969.0
37.00	5855.0
38.00	5197.0
39.00	1886.0
39.90	120.0
44.00	1031.0
44.90	942.0
46.20	213.0
46.90	1060.0
47.90	506.0
49.00	4247.0
50.00	19584.0
51.00	6172.0
51.90	236.0
54.80	318.0
56.00	1673.0
57.00	3052.0
57.90	145.0
59.90	1085.0
61.00	4923.0
62.00	4804.0
63.00	3918.0
63.90	436.0
64.90	239.0
67.00	272.0
68.00	9424.0
69.00	9669.0
70.00	684.0
71.90	562.0
72.90	4113.0
74.00	16624.0
75.00	46576.0
76.00	4113.0
76.90	486.0
78.00	370.0
78.90	3941.0
79.90	1090.0
80.90	4026.0
81.80	763.0
86.00	183.0
87.00	2703.0
88.00	2593.0
90.80	377.0
92.00	2843.0
92.90	4043.0
94.00	10435.0
95.00	79672.0
96.00	5489.0
97.00	100.0
103.90	514.0
104.90	152.0
105.90	516.0
106.80	104.0
109.70	112.0
112.80	130.0
114.90	106.0
115.90	292.0
116.90	544.0
117.90	415.0
118.80	604.0
127.80	270.0
128.80	161.0
129.70	330.0
130.80	139.0
134.60	194.0
136.90	223.0
139.90	118.0
140.80	984.0
142.00	158.0
142.80	1359.0
144.80	170.0
147.80	293.0
149.80	138.0
154.80	209.0
158.90	112.0
160.90	100.0
169.80	140.0
171.10	115.0
171.90	623.0
173.90	69464.0
174.90	5537.0
175.90	67512.0
176.90	4596.0
177.90	140.0

Instrument :
MSVOA_U
ClientSampleId :
BFB28

m/z	Abundance
36.00	1090.0
37.00	5719.0
38.00	5516.0
39.00	1952.0
39.90	125.0
44.00	993.0
44.90	854.0
46.20	185.0
46.90	1090.0
47.90	544.0
49.00	4427.0
50.00	20296.0
51.00	6297.0
51.90	259.0
54.80	329.0
56.00	1816.0
57.00	3091.0
57.90	171.0
59.90	1074.0
61.00	4817.0
62.00	4913.0
63.00	4157.0
64.00	414.0
64.90	216.0
67.10	260.0
68.00	9888.0
69.00	9820.0
70.00	784.0
71.90	541.0
72.90	4310.0
74.00	17200.0
75.00	48584.0
76.00	4167.0
76.90	476.0
78.00	405.0
78.90	4311.0
79.90	989.0
80.90	4001.0
81.80	834.0
86.00	138.0
86.90	2693.0
87.90	2744.0
90.80	357.0
92.00	3160.0
92.90	4122.0
94.00	10966.0
95.00	82752.0
96.00	5673.0
97.00	119.0
103.90	449.0
104.80	180.0
105.90	502.0
106.80	123.0
112.80	127.0
114.90	115.0
115.90	313.0
116.90	644.0
117.90	445.0
118.80	560.0
127.80	308.0
128.80	161.0
129.80	353.0
130.80	204.0
134.70	222.0
136.80	251.0
139.80	116.0
140.80	1017.0
141.90	213.0
142.90	1439.0
144.80	171.0
145.90	142.0
147.80	292.0
149.80	122.0
154.80	240.0
156.90	104.0
160.80	115.0
169.80	164.0
170.90	165.0
171.90	659.0
173.90	74400.0
174.90	5867.0
175.90	72296.0
176.90	4632.0
177.80	123.0

Instrument :
MSVOA_U
ClientSampleId :
BFB28

m/z	Abundance
36.00	1051.0
37.00	5032.0
38.00	5455.0
39.00	1827.0
39.90	118.0
44.00	961.0
45.00	760.0
46.10	137.0
47.00	993.0
47.90	595.0
49.00	4188.0
50.00	19256.0
51.00	5799.0
51.90	249.0
54.80	267.0
56.00	1777.0
57.00	2869.0
57.90	170.0
60.00	990.0
61.00	4464.0
62.00	4553.0
63.00	3937.0
64.00	380.0
64.90	214.0
68.00	9439.0
69.00	9279.0
70.00	813.0
71.90	478.0
73.00	4180.0
74.00	16359.0
75.00	46024.0
76.00	3737.0
76.80	425.0
77.90	384.0
78.90	4143.0
79.90	882.0
80.90	3796.0
81.80	870.0
86.90	2546.0
87.90	2579.0
90.70	341.0
92.00	2950.0
93.00	3944.0
94.00	10706.0
95.00	78768.0
96.00	5395.0
97.00	117.0
103.90	409.0
104.70	160.0
105.80	511.0
106.80	103.0
112.80	134.0
115.80	339.0
116.90	664.0
117.80	450.0
118.80	482.0
127.90	315.0
128.80	163.0
129.80	321.0
130.80	227.0
134.70	229.0
136.80	252.0
139.80	113.0
140.80	1003.0
141.90	220.0
142.90	1354.0
144.90	144.0
145.80	177.0
147.80	229.0
154.80	241.0
156.80	126.0
169.80	126.0
170.90	154.0
171.90	598.0
173.90	72600.0
174.90	5661.0
175.90	71032.0
176.90	4294.0

Instrument :
MSVOA_U
ClientSampleId :
BFB28