

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032719\
 Data File : VU030473.D
 Acq On : 27 Mar 2019 11:03
 Operator : JC/SP
 Sample : VU0327WBL01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK59

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.183	25	29	38	rVB	15068	15502	0.92%	0.122%
2	1.399	89	96	108	rBV	248552	253336	14.96%	1.993%
3	1.678	176	183	203	rVB	194388	245729	14.51%	1.934%
4	2.270	357	367	381	rBV	380542	578784	34.17%	4.554%
5	2.688	493	497	500	rBV	1877	1990	0.12%	0.016%
6	2.772	518	523	525	rBV	1747	1833	0.11%	0.014%
7	3.421	721	725	728	rBV	1319	1163	0.07%	0.009%
8	3.604	779	782	785	rBV	1621	1183	0.07%	0.009%
9	3.971	892	896	899	rBV	1402	1301	0.08%	0.010%
10	4.125	939	944	947	rBV	1449	1375	0.08%	0.011%
11	4.173	947	959	995	rBV	178465	487911	28.80%	3.839%
12	4.643	1090	1105	1128	rVV2	270062	649434	38.34%	5.110%
13	5.042	1223	1229	1231	rBV	1500	1311	0.08%	0.010%
14	5.164	1261	1267	1271	rVB3	1375	1583	0.09%	0.012%
15	5.337	1297	1321	1354	rBV2	558368	1693939	100.00%	13.329%
16	5.884	1478	1491	1510	rBV	474428	941850	55.60%	7.411%
17	6.328	1615	1629	1654	rBV	378576	778123	45.94%	6.123%
18	6.759	1760	1763	1767	rVB	1531	1095	0.06%	0.009%
19	6.887	1799	1803	1804	rBV	1225	969	0.06%	0.008%
20	7.103	1867	1870	1875	rBV2	1656	1949	0.12%	0.015%
21	7.225	1897	1908	1924	rVV	200860	369494	21.81%	2.907%
22	7.562	2000	2013	2034	rBV	693886	1243915	73.43%	9.788%
23	7.775	2076	2079	2083	rVB	1561	963	0.06%	0.008%
24	7.800	2083	2087	2091	rBV2	1646	1634	0.10%	0.013%
25	7.849	2091	2102	2124	rBV	138513	253752	14.98%	1.997%
26	8.122	2183	2187	2192	rBV	1995	2127	0.13%	0.017%
27	8.308	2234	2245	2286	rVV	542896	1057444	62.43%	8.321%
28	8.591	2330	2333	2338	rBV2	1225	1169	0.07%	0.009%
29	8.620	2338	2342	2346	rVV	1315	1053	0.06%	0.008%
30	8.906	2428	2431	2433	rVV	1779	1219	0.07%	0.010%
31	9.086	2474	2487	2512	rBV	679487	1174455	69.33%	9.241%
32	9.257	2534	2540	2543	rBV4	1198	1328	0.08%	0.010%
33	9.385	2574	2580	2586	rBV5	2735	3401	0.20%	0.027%
34	9.649	2657	2662	2667	rBV	1600	1640	0.10%	0.013%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032719\
 Data File : VU030473.D
 Acq On : 27 Mar 2019 11:03
 Operator : JC/SP
 Sample : VU0327WBL01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK59

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

35	9.675	2667	2670	2675	rVB2	1702	1805	0.11%	0.014%
36	9.807	2709	2711	2714	rVV2	1984	1062	0.06%	0.008%
37	10.025	2772	2779	2784	rVB3	1608	2225	0.13%	0.018%
38	10.170	2818	2824	2829	rBV4	1791	2250	0.13%	0.018%
39	10.260	2848	2852	2855	rVB2	1113	901	0.05%	0.007%
40	10.295	2860	2863	2867	rVB	1308	906	0.05%	0.007%
41	10.427	2892	2904	2923	rBV	502721	830498	49.03%	6.535%
42	10.527	2932	2935	2939	rBV	1203	1278	0.08%	0.010%
43	10.575	2943	2950	2954	rVB	942	1350	0.08%	0.011%
44	10.601	2954	2958	2963	rBV3	1446	1549	0.09%	0.012%
45	10.630	2963	2967	2972	rVB	1096	1118	0.07%	0.009%
46	10.832	3027	3030	3035	rVB	1000	947	0.06%	0.007%
47	10.868	3035	3041	3044	rBV	1622	1552	0.09%	0.012%
48	11.025	3086	3090	3093	rBV	1154	887	0.05%	0.007%
49	11.096	3108	3112	3116	rBV	1525	1289	0.08%	0.010%
50	11.119	3116	3119	3123	rBV2	1298	1188	0.07%	0.009%
51	11.164	3129	3133	3136	rBV	1318	991	0.06%	0.008%
52	11.183	3136	3139	3144	rVB2	1190	1272	0.08%	0.010%
53	11.234	3150	3155	3158	rBV	1254	1153	0.07%	0.009%
54	11.418	3205	3212	3213	rBV4	2593	2462	0.15%	0.019%
55	11.482	3219	3232	3257	rBV	581018	961810	56.78%	7.568%
56	11.681	3291	3294	3302	rVB2	1191	1185	0.07%	0.009%
57	11.781	3321	3325	3328	rBV	2351	2285	0.13%	0.018%
58	11.858	3337	3349	3374	rBV	605982	1017750	60.08%	8.008%
59	12.196	3450	3454	3457	rBV	1422	1346	0.08%	0.011%
60	12.273	3474	3478	3480	rBV	1300	1014	0.06%	0.008%
61	12.405	3515	3519	3523	rVB2	1337	985	0.06%	0.008%
62	12.475	3532	3541	3542	rBV2	1437	1630	0.10%	0.013%
63	12.575	3566	3572	3576	rBV2	1677	1716	0.10%	0.014%
64	12.675	3600	3603	3606	rBV3	1286	1123	0.07%	0.009%
65	12.778	3629	3635	3637	rBV2	1263	1247	0.07%	0.010%
66	12.836	3649	3653	3654	rBV2	1543	956	0.06%	0.008%
67	12.900	3665	3673	3679	rBV6	3718	5660	0.33%	0.045%
68	12.932	3680	3683	3689	rVB	1473	992	0.06%	0.008%
69	13.154	3748	3752	3755	rBV2	1406	1174	0.07%	0.009%
70	13.221	3769	3773	3775	rVV2	1149	914	0.05%	0.007%
71	13.247	3778	3781	3787	rVB2	1691	1572	0.09%	0.012%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032719\
 Data File : VU030473.D
 Acq On : 27 Mar 2019 11:03
 Operator : JC/SP
 Sample : VU0327WBL01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK59

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

72	13.299	3793	3797	3800	rBV2	1459	1471	0.09%	0.012%
73	13.356	3811	3815	3818	rBV3	1500	1327	0.08%	0.010%
74	13.389	3822	3825	3831	rVB3	1784	1363	0.08%	0.011%
75	13.417	3831	3834	3840	rBV2	1256	1107	0.07%	0.009%
76	13.517	3855	3865	3875	rVV9	5239	8745	0.52%	0.069%
77	13.630	3897	3900	3904	rVB	1675	1000	0.06%	0.008%
78	13.684	3911	3917	3920	rBV	983	1058	0.06%	0.008%
79	13.758	3930	3940	3946	rBV6	10041	20238	1.19%	0.159%
80	13.938	3993	3996	4000	rVB2	1656	1023	0.06%	0.008%
81	13.996	4004	4014	4017	rBV6	6606	9784	0.58%	0.077%
82	14.208	4073	4080	4082	rBV	1872	2184	0.13%	0.017%
83	14.356	4122	4126	4129	rVB3	1195	1014	0.06%	0.008%
84	14.382	4130	4134	4140	rBV	1016	1119	0.07%	0.009%
85	14.466	4157	4160	4165	rVV	1090	958	0.06%	0.008%
86	14.585	4195	4197	4202	rVB2	1332	914	0.05%	0.007%
87	14.617	4203	4207	4212	rVB2	1326	925	0.05%	0.007%
88	14.736	4241	4244	4251	rVB	1836	1995	0.12%	0.016%
89	14.855	4276	4281	4284	rBV2	1028	1054	0.06%	0.008%
90	14.893	4290	4293	4298	rBV2	1054	952	0.06%	0.007%
91	15.041	4336	4339	4344	rVB2	1480	1264	0.07%	0.010%
92	15.080	4347	4351	4356	rVB2	1851	1397	0.08%	0.011%
93	15.221	4392	4395	4399	rVB2	1636	1062	0.06%	0.008%
94	15.250	4399	4404	4405	rBV2	1184	1006	0.06%	0.008%
95	15.315	4420	4424	4428	rBV	1651	1396	0.08%	0.011%
96	15.337	4429	4431	4437	rVB	1537	1198	0.07%	0.009%
97	15.385	4437	4446	4455	rBV2	1835	4323	0.26%	0.034%
98	15.585	4503	4508	4512	rBV2	1650	1625	0.10%	0.013%
99	15.816	4575	4580	4584	rBV5	1597	1854	0.11%	0.015%
100	16.176	4690	4692	4697	rBV4	1474	1352	0.08%	0.011%


Sum of corrected areas: 12708704

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU032719\
Data File : VU030473.D
Acq On : 27 Mar 2019 11:03
Operator : JC/SP
Sample : VU0327WBL01
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK59

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

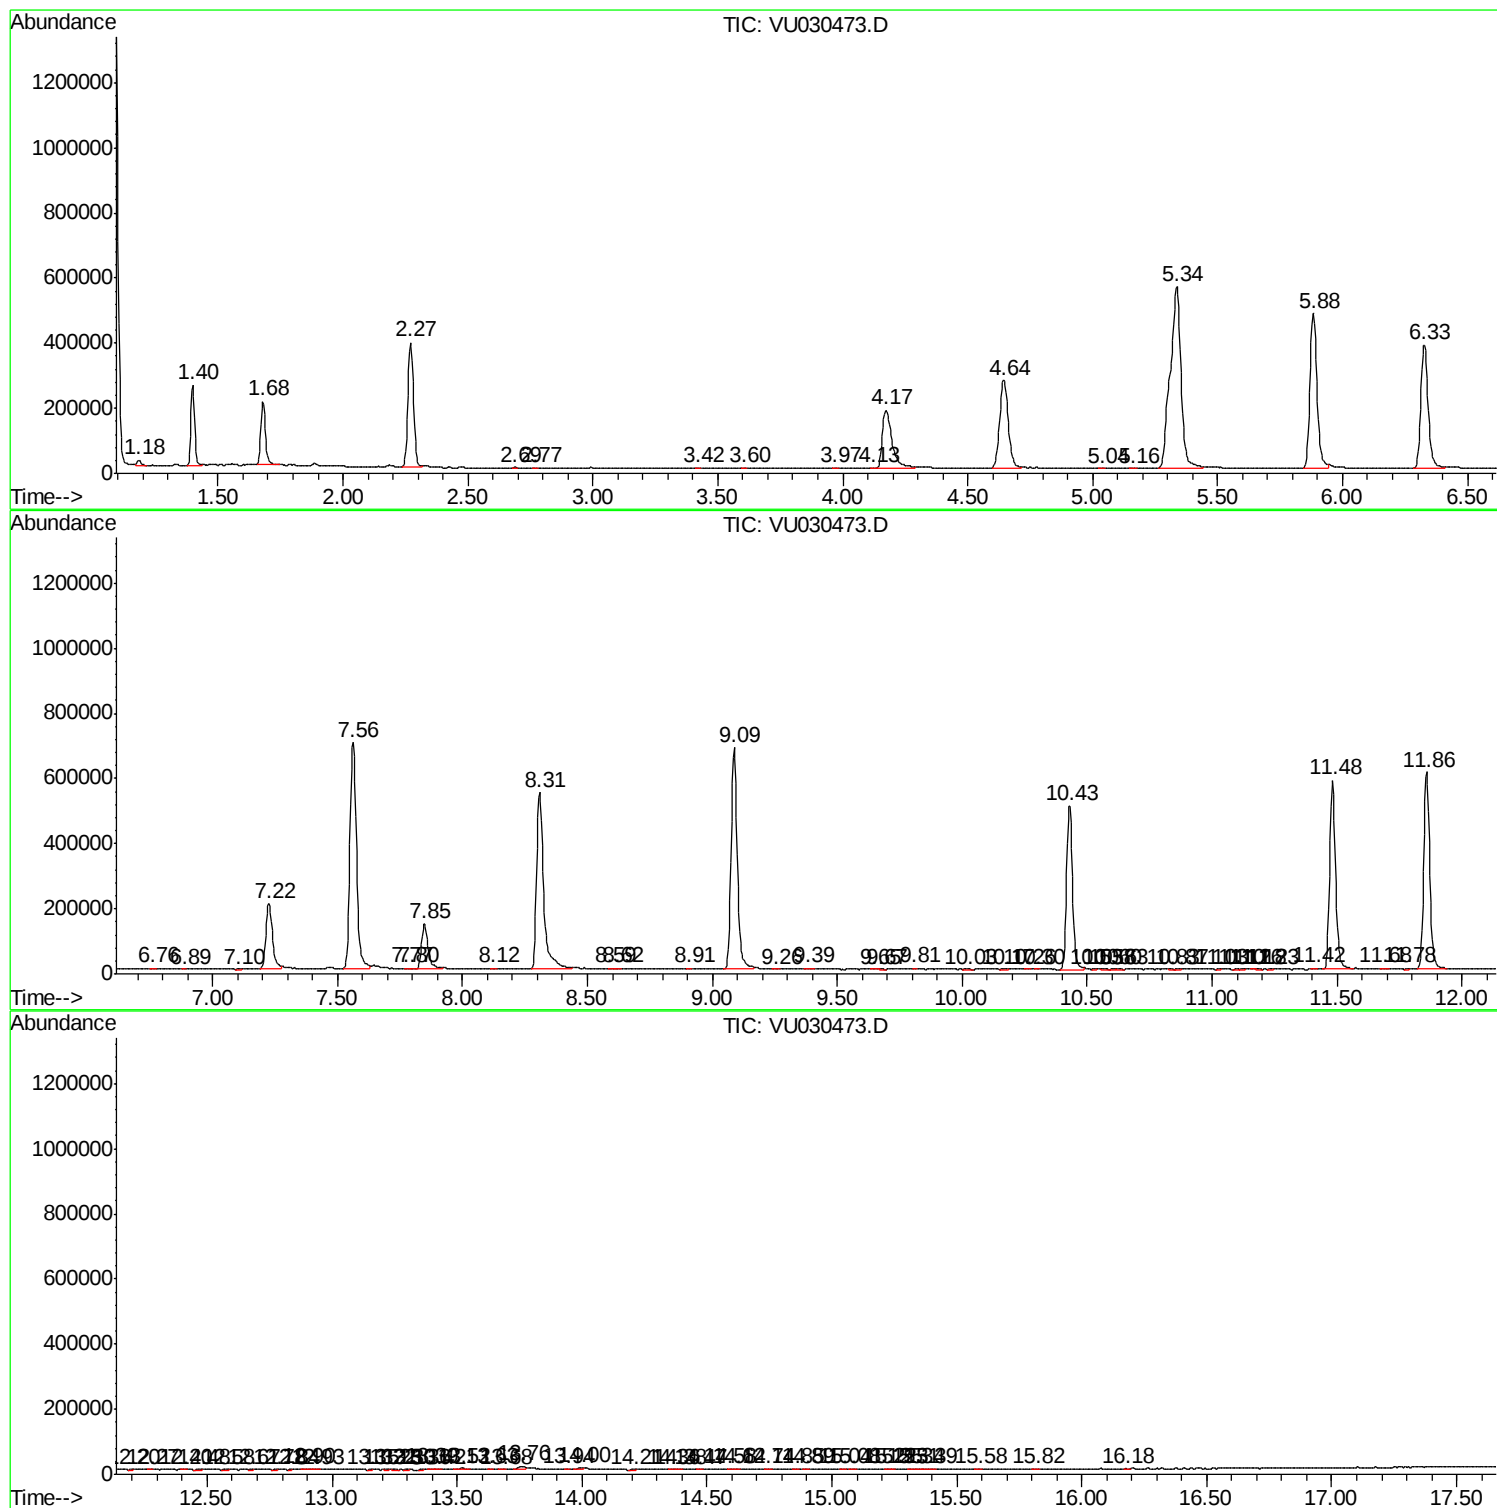

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032719\
Data File : VU030473.D
Acq On : 27 Mar 2019 11:03
Operator : JC/SP
Sample : VU0327WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK59

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032719\
Data File : VU030473.D
Acq On : 27 Mar 2019 11:03
Operator : JC/SP
Sample : VU0327WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK59

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc