

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032719\
 Data File : VU030478.D
 Acq On : 27 Mar 2019 13:09
 Operator : JC/SP
 Sample : K2022-18 20X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C09F3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.183	25	29	37	rVB	14135	13345	0.30%	0.074%
2	1.399	89	96	108	rVB	243603	244429	5.53%	1.361%
3	1.672	174	181	194	rVB	188612	242992	5.50%	1.353%
4	2.270	357	367	381	rBV	381054	578874	13.10%	3.224%
5	4.173	948	959	989	rBV	196220	513040	11.61%	2.858%
6	4.643	1091	1105	1128	rBV	291248	685899	15.52%	3.820%
7	5.337	1299	1321	1348	rBV2	603371	1804876	40.83%	10.053%
8	5.884	1478	1491	1515	rBV	527533	1054805	23.86%	5.875%
9	6.205	1588	1591	1593	rBV	2180	1519	0.03%	0.008%
10	6.328	1615	1629	1653	rBV	415976	845326	19.12%	4.708%
11	7.225	1897	1908	1925	rBV	225849	412837	9.34%	2.299%
12	7.562	2000	2013	2053	rBV	761270	1368911	30.97%	7.625%
13	7.845	2091	2101	2125	rBV	156765	282338	6.39%	1.573%
14	8.308	2234	2245	2279	rBV	613693	1135477	25.69%	6.325%
15	8.836	2406	2409	2413	rBV	1537	1389	0.03%	0.008%
16	9.086	2475	2487	2492	rBV	819599	1373658	31.08%	7.651%
17	9.475	2606	2608	2613	rBV	1097	887	0.02%	0.005%
18	9.549	2628	2631	2634	rVB2	1710	1007	0.02%	0.006%
19	9.575	2634	2639	2644	rBV	1500	1834	0.04%	0.010%
20	9.630	2653	2656	2658	rBV	1505	1020	0.02%	0.006%
21	9.797	2701	2708	2712	rBV	2050	3094	0.07%	0.017%
22	9.865	2726	2729	2731	rBV	1220	870	0.02%	0.005%
23	10.025	2776	2779	2782	rBV	1313	1036	0.02%	0.006%
24	10.109	2800	2805	2809	rBV	2226	2302	0.05%	0.013%
25	10.173	2823	2825	2829	rBV	1197	747	0.02%	0.004%
26	10.221	2837	2840	2845	rVB	1874	1396	0.03%	0.008%
27	10.250	2845	2849	2851	rBV	1098	905	0.02%	0.005%
28	10.279	2855	2858	2861	rBV2	1131	730	0.02%	0.004%
29	10.427	2891	2904	2928	rVB	560091	911867	20.63%	5.079%
30	10.675	2977	2981	2983	rBV	2280	1759	0.04%	0.010%
31	10.742	2997	3002	3007	rBV	2040	2109	0.05%	0.012%
32	10.890	3045	3048	3052	rVB	1492	1068	0.02%	0.006%
33	10.916	3054	3056	3060	rVV	1347	824	0.02%	0.005%
34	10.983	3074	3077	3079	rBV	863	705	0.02%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032719\
 Data File : VU030478.D
 Acq On : 27 Mar 2019 13:09
 Operator : JC/SP
 Sample : K2022-18 20X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C09F3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

35	11.032	3089	3092	3094	rBV	1234	935	0.02%	0.005%
36	11.273	3164	3167	3171	rBV	1216	872	0.02%	0.005%
37	11.418	3202	3212	3220	rBV2	51057	81083	1.83%	0.452%
38	11.482	3220	3232	3255	rVB2	697677	1402120	31.72%	7.810%
39	11.713	3302	3304	3306	rBV3	1299	749	0.02%	0.004%
40	11.874	3333	3354	3381	rBV2	2185329	4420376	100.00%	24.621%
41	12.270	3474	3477	3481	rBV2	1053	826	0.02%	0.005%
42	12.305	3486	3488	3492	rBV	1097	749	0.02%	0.004%
43	12.501	3546	3549	3552	rBV2	1046	791	0.02%	0.004%
44	12.565	3565	3569	3576	rBV	1727	2351	0.05%	0.013%
45	12.832	3650	3652	3657	rVB2	1361	1040	0.02%	0.006%
46	12.858	3657	3660	3662	rBV	1311	944	0.02%	0.005%
47	12.935	3682	3684	3689	rBV	1303	1074	0.02%	0.006%
48	13.118	3738	3741	3745	rVB2	1152	898	0.02%	0.005%
49	13.144	3745	3749	3751	rBV	864	692	0.02%	0.004%
50	13.292	3793	3795	3798	rVB2	1127	648	0.01%	0.004%
51	13.311	3798	3801	3807	rBV	1919	1669	0.04%	0.009%
52	13.340	3807	3810	3814	rVB	1798	1366	0.03%	0.008%
53	13.372	3814	3820	3823	rBV2	1914	2072	0.05%	0.012%
54	13.417	3831	3834	3836	rVB	1115	614	0.01%	0.003%
55	13.437	3836	3840	3841	rBV	1348	943	0.02%	0.005%
56	13.501	3849	3860	3888	rBV	225555	421934	9.55%	2.350%
57	13.649	3904	3906	3911	rVB2	1515	1073	0.02%	0.006%
58	13.816	3955	3958	3960	rBV2	970	700	0.02%	0.004%
59	13.903	3982	3985	3988	rBV2	945	610	0.01%	0.003%
60	13.935	3992	3995	3998	rBV	949	767	0.02%	0.004%
61	13.990	4002	4012	4027	rBV3	32696	66301	1.50%	0.369%
62	14.118	4047	4052	4054	rBV2	1042	1028	0.02%	0.006%
63	14.131	4054	4056	4063	rVB2	1421	1358	0.03%	0.008%
64	14.218	4080	4083	4086	rBV	1313	969	0.02%	0.005%
65	14.305	4105	4110	4113	rBV2	1077	913	0.02%	0.005%
66	14.347	4120	4123	4126	rBV2	1172	697	0.02%	0.004%
67	14.382	4129	4134	4135	rBV	1350	986	0.02%	0.005%
68	14.437	4148	4151	4156	rVB2	1892	1689	0.04%	0.009%
69	14.466	4156	4160	4162	rBV	1263	1037	0.02%	0.006%
70	14.511	4168	4174	4180	rBV2	2175	2773	0.06%	0.015%
71	14.546	4180	4185	4189	rVB	1354	1049	0.02%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032719\
 Data File : VU030478.D
 Acq On : 27 Mar 2019 13:09
 Operator : JC/SP
 Sample : K2022-18 20X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C09F3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

72	14.591	4195	4199	4201	rBV3	827	623	0.01%	0.003%
73	14.671	4221	4224	4227	rBV2	697	626	0.01%	0.003%
74	14.697	4227	4232	4234	rVV2	1225	1250	0.03%	0.007%
75	14.713	4234	4237	4240	rVV	1955	1394	0.03%	0.008%
76	14.749	4243	4248	4251	rVB	1079	1141	0.03%	0.006%
77	14.765	4251	4253	4256	rBV	1003	613	0.01%	0.003%
78	14.829	4268	4273	4275	rVV2	829	856	0.02%	0.005%
79	14.855	4279	4281	4284	rVV2	1177	770	0.02%	0.004%
80	14.961	4310	4314	4319	rVB	1487	1203	0.03%	0.007%
81	14.996	4320	4325	4328	rBV3	960	948	0.02%	0.005%
82	15.015	4328	4331	4334	rVB	1196	731	0.02%	0.004%
83	15.038	4334	4338	4342	rBV	919	1042	0.02%	0.006%
84	15.083	4349	4352	4356	rVB	1610	1183	0.03%	0.007%
85	15.102	4356	4358	4360	rBV	1117	646	0.01%	0.004%
86	15.131	4363	4367	4369	rBV2	1879	1289	0.03%	0.007%
87	15.221	4388	4395	4396	rBV2	1294	1146	0.03%	0.006%
88	15.244	4400	4402	4406	rVV2	765	663	0.01%	0.004%
89	15.279	4410	4413	4418	rVB3	917	752	0.02%	0.004%
90	15.318	4422	4425	4432	rBV3	2219	2217	0.05%	0.012%
91	15.356	4432	4437	4443	rVB2	1794	2420	0.05%	0.013%
92	15.411	4448	4454	4458	rBV4	963	1139	0.03%	0.006%
93	15.459	4466	4469	4471	rVB2	1324	675	0.02%	0.004%
94	15.482	4471	4476	4479	rBV3	1620	1250	0.03%	0.007%
95	15.540	4491	4494	4498	rVB2	1179	996	0.02%	0.006%
96	15.642	4523	4526	4531	rBV2	1120	1225	0.03%	0.007%
97	15.707	4543	4546	4552	rVB3	2728	2506	0.06%	0.014%
98	15.736	4552	4555	4558	rBV2	1185	1036	0.02%	0.006%
99	15.842	4584	4588	4592	rBV3	1361	1451	0.03%	0.008%
100	16.076	4658	4661	4665	rBV4	1291	1214	0.03%	0.007%


Sum of corrected areas: 17953576

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU032719\
Data File : VU030478.D
Acq On : 27 Mar 2019 13:09
Operator : JC/SP
Sample : K2022-18 20X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C09F3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

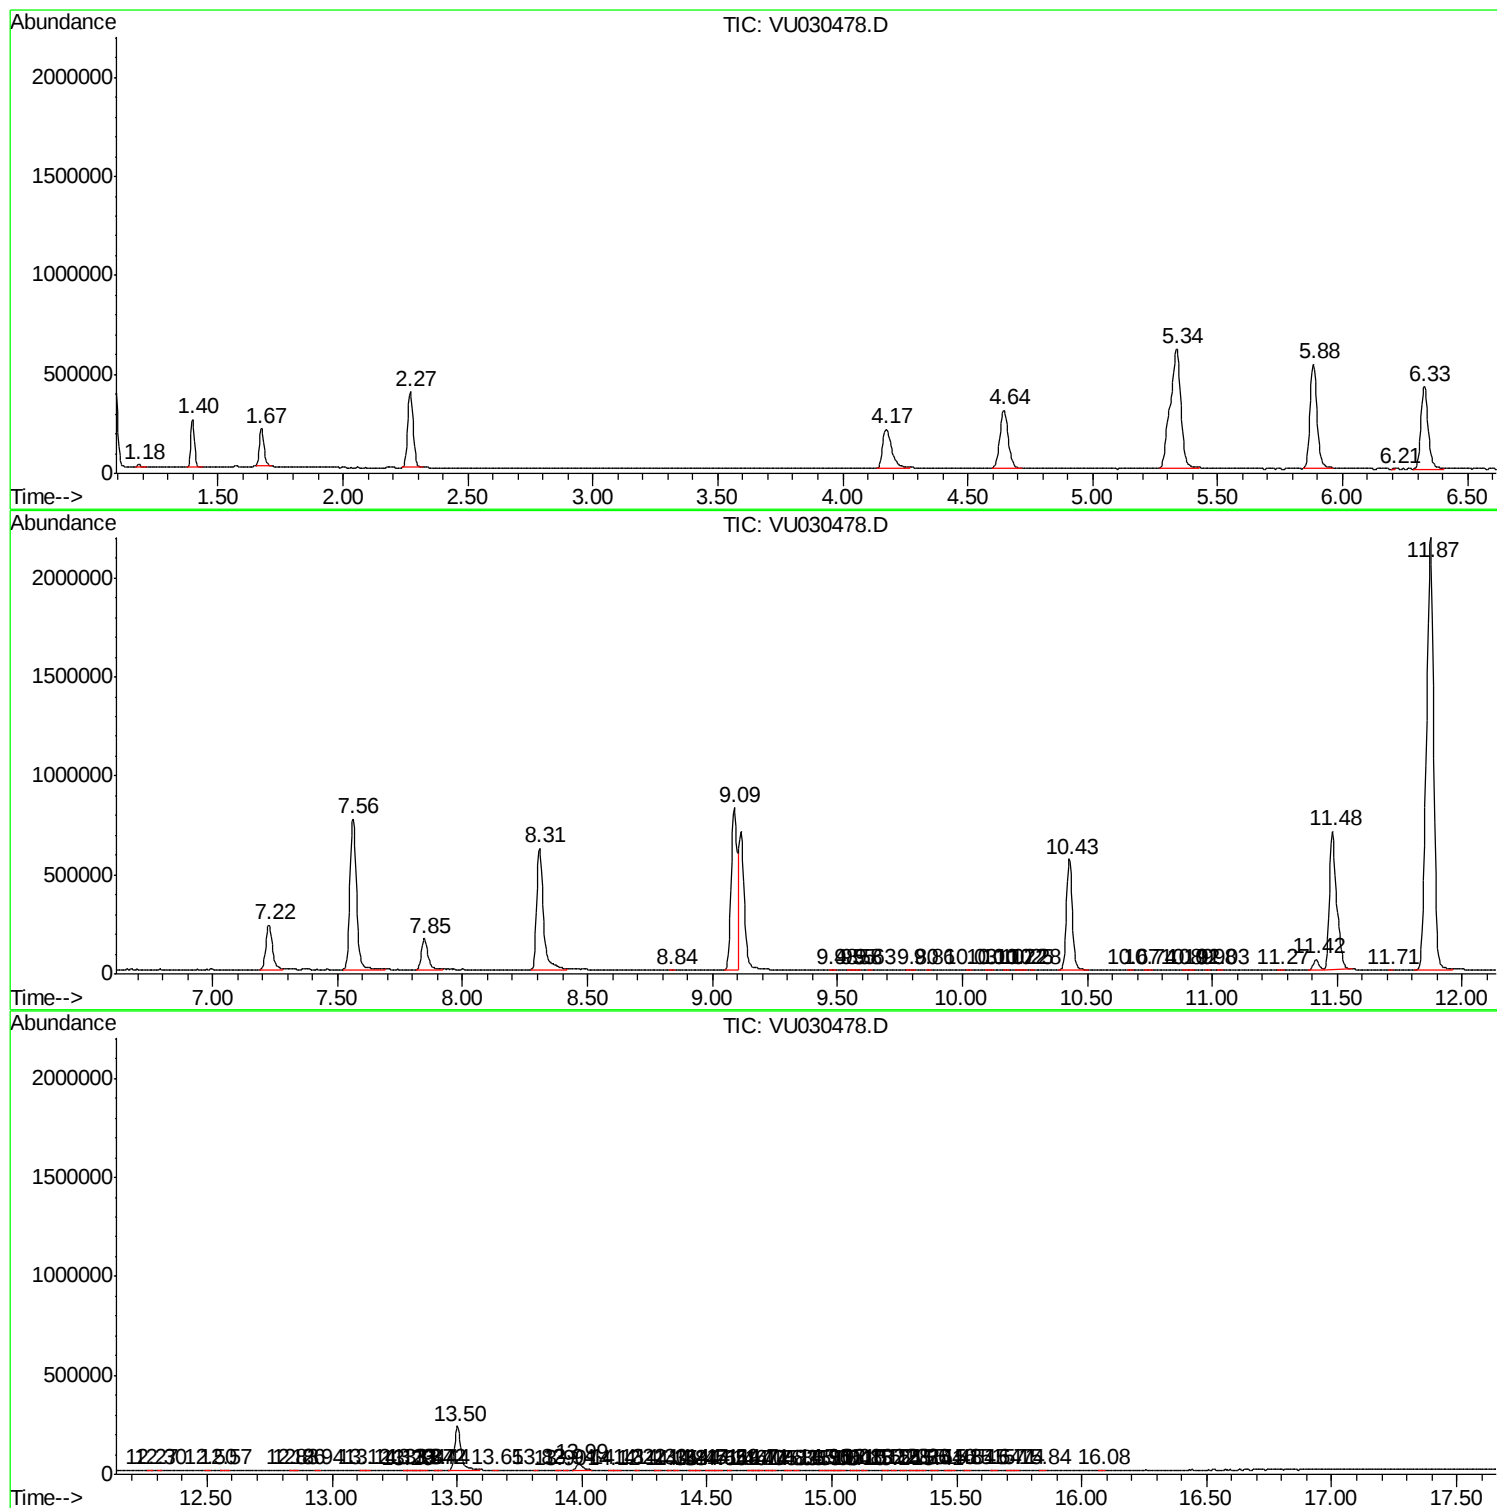

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032719\
Data File : VU030478.D
Acq On : 27 Mar 2019 13:09
Operator : JC/SP
Sample : K2022-18 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C09F3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032719\
Data File : VU030478.D
Acq On : 27 Mar 2019 13:09
Operator : JC/SP
Sample : K2022-18 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C09F3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc