

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032719\
 Data File : VU030500.D
 Acq On : 27 Mar 2019 21:53
 Operator : JC/SP
 Sample : K2120-09
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF5D4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.399	90	96	107	rVB	247775	243966	15.36%	2.017%
2	1.678	176	183	200	rVB	174152	233796	14.72%	1.933%
3	2.270	357	367	379	rBV	358222	542434	34.16%	4.485%
4	2.547	449	453	458	rBV	1193	1220	0.08%	0.010%
5	2.579	459	463	468	rBV	2171	2487	0.16%	0.021%
6	2.662	485	489	500	rBV	1436	2068	0.13%	0.017%
7	2.743	511	514	517	rBV	2067	1292	0.08%	0.011%
8	3.016	594	599	603	rBV	2333	2590	0.16%	0.021%
9	3.235	663	667	670	rBV	1887	1686	0.11%	0.014%
10	3.415	719	723	729	rBV2	1296	1996	0.13%	0.017%
11	3.518	752	755	759	rBV	1406	1423	0.09%	0.012%
12	3.559	765	768	770	rVB2	703	405	0.03%	0.003%
13	3.717	812	817	820	rBV	1049	967	0.06%	0.008%
14	3.736	820	823	826	rVB	1439	869	0.05%	0.007%
15	3.762	827	831	833	rBV	1380	930	0.06%	0.008%
16	3.807	842	845	847	rVB2	768	445	0.03%	0.004%
17	3.826	847	851	853	rBV	1579	1208	0.08%	0.010%
18	3.897	870	873	875	rBV	1175	733	0.05%	0.006%
19	4.042	915	918	922	rBV	873	509	0.03%	0.004%
20	4.174	948	959	990	rBV	150384	415143	26.14%	3.433%
21	4.646	1089	1106	1127	rBV	254807	611932	38.54%	5.060%
22	4.981	1205	1210	1211	rBV2	1554	1114	0.07%	0.009%
23	5.016	1218	1221	1223	rBV	726	446	0.03%	0.004%
24	5.064	1233	1236	1238	rBV	1113	659	0.04%	0.005%
25	5.141	1258	1260	1263	rVB	520	276	0.02%	0.002%
26	5.164	1263	1267	1271	rBV2	1252	1291	0.08%	0.011%
27	5.254	1291	1295	1298	rBV	1063	668	0.04%	0.006%
28	5.338	1298	1321	1338	rBV2	541479	1587920	100.00%	13.129%
29	5.646	1414	1417	1422	rBV	2044	2071	0.13%	0.017%
30	5.717	1436	1439	1442	rBV	1445	1019	0.06%	0.008%
31	5.836	1473	1476	1477	rBV	899	507	0.03%	0.004%
32	5.884	1478	1491	1523	rVV	507044	1036743	65.29%	8.572%
33	6.328	1615	1629	1655	rBV	362371	739045	46.54%	6.111%
34	6.701	1743	1745	1747	rBV	862	483	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032719\
 Data File : VU030500.D
 Acq On : 27 Mar 2019 21:53
 Operator : JC/SP
 Sample : K2120-09
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF5D4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

35	6.804	1775	1777	1778	rBV	504	248	0.02%	0.002%
36	6.836	1783	1787	1790	rBV	2134	1526	0.10%	0.013%
37	6.923	1812	1814	1816	rBV	896	575	0.04%	0.005%
38	6.997	1835	1837	1839	rBV2	708	309	0.02%	0.003%
39	7.016	1839	1843	1849	rBV	1858	2319	0.15%	0.019%
40	7.077	1859	1862	1865	rBV	1832	1503	0.09%	0.012%
41	7.106	1869	1871	1879	rVB2	1208	1234	0.08%	0.010%
42	7.225	1893	1908	1929	rBV	191069	359172	22.62%	2.970%
43	7.495	1989	1992	1995	rBV	1758	1413	0.09%	0.012%
44	7.563	1999	2013	2035	rBV	678202	1216343	76.60%	10.057%
45	7.849	2091	2102	2120	rBV	132262	237160	14.94%	1.961%
46	8.093	2176	2178	2184	rVB2	1418	1104	0.07%	0.009%
47	8.308	2232	2245	2282	rBV	469171	903792	56.92%	7.473%
48	8.701	2364	2367	2370	rBV	1687	1172	0.07%	0.010%
49	8.910	2429	2432	2434	rVB2	742	426	0.03%	0.004%
50	8.939	2434	2441	2445	rBV	2090	2432	0.15%	0.020%
51	8.958	2445	2447	2449	rBV	755	362	0.02%	0.003%
52	8.974	2449	2452	2454	rBV2	1212	695	0.04%	0.006%
53	9.019	2464	2466	2467	rBV	545	241	0.02%	0.002%
54	9.032	2467	2470	2475	rVV	1788	1585	0.10%	0.013%
55	9.087	2475	2487	2515	rBV	727078	1236609	77.88%	10.225%
56	9.312	2555	2557	2560	rVB	1192	630	0.04%	0.005%
57	9.389	2579	2581	2584	rBV	992	795	0.05%	0.007%
58	9.498	2612	2615	2620	rVB2	1137	901	0.06%	0.007%
59	9.533	2623	2626	2629	rBV	1701	1155	0.07%	0.010%
60	9.579	2637	2640	2641	rBV2	782	449	0.03%	0.004%
61	9.630	2650	2656	2661	rBV	1923	2009	0.13%	0.017%
62	9.717	2680	2683	2685	rBV2	1417	846	0.05%	0.007%
63	9.781	2700	2703	2706	rBV	1222	806	0.05%	0.007%
64	9.804	2706	2710	2714	rVV2	1109	1005	0.06%	0.008%
65	10.045	2782	2785	2786	rBV	1115	741	0.05%	0.006%
66	10.222	2834	2840	2846	rBV2	1866	2594	0.16%	0.021%
67	10.427	2889	2904	2923	rBV	454840	750735	47.28%	6.207%
68	10.553	2938	2943	2951	rVB	2621	3722	0.23%	0.031%
69	10.591	2951	2955	2956	rBV	2226	1327	0.08%	0.011%
70	10.717	2991	2994	3003	rBV2	1355	1988	0.13%	0.016%
71	10.775	3006	3012	3015	rBV	2101	2263	0.14%	0.019%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032719\
Data File : VU030500.D
Acq On : 27 Mar 2019 21:53
Operator : JC/SP
Sample : K2120-09
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF5D4

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0

Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Title : VOC Analysis

72	10.877	3041	3044	3046	rBV	746	475	0.03%	0.004%
73	10.958	3067	3069	3074	rVB	1329	895	0.06%	0.007%
74	11.157	3128	3131	3134	rBV	621	457	0.03%	0.004%
75	11.340	3185	3188	3191	rBV	1567	985	0.06%	0.008%
76	11.482	3220	3232	3252	rBV	588706	981217	61.79%	8.113%
77	11.855	3338	3348	3369	rBV	548079	927761	58.43%	7.671%


Sum of corrected areas: 12094317

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU032719\
Data File : VU030500.D
Acq On : 27 Mar 2019 21:53
Operator : JC/SP
Sample : K2120-09
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF5D4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

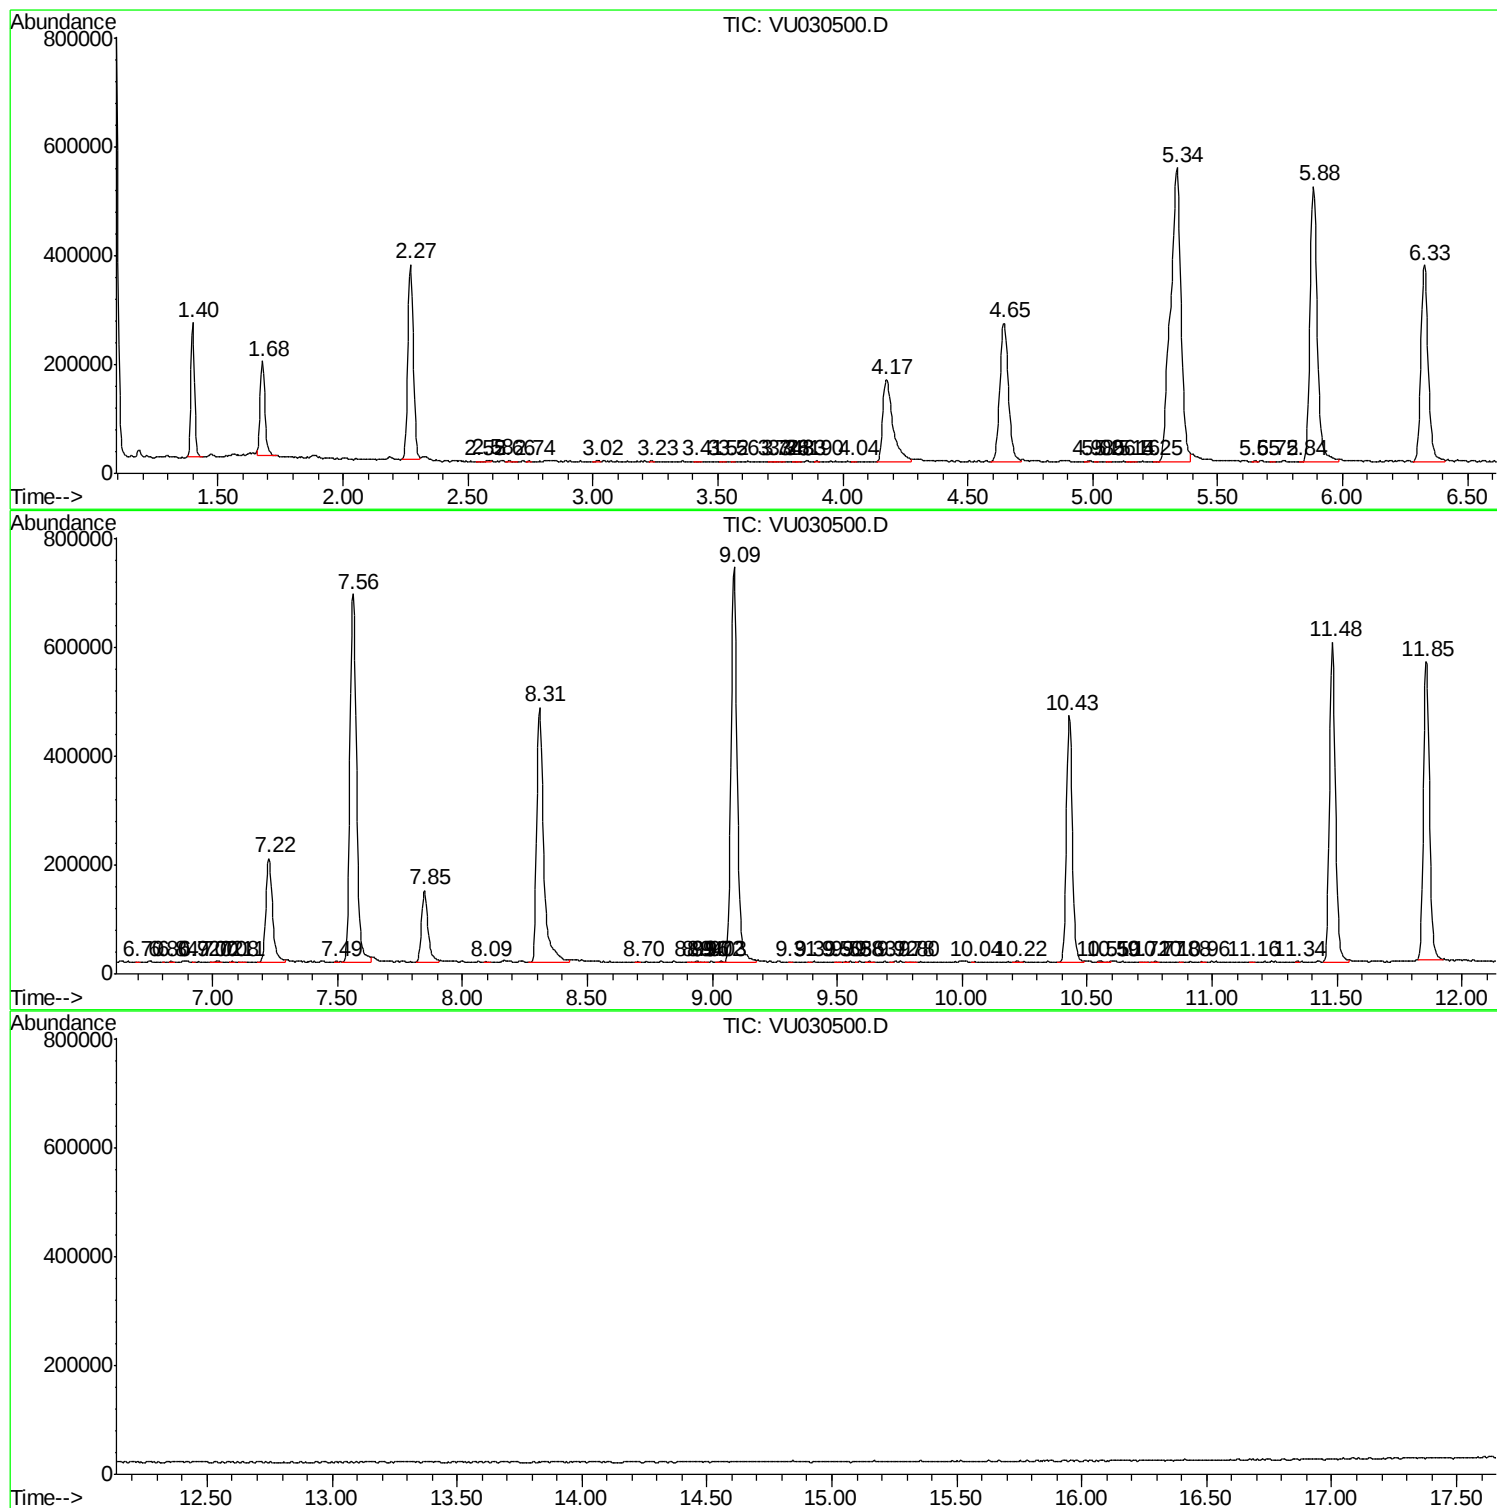

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032719\
Data File : VU030500.D
Acq On : 27 Mar 2019 21:53
Operator : JC/SP
Sample : K2120-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF5D4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU032719\
Data File : VU030500.D
Acq On : 27 Mar 2019 21:53
Operator : JC/SP
Sample : K2120-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF5D4

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc