

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032719\
 Data File : VU030501.D
 Acq On : 27 Mar 2019 22:16
 Operator : JC/SP
 Sample : K2120-10
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF5D5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.399	89	96	107	rBV	245423	245915	15.57%	2.045%
2	1.675	177	182	201	rVB	175509	234285	14.83%	1.948%
3	2.270	357	367	379	rBV	363638	554313	35.10%	4.609%
4	2.936	571	574	575	rBV	1161	731	0.05%	0.006%
5	3.067	610	615	617	rBV	2509	2328	0.15%	0.019%
6	3.228	663	665	668	rBV	898	421	0.03%	0.004%
7	3.334	695	698	703	rBV	1485	1376	0.09%	0.011%
8	3.495	745	748	752	rBV	1645	1471	0.09%	0.012%
9	3.576	768	773	779	rBV	1992	3066	0.19%	0.025%
10	3.752	824	828	830	rBV	1473	1109	0.07%	0.009%
11	3.823	844	850	852	rBV	1226	1240	0.08%	0.010%
12	3.952	887	890	893	rVB	1171	719	0.05%	0.006%
13	3.977	893	898	901	rBV	1830	1671	0.11%	0.014%
14	4.003	901	906	909	rBV	838	904	0.06%	0.008%
15	4.135	943	947	948	rBV	1277	901	0.06%	0.007%
16	4.174	948	959	993	rVV	150990	429066	27.17%	3.568%
17	4.646	1091	1106	1132	rBV	248587	597946	37.86%	4.972%
18	5.003	1214	1217	1222	rBV	811	736	0.05%	0.006%
19	5.148	1259	1262	1265	rBV	1519	1023	0.06%	0.009%
20	5.193	1272	1276	1277	rBV	1192	891	0.06%	0.007%
21	5.235	1286	1289	1290	rBV	871	507	0.03%	0.004%
22	5.338	1299	1321	1351	rBV2	535546	1579349	100.00%	13.133%
23	5.884	1477	1491	1516	rBV	506543	1030537	65.25%	8.569%
24	6.231	1596	1599	1603	rVB	1676	1191	0.08%	0.010%
25	6.254	1603	1606	1608	rBV	1672	1128	0.07%	0.009%
26	6.328	1617	1629	1651	rBV2	348673	702816	44.50%	5.844%
27	6.611	1714	1717	1719	rBV	1772	1098	0.07%	0.009%
28	7.225	1894	1908	1926	rBV	188555	356742	22.59%	2.966%
29	7.563	2001	2013	2033	rBV	671529	1194065	75.60%	9.929%
30	7.849	2092	2102	2134	rBV	131648	232473	14.72%	1.933%
31	8.148	2191	2195	2198	rBV	2550	2234	0.14%	0.019%
32	8.308	2234	2245	2280	rBV	470515	900105	56.99%	7.485%
33	8.813	2399	2402	2405	rBV	1135	856	0.05%	0.007%
34	9.035	2468	2471	2474	rBV	1259	926	0.06%	0.008%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032719\
 Data File : VU030501.D
 Acq On : 27 Mar 2019 22:16
 Operator : JC/SP
 Sample : K2120-10
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF5D5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

35	9.087	2475	2487	2508	rVV	729340	1231347	77.97%	10.239%
36	9.450	2597	2600	2604	rBV	1301	1138	0.07%	0.009%
37	9.614	2648	2651	2654	rBV	1370	1099	0.07%	0.009%
38	10.215	2835	2838	2840	rBV	1807	930	0.06%	0.008%
39	10.312	2865	2868	2870	rBV	1697	1160	0.07%	0.010%
40	10.427	2893	2904	2924	rVB	452162	742036	46.98%	6.170%
41	10.948	3063	3066	3069	rBV	1534	906	0.06%	0.008%
42	11.099	3106	3113	3116	rBV	2218	2851	0.18%	0.024%
43	11.154	3128	3130	3133	rVB	1119	569	0.04%	0.005%
44	11.177	3133	3137	3139	rBV2	1530	1292	0.08%	0.011%
45	11.238	3152	3156	3158	rBV	1829	1273	0.08%	0.011%
46	11.408	3206	3209	3210	rBV2	1633	920	0.06%	0.008%
47	11.482	3220	3232	3251	rBV	596818	995459	63.03%	8.278%
48	11.855	3338	3348	3372	rVB	554741	926237	58.65%	7.702%
49	12.668	3598	3601	3603	rBV	2225	1613	0.10%	0.013%
50	13.012	3706	3708	3709	rBV	704	340	0.02%	0.003%
51	13.041	3714	3717	3721	rVB	1623	1161	0.07%	0.010%
52	13.067	3721	3725	3729	rBV2	1320	1213	0.08%	0.010%
53	13.183	3758	3761	3762	rBV	1091	686	0.04%	0.006%
54	13.311	3798	3801	3802	rBV	519	294	0.02%	0.002%
55	13.328	3802	3806	3808	rBV	1345	1099	0.07%	0.009%
56	13.363	3813	3817	3819	rBV2	1334	1119	0.07%	0.009%
57	13.456	3843	3846	3853	rBV	993	946	0.06%	0.008%
58	13.492	3855	3857	3860	rVB	935	538	0.03%	0.004%
59	13.508	3860	3862	3864	rBV	611	312	0.02%	0.003%
60	13.572	3879	3882	3884	rBV	1351	907	0.06%	0.008%
61	13.665	3906	3911	3915	rBV	1471	1575	0.10%	0.013%
62	13.713	3923	3926	3930	rBV2	1019	1015	0.06%	0.008%
63	13.755	3936	3939	3943	rVB	1432	976	0.06%	0.008%
64	13.781	3943	3947	3952	rBV2	1366	1780	0.11%	0.015%
65	13.884	3972	3979	3982	rBV2	1631	1498	0.09%	0.012%
66	13.987	4009	4011	4014	rBV	1583	1153	0.07%	0.010%
67	14.083	4037	4041	4043	rVB	900	566	0.04%	0.005%
68	14.096	4043	4045	4048	rBV	1249	734	0.05%	0.006%
69	14.157	4059	4064	4069	rBV	2071	2196	0.14%	0.018%
70	14.183	4069	4072	4075	rBV2	1440	1367	0.09%	0.011%
71	14.289	4102	4105	4107	rBV	1096	653	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032719\
Data File : VU030501.D
Acq On : 27 Mar 2019 22:16
Operator : JC/SP
Sample : K2120-10
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF5D5

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Title : VOC Analysis

72	14.334	4114	4119	4124	rVB	1936	1881	0.12%	0.016%
73	14.366	4124	4129	4133	rBV2	2245	2533	0.16%	0.021%
74	14.553	4183	4187	4190	rBV2	1551	1210	0.08%	0.010%
75	14.601	4200	4202	4204	rBV2	850	450	0.03%	0.004%
76	14.726	4235	4241	4244	rBV2	1864	1723	0.11%	0.014%
77	14.839	4273	4276	4278	rBV	1455	958	0.06%	0.008%
78	14.958	4309	4313	4314	rBV2	1518	1096	0.07%	0.009%
79	15.064	4343	4346	4348	rBV	1757	1078	0.07%	0.009%


Sum of corrected areas: 12026026

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU032719\
Data File : VU030501.D
Acq On : 27 Mar 2019 22:16
Operator : JC/SP
Sample : K2120-10
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampled :
BF5D5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

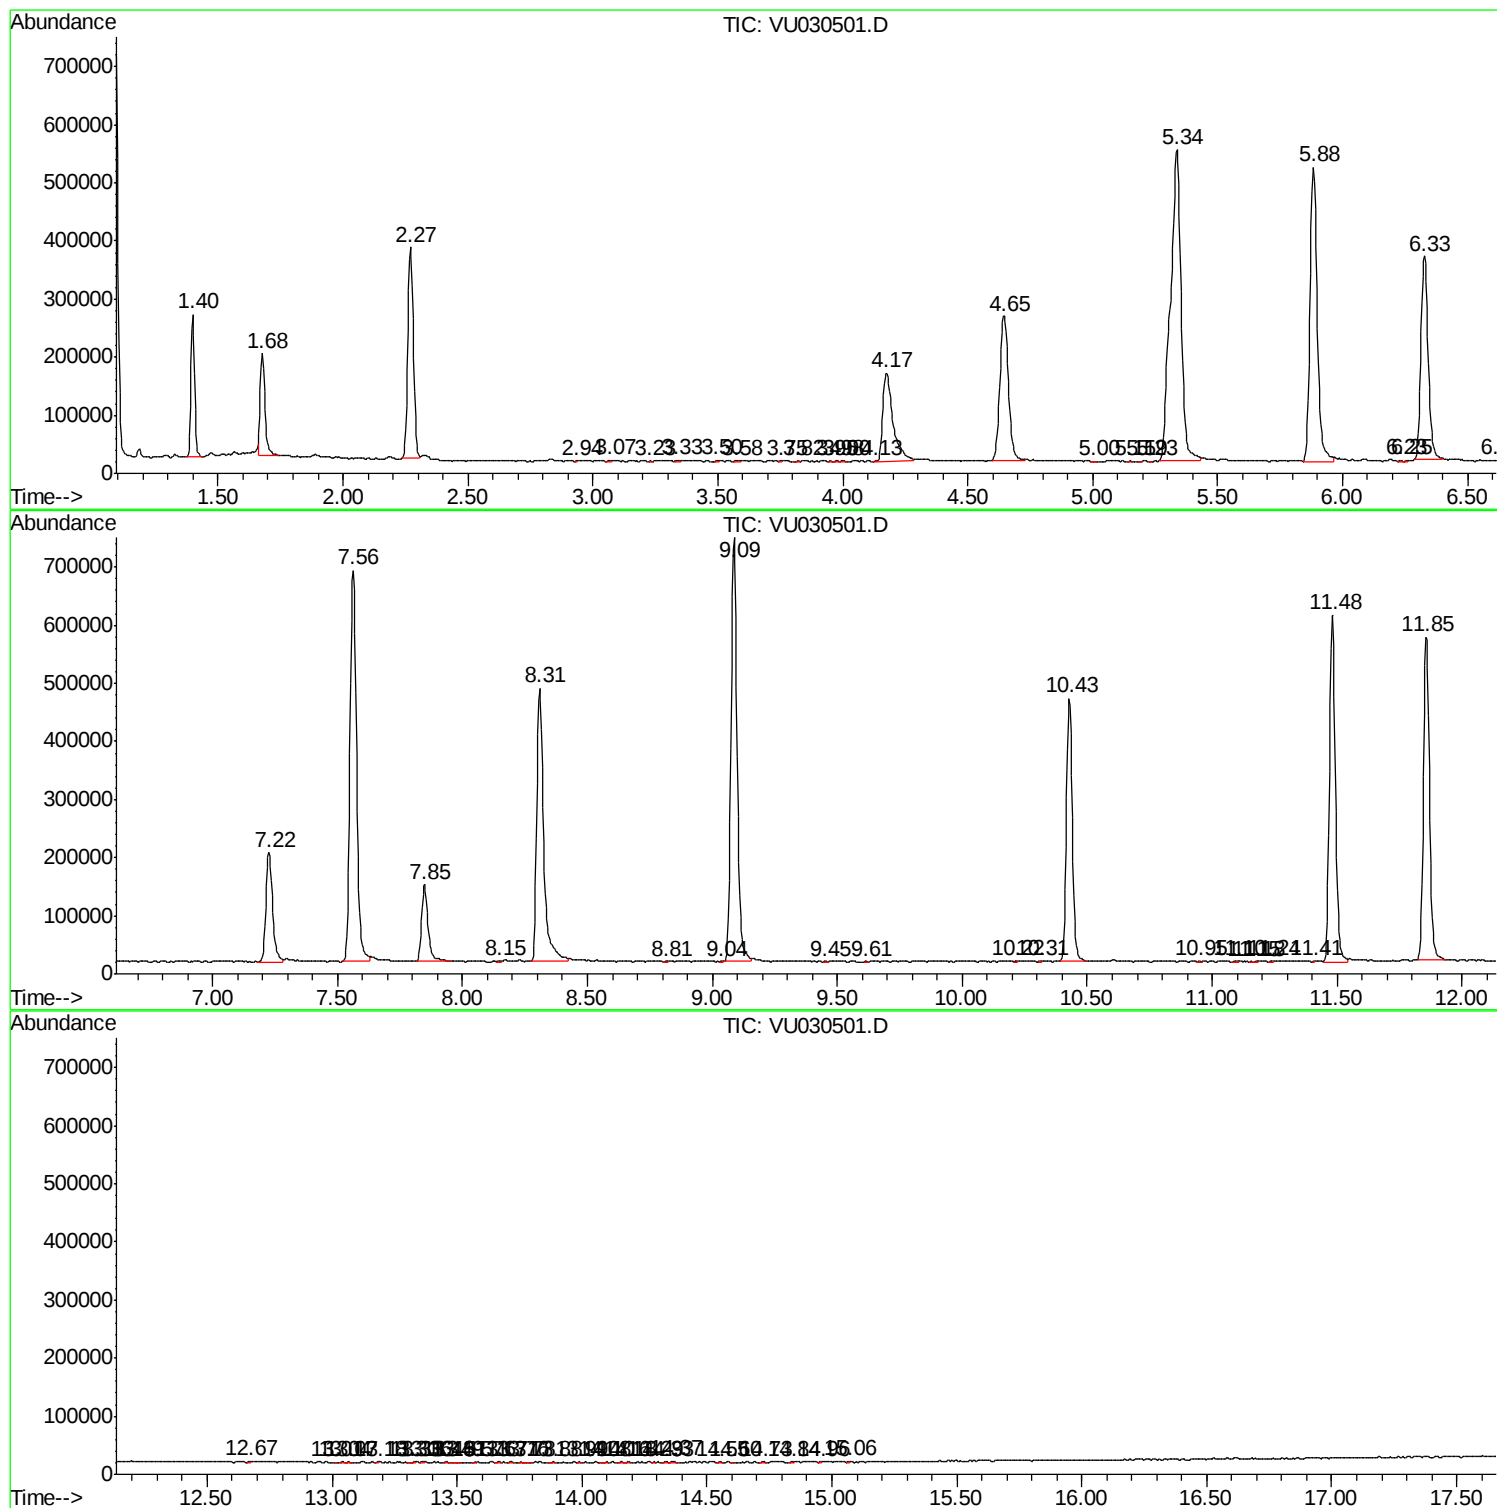

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032719\
Data File : VU030501.D
Acq On : 27 Mar 2019 22:16
Operator : JC/SP
Sample : K2120-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF5D5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU032719\
Data File : VU030501.D
Acq On : 27 Mar 2019 22:16
Operator : JC/SP
Sample : K2120-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF5D5

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc