

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032719\
 Data File : VU030504.D
 Acq On : 27 Mar 2019 23:27
 Operator : JC/SP
 Sample : K2120-13
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF5D8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.183	24	29	37	rBV3	13526	12188	0.78%	0.101%
2	1.399	89	96	107	rBV	242509	246022	15.67%	2.044%
3	1.678	175	183	197	rVB	168936	229596	14.63%	1.907%
4	2.270	357	367	379	rBV	365554	546088	34.79%	4.536%
5	2.614	469	474	478	rBV	1586	1647	0.10%	0.014%
6	2.755	513	518	521	rBV	1778	1693	0.11%	0.014%
7	2.817	534	537	543	rBV2	1396	1526	0.10%	0.013%
8	3.093	619	623	626	rBV	1417	1496	0.10%	0.012%
9	3.238	663	668	671	rBV	1275	1198	0.08%	0.010%
10	3.302	683	688	691	rBV	1056	1042	0.07%	0.009%
11	3.334	693	698	701	rVV	1628	1535	0.10%	0.013%
12	3.353	701	704	709	rVV	1426	1206	0.08%	0.010%
13	3.379	709	712	716	rVB2	1165	1024	0.07%	0.009%
14	3.408	716	721	726	rBV	1214	1121	0.07%	0.009%
15	3.492	743	747	750	rBV	1145	1089	0.07%	0.009%
16	3.630	787	790	796	rVB	1468	1065	0.07%	0.009%
17	3.910	871	877	883	rVB2	1287	1719	0.11%	0.014%
18	3.955	887	891	896	rBV	1190	1457	0.09%	0.012%
19	4.025	910	913	919	rVB	1416	1155	0.07%	0.010%
20	4.173	948	959	991	rVV	148085	401490	25.58%	3.335%
21	4.643	1087	1105	1127	rBV	253125	600510	38.26%	4.988%
22	4.820	1156	1160	1166	rVB	1441	1519	0.10%	0.013%
23	4.968	1202	1206	1210	rBV	1851	1531	0.10%	0.013%
24	5.125	1253	1255	1259	rVB	1735	1037	0.07%	0.009%
25	5.154	1259	1264	1267	rBV	1020	1197	0.08%	0.010%
26	5.209	1277	1281	1284	rBV	1630	1359	0.09%	0.011%
27	5.337	1298	1321	1350	rBV2	528508	1569568	100.00%	13.038%
28	5.884	1476	1491	1516	rBV	501211	1019158	64.93%	8.466%
29	6.205	1586	1591	1593	rBV	1230	1122	0.07%	0.009%
30	6.328	1613	1629	1656	rBV	358650	735642	46.87%	6.111%
31	6.807	1774	1778	1781	rBV	1418	1139	0.07%	0.009%
32	6.993	1833	1836	1840	rVB	2109	1555	0.10%	0.013%
33	7.157	1883	1887	1894	rBV3	1511	1587	0.10%	0.013%
34	7.225	1894	1908	1928	rBV	190062	352424	22.45%	2.928%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032719\
 Data File : VU030504.D
 Acq On : 27 Mar 2019 23:27
 Operator : JC/SP
 Sample : K2120-13
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF5D8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

35	7.424	1967	1970	1975	rBV	1456	1511	0.10%	0.013%
36	7.514	1994	1998	2000	rBV	1486	1052	0.07%	0.009%
37	7.562	2000	2013	2034	rBV	675278	1199384	76.41%	9.963%
38	7.848	2091	2102	2119	rBV	129621	233597	14.88%	1.940%
39	7.984	2141	2144	2149	rBV	1731	1667	0.11%	0.014%
40	8.128	2185	2189	2192	rBV	1487	1177	0.07%	0.010%
41	8.308	2234	2245	2276	rBV	470956	895013	57.02%	7.435%
42	8.652	2349	2352	2355	rBV	1436	1149	0.07%	0.010%
43	8.958	2444	2447	2451	rVB	1624	1179	0.08%	0.010%
44	8.990	2451	2457	2459	rBV	1022	1120	0.07%	0.009%
45	9.086	2474	2487	2509	rBV	727637	1231474	78.46%	10.230%
46	9.324	2558	2561	2565	rBV	1667	1417	0.09%	0.012%
47	9.485	2608	2611	2614	rVB	1813	1100	0.07%	0.009%
48	9.652	2660	2663	2670	rBV2	1018	1070	0.07%	0.009%
49	9.861	2724	2728	2736	rBV	1660	2403	0.15%	0.020%
50	10.022	2774	2778	2780	rBV2	1479	1230	0.08%	0.010%
51	10.073	2790	2794	2801	rBV	1746	2089	0.13%	0.017%
52	10.205	2833	2835	2841	rVB2	1115	1037	0.07%	0.009%
53	10.318	2865	2870	2872	rBV	1222	1054	0.07%	0.009%
54	10.337	2872	2876	2879	rVB	1456	1078	0.07%	0.009%
55	10.427	2893	2904	2926	rVV	456827	740896	47.20%	6.155%
56	10.707	2987	2991	2993	rBV	1710	1097	0.07%	0.009%
57	10.781	3010	3014	3020	rVB2	1519	1400	0.09%	0.012%
58	10.974	3069	3074	3077	rBV	1177	1374	0.09%	0.011%
59	11.051	3094	3098	3101	rBV2	1223	1199	0.08%	0.010%
60	11.318	3178	3181	3189	rVB	1597	1614	0.10%	0.013%
61	11.360	3189	3194	3201	rBV	1819	2433	0.16%	0.020%
62	11.424	3211	3214	3220	rBB	1028	1024	0.07%	0.009%
63	11.482	3220	3232	3256	rBV	593553	982301	62.58%	8.160%
64	11.636	3276	3280	3281	rBV2	1630	1102	0.07%	0.009%
65	11.855	3337	3348	3372	rVV	538242	923071	58.81%	7.668%
66	12.102	3421	3425	3427	rBV4	1418	1215	0.08%	0.010%
67	12.160	3438	3443	3448	rBV	1540	1606	0.10%	0.013%
68	12.543	3559	3562	3568	rVB	1934	1541	0.10%	0.013%
69	12.569	3568	3570	3574	rBV	1507	1127	0.07%	0.009%
70	12.758	3625	3629	3637	rVV2	1431	2018	0.13%	0.017%
71	12.893	3667	3671	3676	rVB2	1602	1463	0.09%	0.012%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032719\
 Data File : VU030504.D
 Acq On : 27 Mar 2019 23:27
 Operator : JC/SP
 Sample : K2120-13
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF5D8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

72	13.067	3720	3725	3730	rVV2	1672	1754	0.11%	0.015%
73	13.096	3730	3734	3738	rVB	1492	1172	0.07%	0.010%
74	13.141	3743	3748	3751	rBV	1539	1421	0.09%	0.012%
75	13.186	3759	3762	3767	rBV2	1219	1235	0.08%	0.010%
76	13.433	3837	3839	3848	rVB	1687	1815	0.12%	0.015%
77	13.482	3848	3854	3855	rBV	1176	1122	0.07%	0.009%
78	13.524	3863	3867	3870	rVB	1870	1376	0.09%	0.011%
79	13.569	3875	3881	3884	rVB2	1549	1528	0.10%	0.013%
80	13.588	3884	3887	3890	rBV	1213	1011	0.06%	0.008%
81	13.665	3907	3911	3916	rBV2	1465	1416	0.09%	0.012%
82	13.729	3925	3931	3935	rBV2	1009	1454	0.09%	0.012%
83	13.806	3952	3955	3961	rBV2	1173	1078	0.07%	0.009%
84	13.983	4006	4010	4022	rVB2	1714	2587	0.16%	0.021%
85	14.102	4044	4047	4051	rVB	1208	1010	0.06%	0.008%
86	14.128	4051	4055	4064	rVB3	1315	1778	0.11%	0.015%
87	14.176	4064	4070	4073	rBV2	1238	1242	0.08%	0.010%
88	14.324	4113	4116	4121	rVB2	1659	1469	0.09%	0.012%
89	14.369	4121	4130	4134	rBV2	2017	2712	0.17%	0.023%
90	14.395	4134	4138	4142	rVV2	1392	1511	0.10%	0.013%
91	14.742	4242	4246	4249	rVV2	1248	1200	0.08%	0.010%
92	14.768	4252	4254	4260	rVB2	1470	1409	0.09%	0.012%
93	14.835	4272	4275	4278	rBV	1521	1111	0.07%	0.009%
94	14.896	4287	4294	4299	rBV3	1644	2400	0.15%	0.020%
95	14.961	4309	4314	4317	rVB2	1388	1160	0.07%	0.010%
96	15.019	4328	4332	4335	rBV	1411	1112	0.07%	0.009%
97	15.150	4367	4373	4379	rBV2	2277	3432	0.22%	0.029%
98	15.240	4398	4401	4408	rVB2	1301	1534	0.10%	0.013%
99	15.282	4408	4414	4421	rBV2	1899	2715	0.17%	0.023%
100	15.472	4470	4473	4476	rBV3	1636	1309	0.08%	0.011%


Sum of corrected areas: 12038060

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU032719\
Data File : VU030504.D
Acq On : 27 Mar 2019 23:27
Operator : JC/SP
Sample : K2120-13
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampled :
BF5D8

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

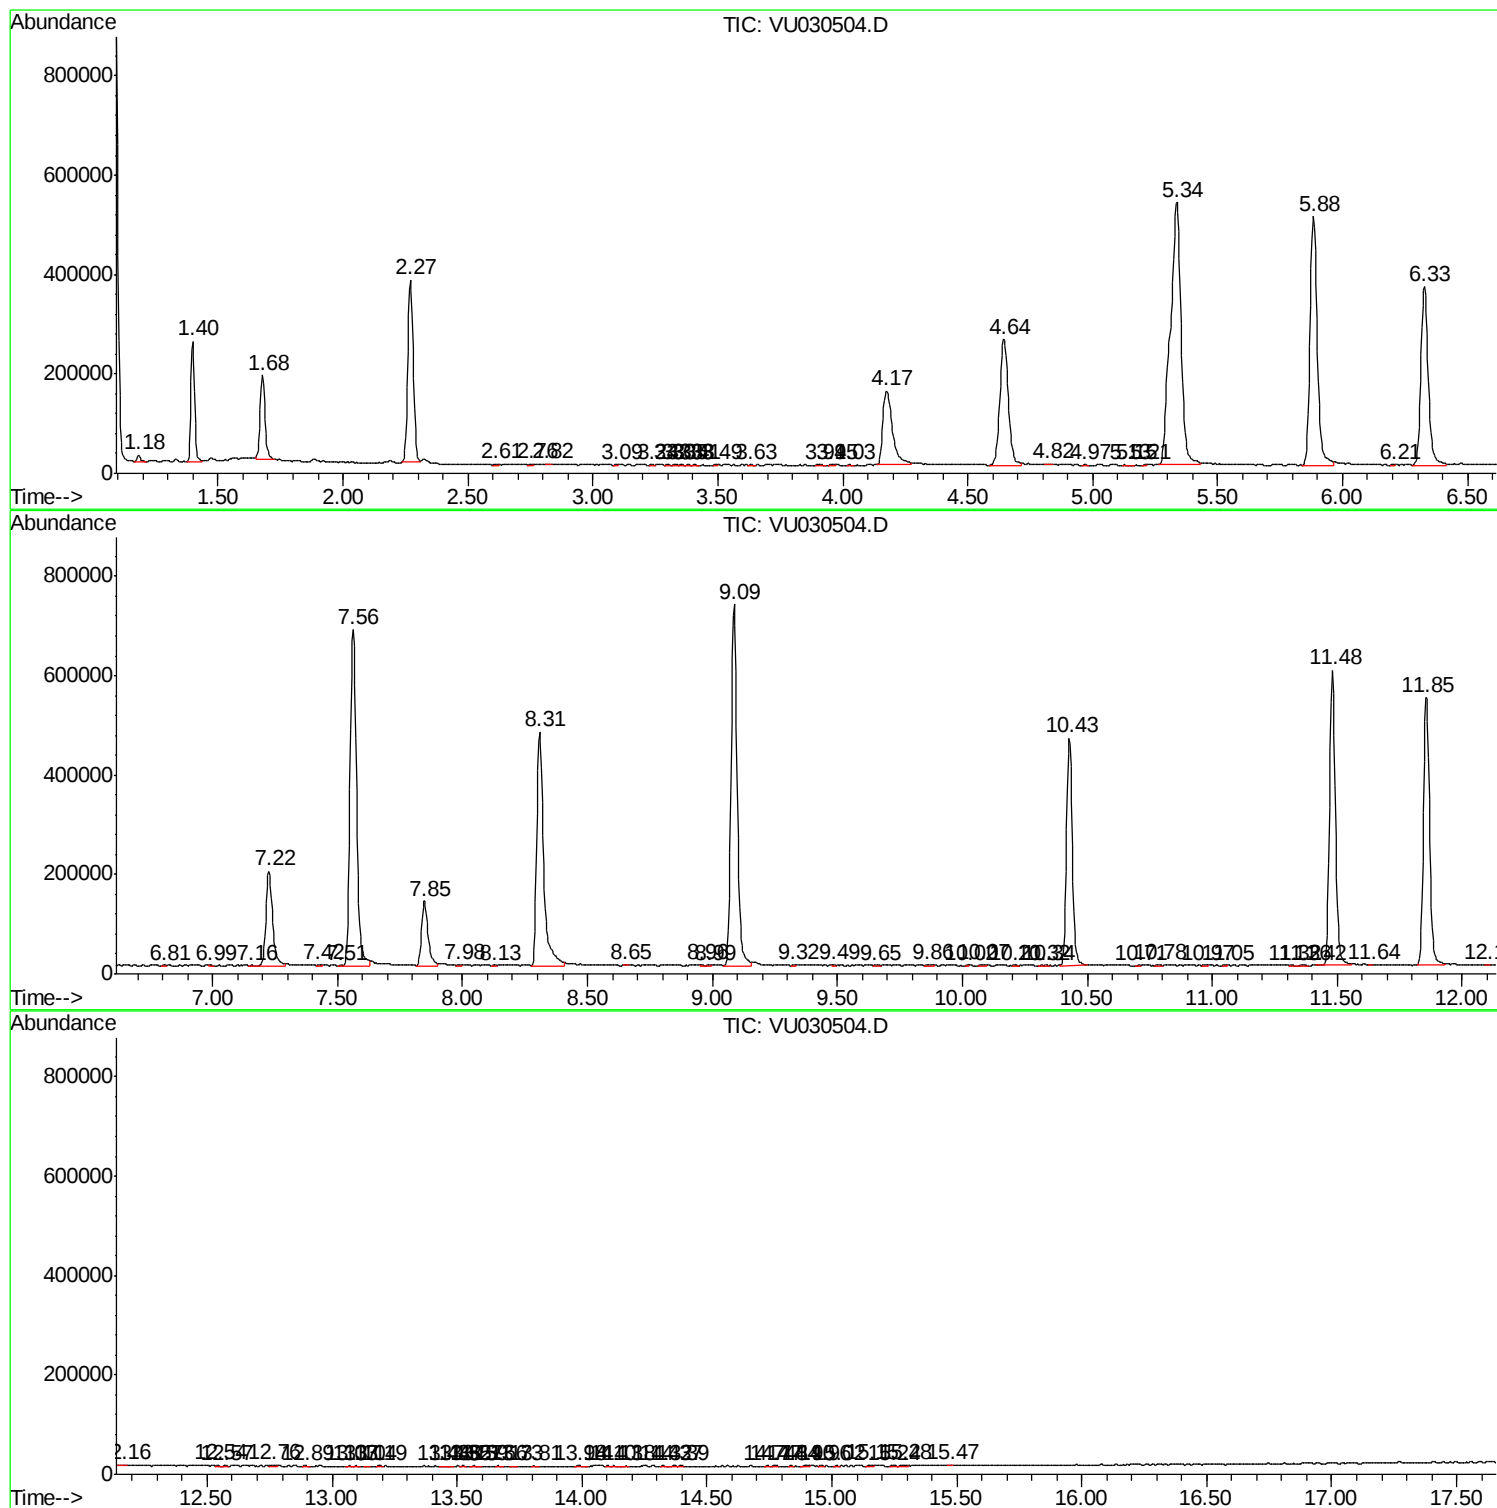

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032719\
Data File : VU030504.D
Acq On : 27 Mar 2019 23:27
Operator : JC/SP
Sample : K2120-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF5D8

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032719\
Data File : VU030504.D
Acq On : 27 Mar 2019 23:27
Operator : JC/SP
Sample : K2120-13
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF5D8

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc