

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032719\
 Data File : VU030505.D
 Acq On : 27 Mar 2019 23:50
 Operator : JC/SP
 Sample : K2120-14
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF5D9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.183	25	29	37	rVB2	13028	12953	0.83%	0.108%
2	1.399	89	96	109	rBV	247394	244841	15.62%	2.045%
3	1.678	175	183	198	rVB	172148	228731	14.60%	1.910%
4	2.270	357	367	379	rBV	354304	537348	34.29%	4.488%
5	2.428	414	416	420	rBV	1223	990	0.06%	0.008%
6	2.473	426	430	433	rBV2	1716	1507	0.10%	0.013%
7	2.627	475	478	480	rBV	1339	897	0.06%	0.007%
8	2.659	485	488	491	rBV2	1319	853	0.05%	0.007%
9	4.177	948	960	991	rBV	147475	416615	26.59%	3.480%
10	4.643	1090	1105	1126	rBV	248996	588513	37.56%	4.915%
11	5.337	1299	1321	1355	rBV2	529954	1567051	100.00%	13.088%
12	5.701	1431	1434	1437	rVB	1441	897	0.06%	0.007%
13	5.772	1448	1456	1461	rBV3	1578	1958	0.12%	0.016%
14	5.813	1464	1469	1474	rBV	1204	1233	0.08%	0.010%
15	5.884	1477	1491	1517	rBV	504144	1025048	65.41%	8.561%
16	6.328	1615	1629	1656	rBV	345294	714782	45.61%	5.970%
17	6.508	1681	1685	1688	rBV4	1462	1384	0.09%	0.012%
18	6.794	1771	1774	1778	rVB	1458	1091	0.07%	0.009%
19	6.945	1815	1821	1824	rVB3	952	928	0.06%	0.008%
20	7.173	1886	1892	1895	rVB2	1099	1146	0.07%	0.010%
21	7.225	1895	1908	1930	rBV	186709	346613	22.12%	2.895%
22	7.344	1943	1945	1953	rVB2	1564	1788	0.11%	0.015%
23	7.382	1954	1957	1967	rBV	1243	1434	0.09%	0.012%
24	7.562	1997	2013	2035	rBV	668376	1195627	76.30%	9.986%
25	7.849	2092	2102	2127	rBV	126504	228253	14.57%	1.906%
26	7.971	2137	2140	2148	rVB3	1896	1658	0.11%	0.014%
27	8.093	2174	2178	2183	rBV2	1074	1383	0.09%	0.012%
28	8.173	2196	2203	2212	rVB4	2744	4827	0.31%	0.040%
29	8.234	2212	2222	2226	rBV6	2263	3270	0.21%	0.027%
30	8.308	2230	2245	2279	rBV	463243	894774	57.10%	7.473%
31	8.649	2345	2351	2355	rBV4	1017	1426	0.09%	0.012%
32	8.742	2376	2380	2383	rBV	1176	1006	0.06%	0.008%
33	8.797	2394	2397	2400	rBV	1688	1127	0.07%	0.009%
34	8.974	2449	2452	2458	rVB2	895	921	0.06%	0.008%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032719\
 Data File : VU030505.D
 Acq On : 27 Mar 2019 23:50
 Operator : JC/SP
 Sample : K2120-14
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF5D9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

35	9.009	2458	2463	2466	rBV	954	1070	0.07%	0.009%
36	9.086	2475	2487	2526	rVV	719864	1229099	78.43%	10.266%
37	9.241	2534	2535	2540	rVB2	1825	987	0.06%	0.008%
38	9.270	2540	2544	2546	rBV2	1103	904	0.06%	0.008%
39	9.312	2554	2557	2562	rVB3	1285	1037	0.07%	0.009%
40	9.382	2575	2579	2582	rVV3	1026	901	0.06%	0.008%
41	9.463	2600	2604	2608	rBV	1127	970	0.06%	0.008%
42	9.723	2683	2685	2690	rVB2	1141	915	0.06%	0.008%
43	9.755	2690	2695	2700	rBV2	934	1139	0.07%	0.010%
44	9.794	2702	2707	2712	rVB2	1423	1796	0.11%	0.015%
45	9.839	2717	2721	2728	rBV	1678	2070	0.13%	0.017%
46	9.887	2733	2736	2740	rVB	1567	1100	0.07%	0.009%
47	9.913	2740	2744	2746	rBV2	1297	984	0.06%	0.008%
48	10.003	2767	2772	2780	rBV4	1665	2325	0.15%	0.019%
49	10.038	2780	2783	2792	rVV3	1172	1476	0.09%	0.012%
50	10.074	2792	2794	2800	rVB2	883	858	0.05%	0.007%
51	10.109	2800	2805	2809	rBV2	1032	1331	0.08%	0.011%
52	10.186	2826	2829	2832	rBV2	1224	1078	0.07%	0.009%
53	10.228	2838	2842	2844	rBV	990	857	0.05%	0.007%
54	10.247	2845	2848	2852	rVV	1160	921	0.06%	0.008%
55	10.276	2852	2857	2862	rVV3	1567	1496	0.10%	0.012%
56	10.427	2888	2904	2931	rBV	457083	746343	47.63%	6.234%
57	10.562	2941	2946	2951	rBV3	853	1176	0.08%	0.010%
58	10.607	2953	2960	2963	rBV4	2667	3136	0.20%	0.026%
59	10.730	2991	2998	3001	rBV3	2051	2084	0.13%	0.017%
60	10.784	3011	3015	3017	rBV2	994	848	0.05%	0.007%
61	10.984	3073	3077	3081	rBV	1441	1419	0.09%	0.012%
62	11.048	3090	3097	3105	rBV	2013	3328	0.21%	0.028%
63	11.176	3131	3137	3143	rVB2	856	1157	0.07%	0.010%
64	11.257	3158	3162	3167	rVB2	1262	1375	0.09%	0.011%
65	11.408	3205	3209	3214	rVB2	1359	1213	0.08%	0.010%
66	11.482	3219	3232	3251	rBV	589316	972681	62.07%	8.124%
67	11.858	3337	3349	3369	rBV	543381	908888	58.00%	7.591%
68	12.189	3448	3452	3456	rBV3	1410	1302	0.08%	0.011%
69	12.324	3490	3494	3499	rBV3	1629	1516	0.10%	0.013%
70	12.623	3584	3587	3593	rVB3	1400	1432	0.09%	0.012%
71	12.771	3630	3633	3635	rBV	1322	918	0.06%	0.008%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032719\
 Data File : VU030505.D
 Acq On : 27 Mar 2019 23:50
 Operator : JC/SP
 Sample : K2120-14
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF5D9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

72	12.926	3678	3681	3684	rBV	1348	1148	0.07%	0.010%
73	12.945	3684	3687	3692	rVB	1472	1113	0.07%	0.009%
74	13.073	3723	3727	3729	rBV	1160	892	0.06%	0.007%
75	13.090	3729	3732	3735	rVV2	1318	950	0.06%	0.008%
76	13.135	3744	3746	3752	rVB	1623	1232	0.08%	0.010%
77	13.324	3801	3805	3808	rBV2	1191	1051	0.07%	0.009%
78	13.389	3821	3825	3833	rVB2	1451	1955	0.12%	0.016%
79	13.501	3855	3860	3862	rBV	1403	1227	0.08%	0.010%
80	13.617	3891	3896	3904	rBV	1214	1244	0.08%	0.010%
81	13.868	3969	3974	3977	rBV2	1609	1681	0.11%	0.014%
82	13.913	3985	3988	3992	rBV2	918	875	0.06%	0.007%
83	13.945	3992	3998	4001	rBV2	1032	1152	0.07%	0.010%
84	14.067	4033	4036	4046	rVB2	1444	2130	0.14%	0.018%
85	14.273	4090	4100	4104	rBV2	2003	3087	0.20%	0.026%
86	14.713	4234	4237	4242	rBV2	1520	1231	0.08%	0.010%
87	14.951	4306	4311	4313	rBV2	863	929	0.06%	0.008%
88	15.099	4354	4357	4359	rBV2	1346	887	0.06%	0.007%
89	15.244	4399	4402	4405	rBV3	1284	1056	0.07%	0.009%
90	15.318	4422	4425	4429	rVV2	1135	900	0.06%	0.008%
91	15.376	4440	4443	4449	rBV3	866	850	0.05%	0.007%
92	15.659	4525	4531	4534	rBV4	1360	1269	0.08%	0.011%
93	15.681	4534	4538	4541	rBV3	1424	1184	0.08%	0.010%
94	15.739	4551	4556	4558	rBV3	1098	862	0.06%	0.007%
95	15.864	4591	4595	4599	rBV2	1924	1663	0.11%	0.014%
96	15.938	4614	4618	4623	rVB4	1243	1260	0.08%	0.011%
97	15.974	4623	4629	4633	rBV4	1898	2746	0.18%	0.023%
98	16.012	4638	4641	4645	rBV3	915	931	0.06%	0.008%
99	16.083	4661	4663	4670	rVB5	1758	1503	0.10%	0.013%
100	16.112	4670	4672	4676	rBV3	1184	997	0.06%	0.008%


Sum of corrected areas: 11973008

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU032719\
Data File : VU030505.D
Acq On : 27 Mar 2019 23:50
Operator : JC/SP
Sample : K2120-14
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF5D9

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

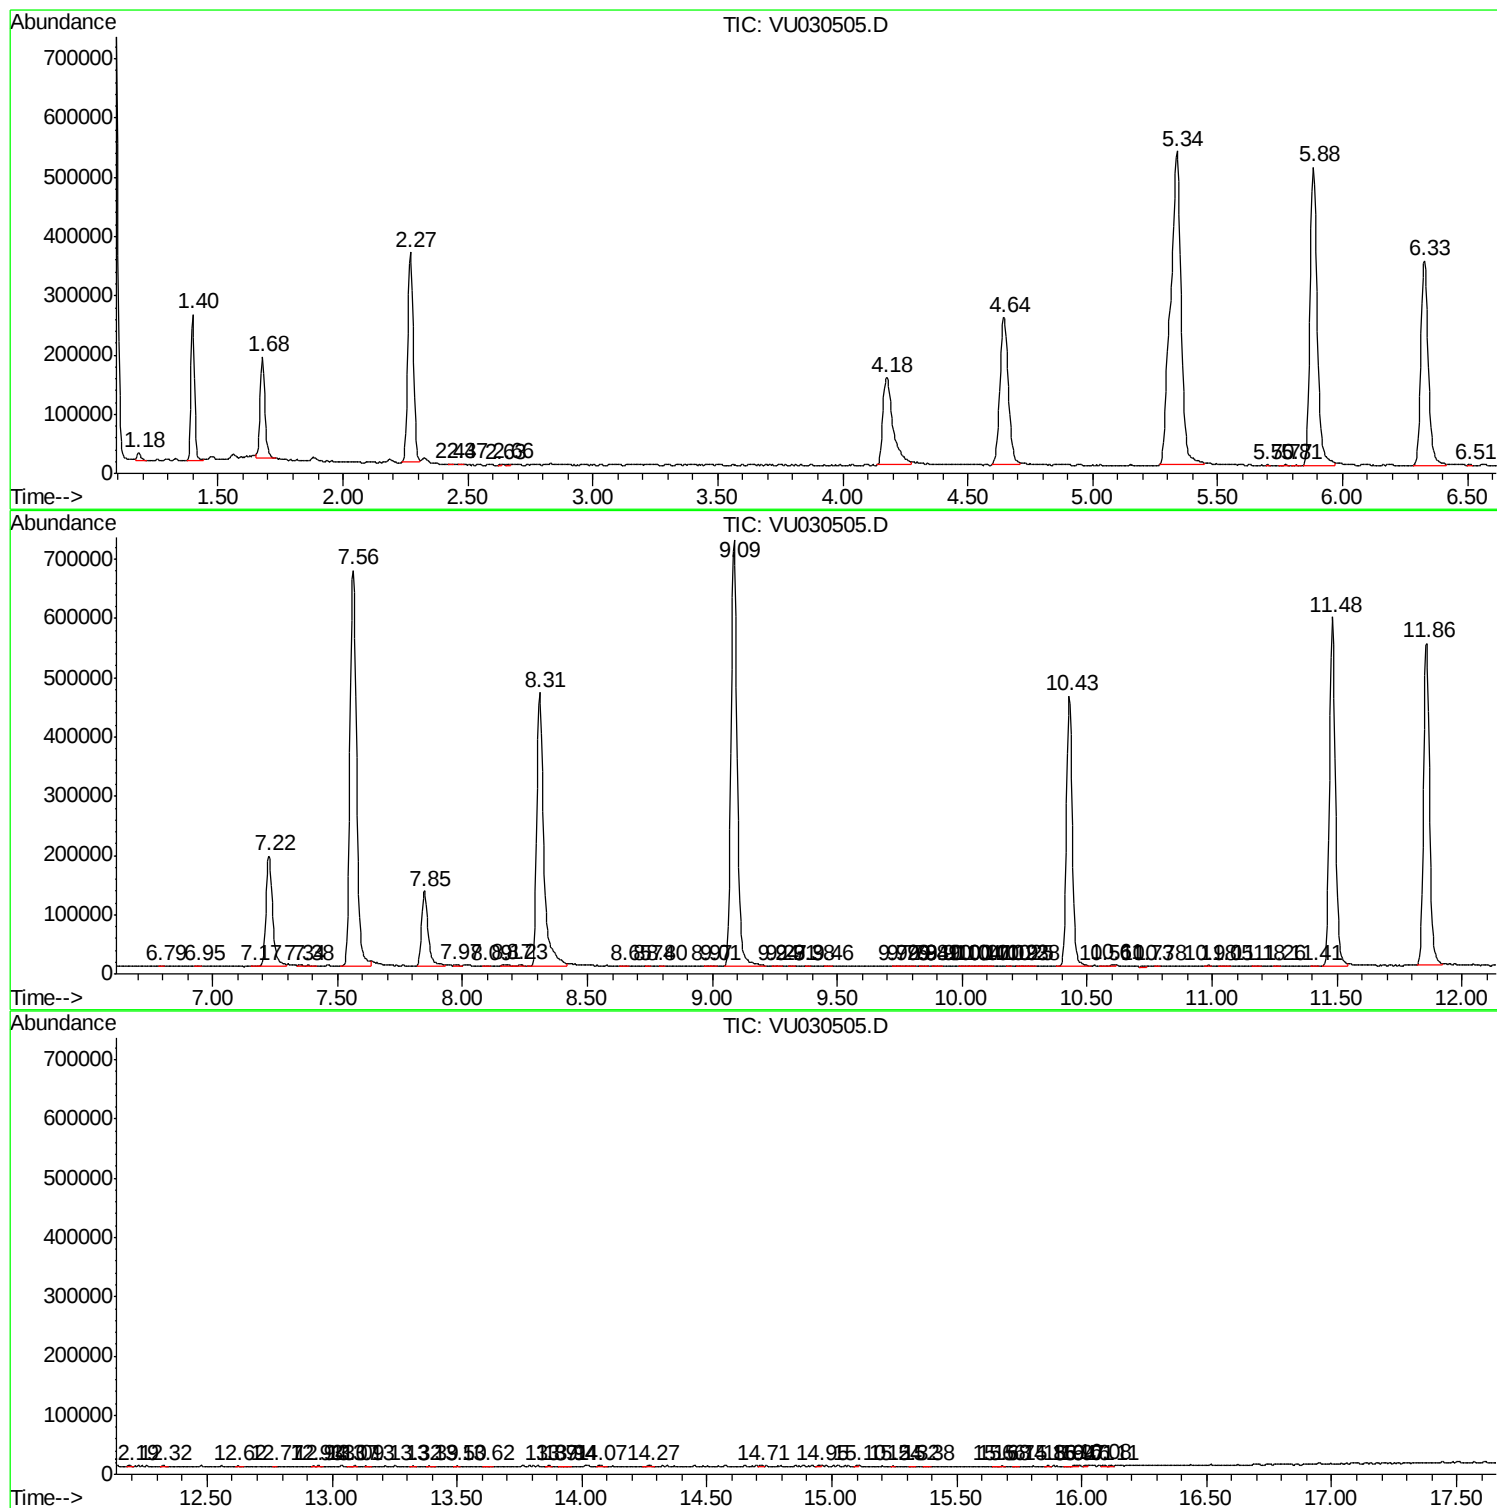

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032719\
Data File : VU030505.D
Acq On : 27 Mar 2019 23:50
Operator : JC/SP
Sample : K2120-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF5D9

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032719\
Data File : VU030505.D
Acq On : 27 Mar 2019 23:50
Operator : JC/SP
Sample : K2120-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF5D9

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc