

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032719\
 Data File : VU030507.D
 Acq On : 28 Mar 2019 00:37
 Operator : JC/SP
 Sample : K2128-11 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF1A6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.183	24	29	37	rBV3	13219	13142	0.83%	0.110%
2	1.399	89	96	106	rBV	235095	237589	14.97%	1.980%
3	1.675	175	182	200	rVB	175988	235916	14.87%	1.966%
4	2.270	356	367	380	rBV	360097	547791	34.52%	4.564%
5	2.434	414	418	420	rBV4	1619	1254	0.08%	0.010%
6	2.579	460	463	468	rBV	1071	988	0.06%	0.008%
7	2.727	506	509	514	rVB2	1321	1153	0.07%	0.010%
8	2.823	536	539	542	rBV2	1167	1087	0.07%	0.009%
9	2.965	579	583	586	rBV	1275	898	0.06%	0.007%
10	3.502	744	750	755	rBV2	1277	1712	0.11%	0.014%
11	3.530	756	759	763	rVV2	1144	893	0.06%	0.007%
12	3.624	784	788	789	rBV	1403	1033	0.07%	0.009%
13	3.929	879	883	887	rVB	1391	1041	0.07%	0.009%
14	3.990	899	902	905	rBV2	1024	774	0.05%	0.006%
15	4.173	948	959	991	rBV2	157401	436184	27.49%	3.634%
16	4.518	1064	1066	1073	rVB	1772	1338	0.08%	0.011%
17	4.582	1082	1086	1088	rBV2	924	796	0.05%	0.007%
18	4.643	1089	1105	1124	rBV	249952	594873	37.49%	4.957%
19	4.958	1198	1203	1208	rVB2	2305	2698	0.17%	0.022%
20	4.993	1210	1214	1216	rBV4	996	713	0.04%	0.006%
21	5.029	1221	1225	1229	rBV	1623	1585	0.10%	0.013%
22	5.119	1249	1253	1256	rBV	1277	984	0.06%	0.008%
23	5.141	1256	1260	1262	rBV2	1319	1121	0.07%	0.009%
24	5.212	1279	1282	1285	rBV	1442	1010	0.06%	0.008%
25	5.337	1297	1321	1360	rBV2	526961	1586681	100.00%	13.221%
26	5.884	1478	1491	1519	rBV	499781	1004447	63.30%	8.369%
27	6.186	1576	1585	1595	rBV4	10622	19661	1.24%	0.164%
28	6.328	1614	1629	1651	rBV	352910	721225	45.45%	6.009%
29	6.569	1698	1704	1708	rBV3	1117	1288	0.08%	0.011%
30	6.643	1723	1727	1729	rBV	999	800	0.05%	0.007%
31	6.707	1744	1747	1751	rVB	1194	936	0.06%	0.008%
32	6.730	1751	1754	1757	rBV	1001	825	0.05%	0.007%
33	6.765	1762	1765	1768	rBV	1044	717	0.05%	0.006%
34	6.807	1775	1778	1780	rBV	1211	814	0.05%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032719\
 Data File : VU030507.D
 Acq On : 28 Mar 2019 00:37
 Operator : JC/SP
 Sample : K2128-11 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF1A6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

35	6.890	1800	1804	1810	rVB	1394	1564	0.10%	0.013%
36	6.935	1810	1818	1822	rBV3	1466	2236	0.14%	0.019%
37	7.132	1873	1879	1884	rVB	1895	2535	0.16%	0.021%
38	7.161	1884	1888	1890	rBV	1052	865	0.05%	0.007%
39	7.177	1890	1893	1896	rVB2	1166	887	0.06%	0.007%
40	7.225	1896	1908	1928	rBV	185539	349701	22.04%	2.914%
41	7.562	1999	2013	2052	rVV	676721	1211299	76.34%	10.093%
42	7.849	2090	2102	2120	rBV	129516	228595	14.41%	1.905%
43	8.003	2146	2150	2154	rVB	1021	985	0.06%	0.008%
44	8.090	2172	2177	2180	rVB2	886	769	0.05%	0.006%
45	8.132	2185	2190	2192	rBV3	1107	1059	0.07%	0.009%
46	8.157	2195	2198	2202	rVB	912	643	0.04%	0.005%
47	8.206	2202	2213	2218	rBV3	1546	3248	0.20%	0.027%
48	8.260	2226	2230	2233	rBV2	1061	812	0.05%	0.007%
49	8.308	2234	2245	2287	rBV	485850	914297	57.62%	7.618%
50	8.717	2367	2372	2375	rBV2	948	924	0.06%	0.008%
51	8.768	2385	2388	2391	rBV	857	622	0.04%	0.005%
52	8.829	2400	2407	2410	rBV3	887	958	0.06%	0.008%
53	8.881	2419	2423	2429	rBV2	1672	1998	0.13%	0.017%
54	8.948	2439	2444	2446	rBV	1346	907	0.06%	0.008%
55	9.013	2461	2464	2468	rVB2	826	685	0.04%	0.006%
56	9.038	2468	2472	2474	rBV2	977	704	0.04%	0.006%
57	9.086	2474	2487	2516	rBV	716493	1211205	76.34%	10.092%
58	9.299	2549	2553	2557	rBV4	1254	1275	0.08%	0.011%
59	9.427	2590	2593	2596	rBV2	930	649	0.04%	0.005%
60	9.556	2630	2633	2637	rBV2	845	640	0.04%	0.005%
61	9.643	2657	2660	2663	rVV	1235	925	0.06%	0.008%
62	9.662	2663	2666	2671	rVB2	1115	819	0.05%	0.007%
63	9.710	2675	2681	2685	rVB2	1281	1232	0.08%	0.010%
64	9.742	2685	2691	2693	rBV3	1453	1536	0.10%	0.013%
65	9.887	2728	2736	2737	rBV	1345	1468	0.09%	0.012%
66	9.955	2754	2757	2762	rVV3	752	669	0.04%	0.006%
67	10.080	2790	2796	2799	rBV2	1395	1533	0.10%	0.013%
68	10.170	2819	2824	2828	rBV3	1335	1586	0.10%	0.013%
69	10.218	2836	2839	2844	rBV2	715	664	0.04%	0.006%
70	10.363	2882	2884	2888	rVB	1358	731	0.05%	0.006%
71	10.427	2892	2904	2923	rBV	454002	742745	46.81%	6.189%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032719\
 Data File : VU030507.D
 Acq On : 28 Mar 2019 00:37
 Operator : JC/SP
 Sample : K2128-11 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF1A6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

72	10.514	2928	2931	2934	rVB	1289	727	0.05%	0.006%
73	10.549	2940	2942	2946	rVB2	1242	933	0.06%	0.008%
74	10.572	2946	2949	2951	rBV2	977	763	0.05%	0.006%
75	10.662	2974	2977	2982	rVB2	1035	804	0.05%	0.007%
76	10.742	2996	3002	3004	rBV2	1062	1008	0.06%	0.008%
77	10.765	3007	3009	3016	rVB	947	964	0.06%	0.008%
78	10.935	3059	3062	3064	rBV	788	641	0.04%	0.005%
79	10.971	3070	3073	3077	rBV2	892	694	0.04%	0.006%
80	11.051	3095	3098	3100	rBV2	1228	806	0.05%	0.007%
81	11.135	3120	3124	3129	rBV	1298	1386	0.09%	0.012%
82	11.196	3140	3143	3150	rBV3	854	751	0.05%	0.006%
83	11.231	3150	3154	3158	rVB2	1354	988	0.06%	0.008%
84	11.418	3207	3212	3214	rBV2	1396	1218	0.08%	0.010%
85	11.482	3220	3232	3251	rBV	567358	942362	59.39%	7.852%
86	11.710	3300	3303	3308	rBV2	1057	953	0.06%	0.008%
87	11.858	3336	3349	3370	rBV	545579	913517	57.57%	7.612%
88	12.257	3470	3473	3477	rBV	1595	1211	0.08%	0.010%
89	12.331	3492	3496	3498	rBV3	1088	849	0.05%	0.007%
90	12.456	3532	3535	3538	rBV2	1370	1114	0.07%	0.009%
91	12.504	3548	3550	3553	rVB	1399	740	0.05%	0.006%
92	12.530	3554	3558	3562	rBV2	1030	1073	0.07%	0.009%
93	12.646	3587	3594	3597	rBV3	1243	1573	0.10%	0.013%
94	13.395	3824	3827	3829	rBV2	1320	889	0.06%	0.007%
95	13.475	3847	3852	3857	rBV	1366	1717	0.11%	0.014%
96	13.524	3864	3867	3873	rVB2	1137	924	0.06%	0.008%
97	13.771	3939	3944	3947	rBV2	1875	1693	0.11%	0.014%
98	13.845	3963	3967	3970	rBV3	1328	1267	0.08%	0.011%
99	14.421	4143	4146	4150	rVB	1255	947	0.06%	0.008%
100	15.710	4543	4547	4548	rBV3	1522	1214	0.08%	0.010%


Sum of corrected areas: 12001663

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU032719\
Data File : VU030507.D
Acq On : 28 Mar 2019 00:37
Operator : JC/SP
Sample : K2128-11 50X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF1A6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

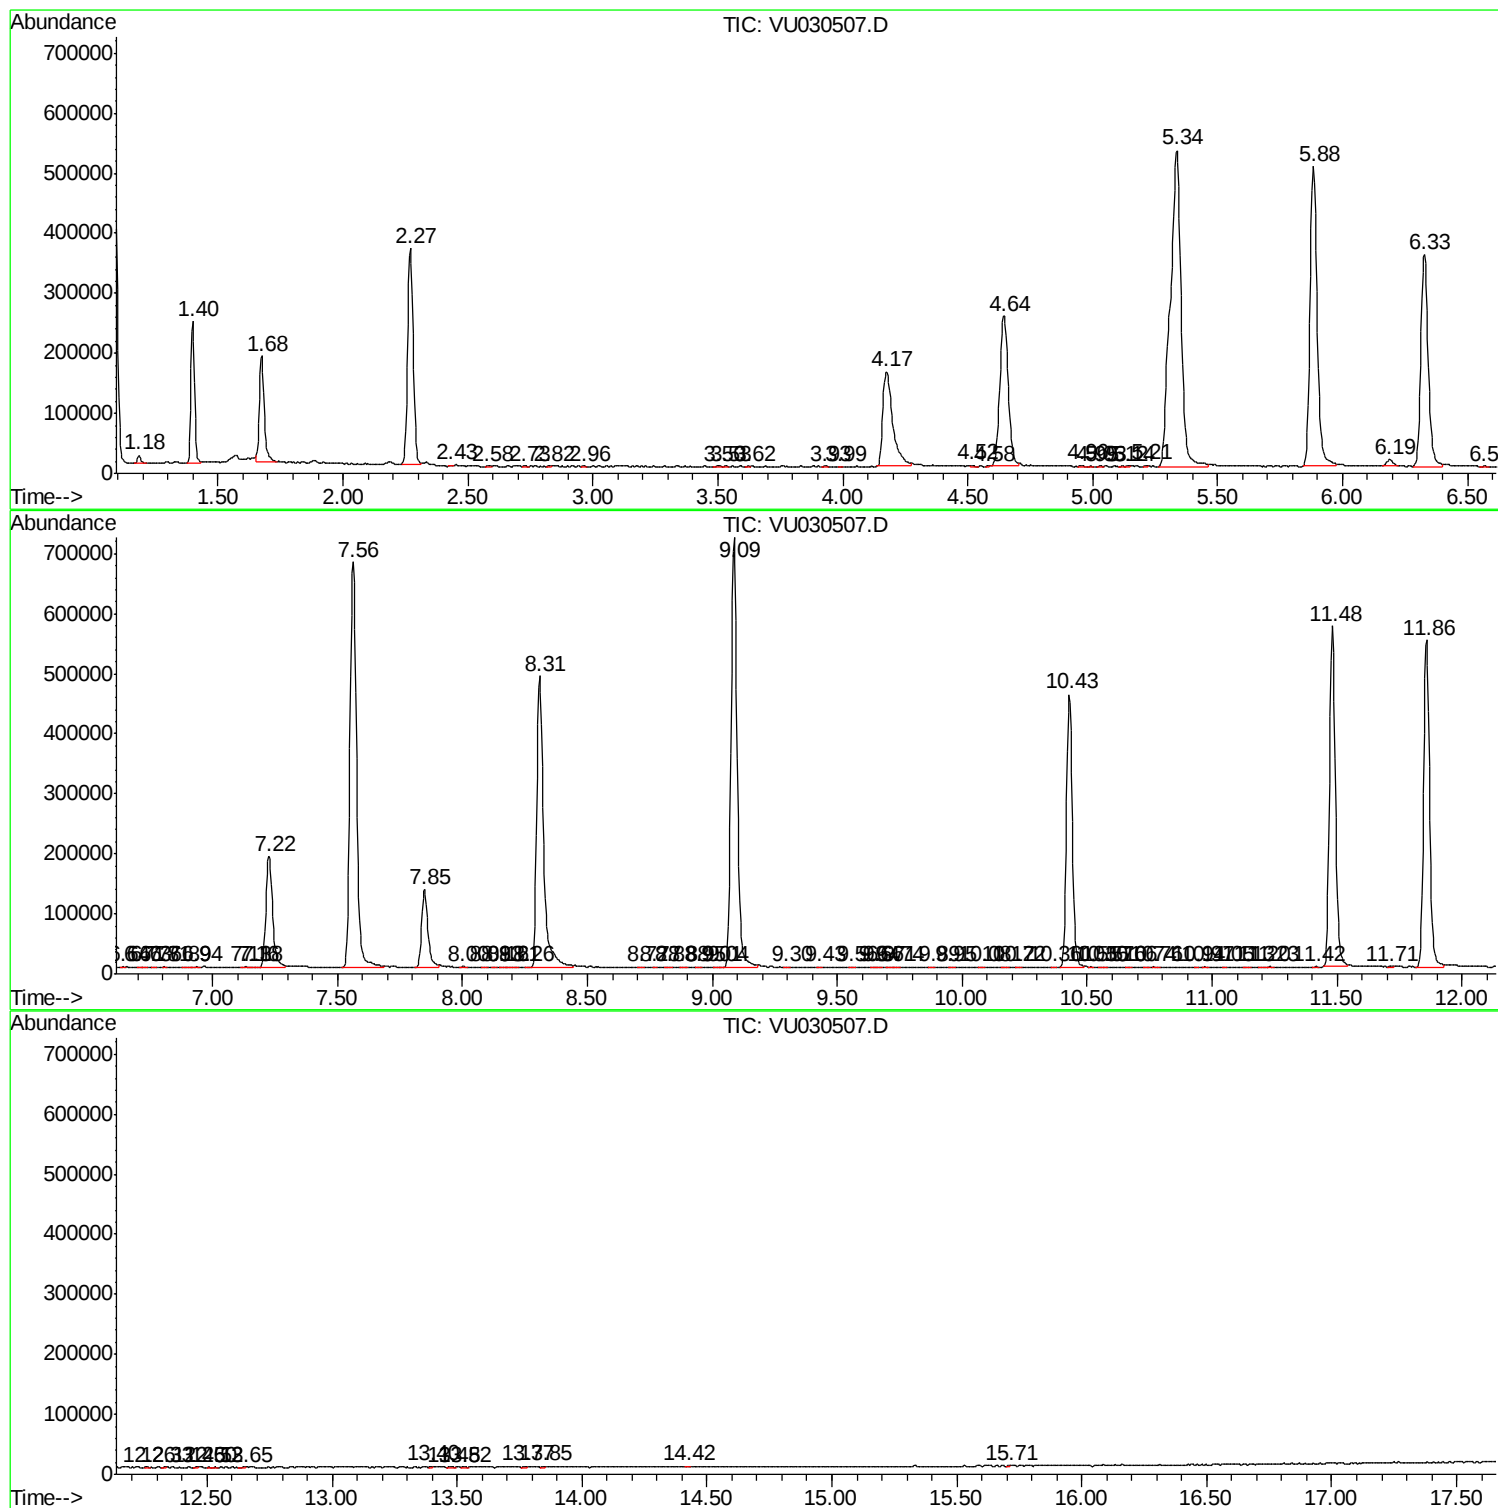

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032719\
Data File : VU030507.D
Acq On : 28 Mar 2019 00:37
Operator : JC/SP
Sample : K2128-11 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF1A6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032719\
Data File : VU030507.D
Acq On : 28 Mar 2019 00:37
Operator : JC/SP
Sample : K2128-11 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF1A6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
