

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032719\
 Data File : VU030508.D
 Acq On : 28 Mar 2019 01:01
 Operator : JC/SP
 Sample : K2128-12 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF1A7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.183	24	29	34	rBV	13380	12061	0.77%	0.100%
2	1.399	89	96	106	rBV	242131	237364	15.09%	1.971%
3	1.672	174	181	199	rVB	171038	228992	14.55%	1.901%
4	2.270	356	367	379	rBV	356125	539859	34.31%	4.482%
5	2.457	415	425	431	rBV6	2821	4759	0.30%	0.040%
6	2.521	439	445	449	rBV4	1058	1263	0.08%	0.010%
7	2.691	494	498	501	rBV2	2506	2341	0.15%	0.019%
8	3.032	601	604	609	rBV	1422	1140	0.07%	0.009%
9	3.158	637	643	646	rBV	1385	1327	0.08%	0.011%
10	3.228	661	665	672	rVB2	1028	1078	0.07%	0.009%
11	3.325	690	695	698	rVB	1387	1296	0.08%	0.011%
12	3.341	698	700	705	rBV	1134	958	0.06%	0.008%
13	3.373	705	710	712	rBV	1499	1227	0.08%	0.010%
14	3.489	742	746	749	rBV	1479	1165	0.07%	0.010%
15	3.653	792	797	799	rBV2	945	892	0.06%	0.007%
16	3.862	858	862	867	rVB2	1188	1014	0.06%	0.008%
17	3.916	872	879	880	rBV3	1321	1318	0.08%	0.011%
18	4.103	933	937	942	rBV	1117	944	0.06%	0.008%
19	4.177	947	960	990	rBV	165329	438550	27.87%	3.641%
20	4.521	1060	1067	1071	rBV	1058	1397	0.09%	0.012%
21	4.646	1088	1106	1126	rBV	255549	601882	38.25%	4.997%
22	4.952	1196	1201	1206	rVB	1228	1344	0.09%	0.011%
23	5.003	1211	1217	1220	rBV3	1606	1596	0.10%	0.013%
24	5.058	1230	1234	1240	rVB	1855	2390	0.15%	0.020%
25	5.100	1240	1247	1248	rBV	1419	1558	0.10%	0.013%
26	5.161	1259	1266	1268	rBV	1244	1475	0.09%	0.012%
27	5.193	1273	1276	1281	rVB	1468	1187	0.08%	0.010%
28	5.222	1281	1285	1287	rBV	1144	912	0.06%	0.008%
29	5.338	1292	1321	1355	rBV2	530155	1573474	100.00%	13.064%
30	5.659	1418	1421	1425	rVV2	1052	874	0.06%	0.007%
31	5.685	1426	1429	1434	rVB4	1036	847	0.05%	0.007%
32	5.884	1477	1491	1519	rBV	498326	999135	63.50%	8.295%
33	6.267	1607	1610	1612	rBV2	1138	866	0.06%	0.007%
34	6.328	1615	1629	1654	rVV	357658	725782	46.13%	6.026%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032719\
 Data File : VU030508.D
 Acq On : 28 Mar 2019 01:01
 Operator : JC/SP
 Sample : K2128-12 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF1A7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

35	6.592	1708	1711	1714	rVB	1733	1088	0.07%	0.009%
36	6.614	1714	1718	1722	rBV2	1228	1226	0.08%	0.010%
37	6.852	1786	1792	1797	rVB2	1468	1875	0.12%	0.016%
38	7.145	1877	1883	1890	rBV3	1024	1369	0.09%	0.011%
39	7.225	1894	1908	1930	rBV	187969	347273	22.07%	2.883%
40	7.411	1962	1966	1973	rVB3	1484	2007	0.13%	0.017%
41	7.453	1973	1979	1983	rBV	1532	1568	0.10%	0.013%
42	7.563	2000	2013	2034	rBV	680541	1192203	75.77%	9.898%
43	7.794	2077	2085	2087	rBV3	1076	1372	0.09%	0.011%
44	7.849	2092	2102	2123	rVV	126084	227499	14.46%	1.889%
45	8.058	2163	2167	2170	rBV	1188	904	0.06%	0.008%
46	8.093	2175	2178	2182	rVB3	1715	1395	0.09%	0.012%
47	8.128	2183	2189	2195	rBV5	1394	1687	0.11%	0.014%
48	8.231	2217	2221	2225	rBV	901	858	0.05%	0.007%
49	8.309	2234	2245	2281	rBV	506272	957005	60.82%	7.946%
50	8.546	2314	2319	2324	rBV3	1595	2251	0.14%	0.019%
51	8.604	2334	2337	2345	rVB2	1471	1569	0.10%	0.013%
52	8.913	2427	2433	2437	rBV3	1362	1173	0.07%	0.010%
53	9.087	2474	2487	2512	rBV	725310	1224523	77.82%	10.167%
54	9.460	2599	2603	2609	rBV4	1017	1180	0.07%	0.010%
55	9.543	2623	2629	2630	rBV2	1029	912	0.06%	0.008%
56	9.624	2651	2654	2657	rVB	1501	926	0.06%	0.008%
57	9.656	2657	2664	2665	rBV2	1219	1205	0.08%	0.010%
58	9.759	2689	2696	2700	rBV2	1093	1437	0.09%	0.012%
59	9.804	2706	2710	2714	rBV	1338	1411	0.09%	0.012%
60	9.887	2728	2736	2739	rBV2	1117	1541	0.10%	0.013%
61	9.926	2745	2748	2752	rVB	1466	1010	0.06%	0.008%
62	10.022	2773	2778	2783	rBV2	1341	1623	0.10%	0.013%
63	10.148	2814	2817	2821	rBV2	911	893	0.06%	0.007%
64	10.353	2875	2881	2886	rBV	1018	1364	0.09%	0.011%
65	10.427	2892	2904	2929	rVB	466530	758763	48.22%	6.300%
66	10.524	2930	2934	2938	rBV	1158	1209	0.08%	0.010%
67	10.714	2988	2993	2999	rVB2	1206	1333	0.08%	0.011%
68	10.759	2999	3007	3010	rBV3	1518	1750	0.11%	0.015%
69	10.804	3018	3021	3025	rVB	1231	937	0.06%	0.008%
70	10.955	3065	3068	3071	rVV	1284	869	0.06%	0.007%
71	10.980	3071	3076	3080	rVV2	1250	1249	0.08%	0.010%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032719\
 Data File : VU030508.D
 Acq On : 28 Mar 2019 01:01
 Operator : JC/SP
 Sample : K2128-12 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF1A7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

72	11.205	3143	3146	3151	rVB	1294	1059	0.07%	0.009%
73	11.234	3151	3155	3161	rVB2	1073	982	0.06%	0.008%
74	11.321	3179	3182	3185	rVB	1264	897	0.06%	0.007%
75	11.344	3185	3189	3192	rBV2	1386	1169	0.07%	0.010%
76	11.366	3192	3196	3200	rBV3	882	885	0.06%	0.007%
77	11.482	3220	3232	3257	rBV	575479	966642	61.43%	8.026%
78	11.797	3327	3330	3335	rBV2	1165	1059	0.07%	0.009%
79	11.858	3336	3349	3365	rBV	542394	901898	57.32%	7.488%
80	12.450	3528	3533	3538	rVV4	880	977	0.06%	0.008%
81	12.588	3571	3576	3580	rBV	1152	1310	0.08%	0.011%
82	12.736	3613	3622	3626	rBV	1819	2533	0.16%	0.021%
83	12.784	3633	3637	3641	rVB2	1090	912	0.06%	0.008%
84	12.852	3655	3658	3663	rBV	935	974	0.06%	0.008%
85	13.373	3816	3820	3824	rVB2	1438	1255	0.08%	0.010%
86	13.469	3847	3850	3854	rVB	1287	1015	0.06%	0.008%
87	13.495	3854	3858	3863	rBV2	1486	1612	0.10%	0.013%
88	13.527	3863	3868	3872	rBV3	891	858	0.05%	0.007%
89	13.620	3890	3897	3901	rBV2	1185	1604	0.10%	0.013%
90	14.064	4030	4035	4040	rBV3	1630	2045	0.13%	0.017%
91	14.189	4070	4074	4076	rBV	930	854	0.05%	0.007%
92	14.238	4085	4089	4090	rBV	1411	1011	0.06%	0.008%
93	14.405	4139	4141	4150	rVB2	1153	1400	0.09%	0.012%
94	14.607	4200	4204	4208	rBV	2070	1906	0.12%	0.016%
95	14.768	4248	4254	4259	rBV3	905	1380	0.09%	0.011%
96	15.064	4343	4346	4351	rBV	1725	1620	0.10%	0.013%
97	15.118	4357	4363	4365	rBV2	1437	1682	0.11%	0.014%
98	15.160	4371	4376	4380	rBV2	1182	1219	0.08%	0.010%
99	15.373	4439	4442	4447	rBV4	904	951	0.06%	0.008%
100	16.311	4728	4734	4737	rBV3	1888	2077	0.13%	0.017%


Sum of corrected areas: 12044510

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU032719\
Data File : VU030508.D
Acq On : 28 Mar 2019 01:01
Operator : JC/SP
Sample : K2128-12 50X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF1A7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

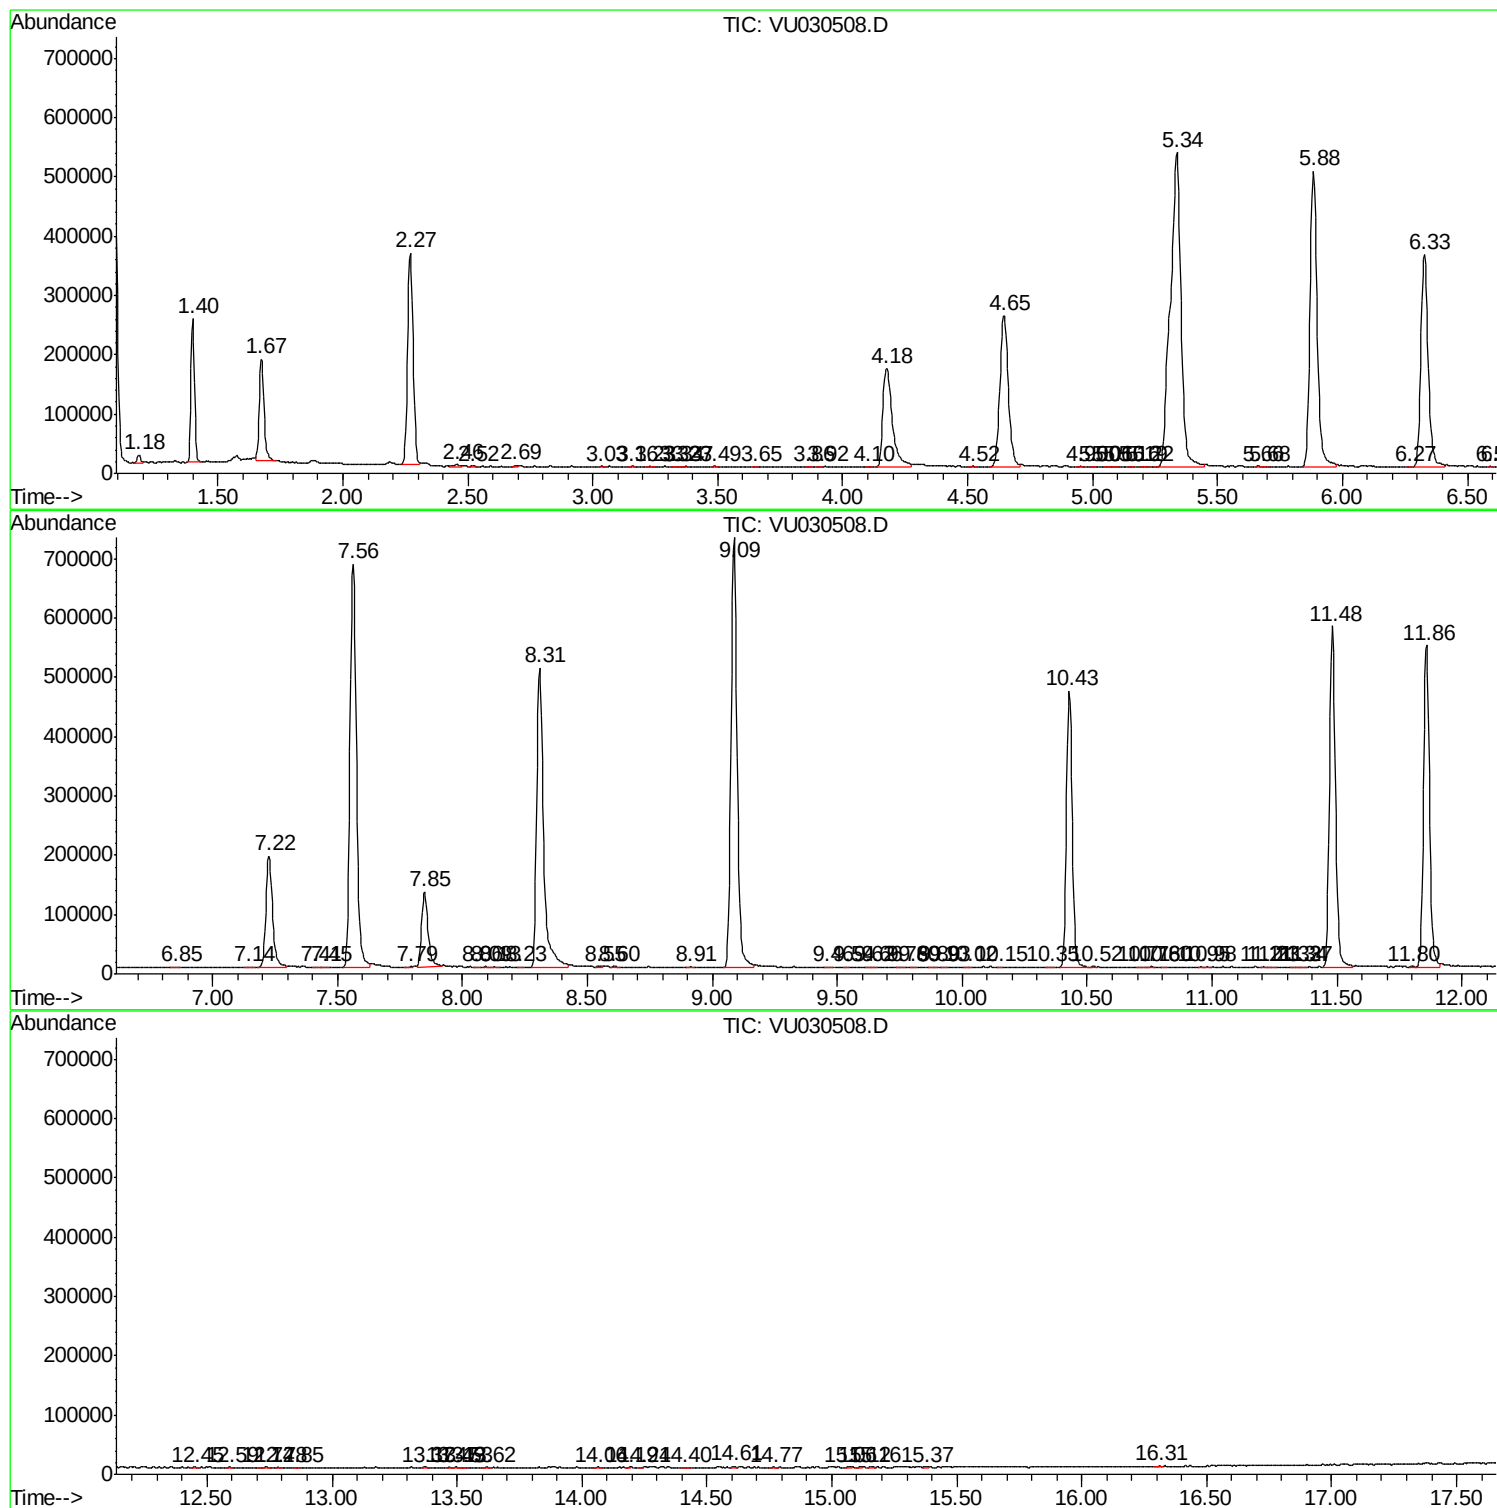

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032719\
Data File : VU030508.D
Acq On : 28 Mar 2019 01:01
Operator : JC/SP
Sample : K2128-12 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF1A7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032719\
Data File : VU030508.D
Acq On : 28 Mar 2019 01:01
Operator : JC/SP
Sample : K2128-12 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF1A7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
