

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032719\
 Data File : VU030509.D
 Acq On : 28 Mar 2019 01:24
 Operator : JC/SP
 Sample : K2128-14 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF1H2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.183	24	29	37	rVB	13038	12325	0.81%	0.106%
2	1.399	89	96	107	rBV	223585	227023	14.84%	1.952%
3	1.672	174	181	197	rVB	165118	218878	14.31%	1.882%
4	2.270	355	367	382	rBV	335850	519921	33.99%	4.470%
5	2.601	468	470	472	rBV	814	517	0.03%	0.004%
6	2.965	580	583	587	rBV2	826	584	0.04%	0.005%
7	3.083	616	620	623	rBV	906	752	0.05%	0.006%
8	3.112	627	629	632	rVV	1417	1006	0.07%	0.009%
9	3.141	636	638	642	rVB	955	531	0.03%	0.005%
10	3.209	656	659	660	rBV	1008	570	0.04%	0.005%
11	3.289	681	684	688	rVB2	925	681	0.04%	0.006%
12	3.399	712	718	723	rBV3	1671	2318	0.15%	0.020%
13	3.630	784	790	794	rBV3	847	1086	0.07%	0.009%
14	3.890	868	871	876	rVB2	560	572	0.04%	0.005%
15	4.003	903	906	908	rBV	1042	706	0.05%	0.006%
16	4.074	922	928	933	rBV2	1016	1242	0.08%	0.011%
17	4.173	948	959	993	rVV	159679	427704	27.96%	3.678%
18	4.363	1015	1018	1022	rBV	1533	1256	0.08%	0.011%
19	4.514	1062	1065	1073	rVB	831	740	0.05%	0.006%
20	4.556	1075	1078	1084	rVV	1101	965	0.06%	0.008%
21	4.643	1091	1105	1127	rBV	243187	575964	37.65%	4.952%
22	4.791	1149	1151	1154	rVB2	1305	740	0.05%	0.006%
23	4.810	1154	1157	1160	rVB2	1043	675	0.04%	0.006%
24	4.884	1177	1180	1183	rVV3	853	626	0.04%	0.005%
25	5.013	1217	1220	1224	rVB	1101	810	0.05%	0.007%
26	5.077	1236	1240	1242	rBV	993	726	0.05%	0.006%
27	5.161	1259	1266	1270	rVB3	890	1086	0.07%	0.009%
28	5.218	1279	1284	1286	rBV	814	790	0.05%	0.007%
29	5.337	1297	1321	1354	rBV2	511200	1529738	100.00%	13.153%
30	5.527	1377	1380	1383	rBV3	1334	1090	0.07%	0.009%
31	5.636	1409	1414	1417	rVB3	1242	958	0.06%	0.008%
32	5.672	1423	1425	1432	rVB3	1014	715	0.05%	0.006%
33	5.771	1453	1456	1461	rVB2	1582	1471	0.10%	0.013%
34	5.800	1461	1465	1470	rBV	1434	1387	0.09%	0.012%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032719\
 Data File : VU030509.D
 Acq On : 28 Mar 2019 01:24
 Operator : JC/SP
 Sample : K2128-14 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF1H2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

35	5.884	1477	1491	1527	rBV	480605	982655	64.24%	8.449%
36	6.058	1542	1545	1547	rBV2	755	561	0.04%	0.005%
37	6.090	1552	1555	1558	rVB	1323	946	0.06%	0.008%
38	6.170	1576	1580	1581	rBV	1203	759	0.05%	0.007%
39	6.193	1583	1587	1590	rVB2	1368	1155	0.08%	0.010%
40	6.257	1604	1607	1612	rBV2	691	507	0.03%	0.004%
41	6.328	1615	1629	1654	rBV	341306	699017	45.70%	6.010%
42	6.591	1707	1711	1715	rBV2	922	852	0.06%	0.007%
43	6.646	1723	1728	1734	rBV2	1568	1823	0.12%	0.016%
44	6.685	1734	1740	1745	rVB3	687	1070	0.07%	0.009%
45	6.733	1751	1755	1758	rBV2	709	628	0.04%	0.005%
46	6.762	1758	1764	1768	rVB	1723	2088	0.14%	0.018%
47	6.845	1785	1790	1803	rVB2	879	1984	0.13%	0.017%
48	6.903	1803	1808	1809	rBV2	907	720	0.05%	0.006%
49	6.955	1820	1824	1826	rBV	743	552	0.04%	0.005%
50	7.225	1897	1908	1930	rBV	177532	327646	21.42%	2.817%
51	7.431	1968	1972	1974	rVV	813	553	0.04%	0.005%
52	7.443	1974	1976	1981	rVV2	791	476	0.03%	0.004%
53	7.476	1981	1986	1991	rVB2	1318	1294	0.08%	0.011%
54	7.562	2000	2013	2035	rBV	632022	1127405	73.70%	9.694%
55	7.800	2083	2087	2090	rBV3	861	793	0.05%	0.007%
56	7.845	2090	2101	2122	rBV	123811	221523	14.48%	1.905%
57	8.086	2172	2176	2180	rVV3	1385	1120	0.07%	0.010%
58	8.154	2193	2197	2200	rBV3	1038	833	0.05%	0.007%
59	8.254	2225	2228	2233	rVB3	896	834	0.05%	0.007%
60	8.308	2234	2245	2279	rBV	503411	945057	61.78%	8.126%
61	8.665	2350	2356	2358	rBV3	1539	1698	0.11%	0.015%
62	8.900	2424	2429	2431	rBV3	1019	961	0.06%	0.008%
63	8.996	2454	2459	2466	rVB3	984	1286	0.08%	0.011%
64	9.086	2475	2487	2522	rBV	701842	1181632	77.24%	10.160%
65	9.344	2563	2567	2573	rBV	1740	1668	0.11%	0.014%
66	9.588	2640	2643	2645	rBV	893	620	0.04%	0.005%
67	9.678	2668	2671	2674	rVB	982	620	0.04%	0.005%
68	9.694	2674	2676	2678	rBV	967	564	0.04%	0.005%
69	9.710	2678	2681	2686	rVB	1113	1097	0.07%	0.009%
70	9.868	2726	2730	2732	rBV2	977	731	0.05%	0.006%
71	9.938	2746	2752	2756	rBV2	1057	1229	0.08%	0.011%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032719\
 Data File : VU030509.D
 Acq On : 28 Mar 2019 01:24
 Operator : JC/SP
 Sample : K2128-14 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF1H2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

72	10.006	2770	2773	2777	rBV	613	534	0.03%	0.005%
73	10.135	2810	2813	2819	rVV2	979	1143	0.07%	0.010%
74	10.212	2832	2837	2842	rBV	1097	1403	0.09%	0.012%
75	10.273	2852	2856	2858	rBV2	1112	977	0.06%	0.008%
76	10.427	2892	2904	2929	rBV	457327	743476	48.60%	6.393%
77	10.591	2952	2955	2957	rBV2	763	492	0.03%	0.004%
78	10.659	2972	2976	2979	rBV	621	626	0.04%	0.005%
79	11.109	3112	3116	3121	rBV2	1166	1419	0.09%	0.012%
80	11.299	3172	3175	3178	rVB	1418	878	0.06%	0.008%
81	11.482	3220	3232	3254	rBV	560084	933313	61.01%	8.025%
82	11.858	3337	3349	3368	rBV	517016	875303	57.22%	7.526%
83	12.090	3418	3421	3426	rBV5	1290	1519	0.10%	0.013%
84	12.321	3489	3493	3496	rBV3	1519	1563	0.10%	0.013%
85	12.376	3507	3510	3515	rVB	1108	819	0.05%	0.007%
86	12.427	3522	3526	3529	rBV	1206	1090	0.07%	0.009%
87	12.559	3563	3567	3575	rVV4	1336	1807	0.12%	0.016%
88	12.752	3623	3627	3630	rBV2	946	790	0.05%	0.007%
89	12.823	3646	3649	3654	rVV	1166	1033	0.07%	0.009%
90	12.848	3654	3657	3665	rVB	1669	1986	0.13%	0.017%
91	13.183	3758	3761	3766	rBV2	1043	1176	0.08%	0.010%
92	13.501	3857	3860	3863	rBV	1111	728	0.05%	0.006%
93	13.578	3882	3884	3889	rBV2	648	637	0.04%	0.005%
94	13.626	3896	3899	3901	rBV	1383	980	0.06%	0.008%
95	13.813	3955	3957	3961	rVB3	927	546	0.04%	0.005%
96	14.253	4091	4094	4095	rBV	967	601	0.04%	0.005%
97	14.430	4146	4149	4152	rBV2	1397	883	0.06%	0.008%
98	14.446	4152	4154	4158	rVB	1383	814	0.05%	0.007%
99	14.806	4263	4266	4268	rBV3	1107	874	0.06%	0.008%
100	15.858	4590	4593	4598	rBV5	1647	1744	0.11%	0.015%


Sum of corrected areas: 11630264

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU032719\
Data File : VU030509.D
Acq On : 28 Mar 2019 01:24
Operator : JC/SP
Sample : K2128-14 50X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF1H2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

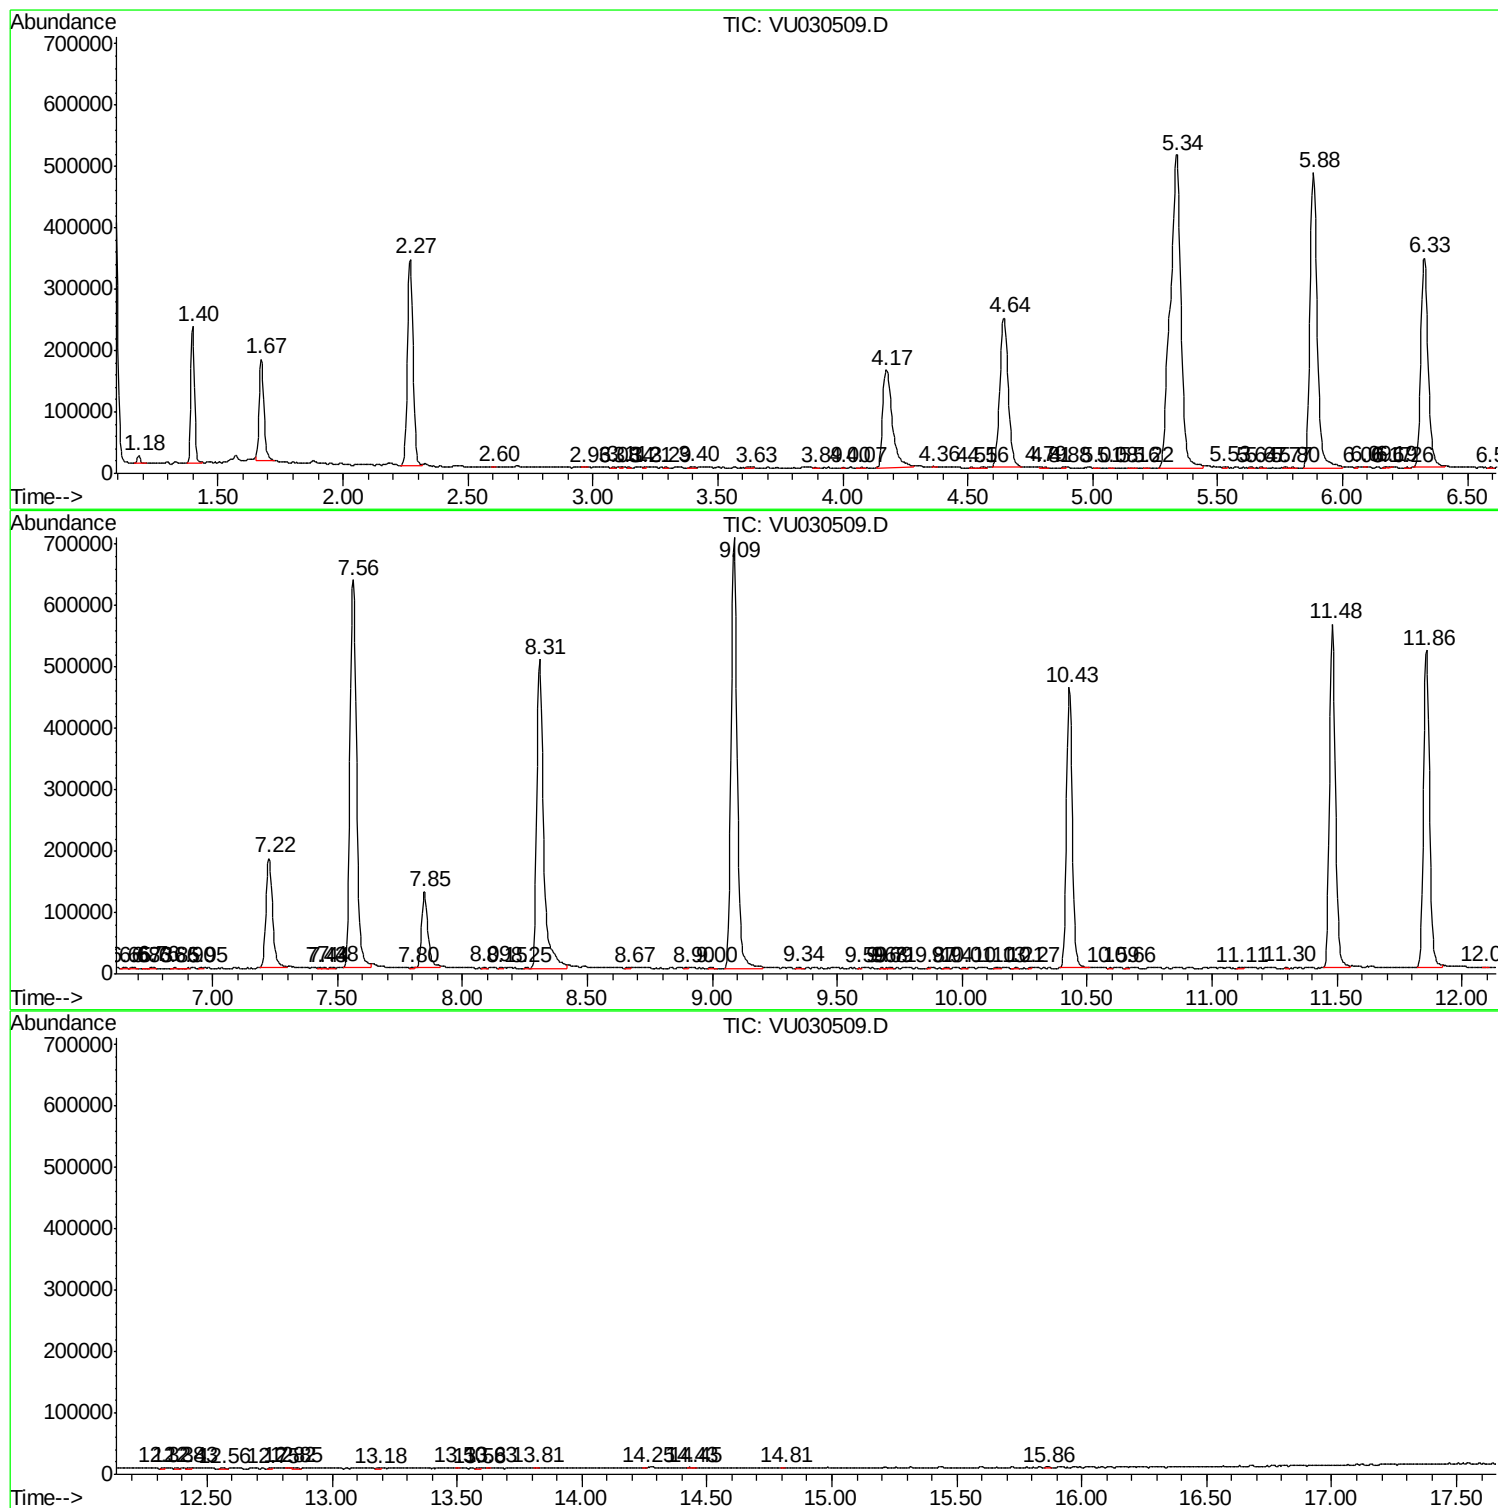

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032719\
Data File : VU030509.D
Acq On : 28 Mar 2019 01:24
Operator : JC/SP
Sample : K2128-14 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF1H2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032719\
Data File : VU030509.D
Acq On : 28 Mar 2019 01:24
Operator : JC/SP
Sample : K2128-14 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF1H2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
