


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU032719\
 Data File : VU030471.D
 Acq On : 27 Mar 2019 10:04
 Operator : JC/SP
 Sample : BFB45
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB45

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis
 Last Update : Thu Mar 28 02:45:06 2019

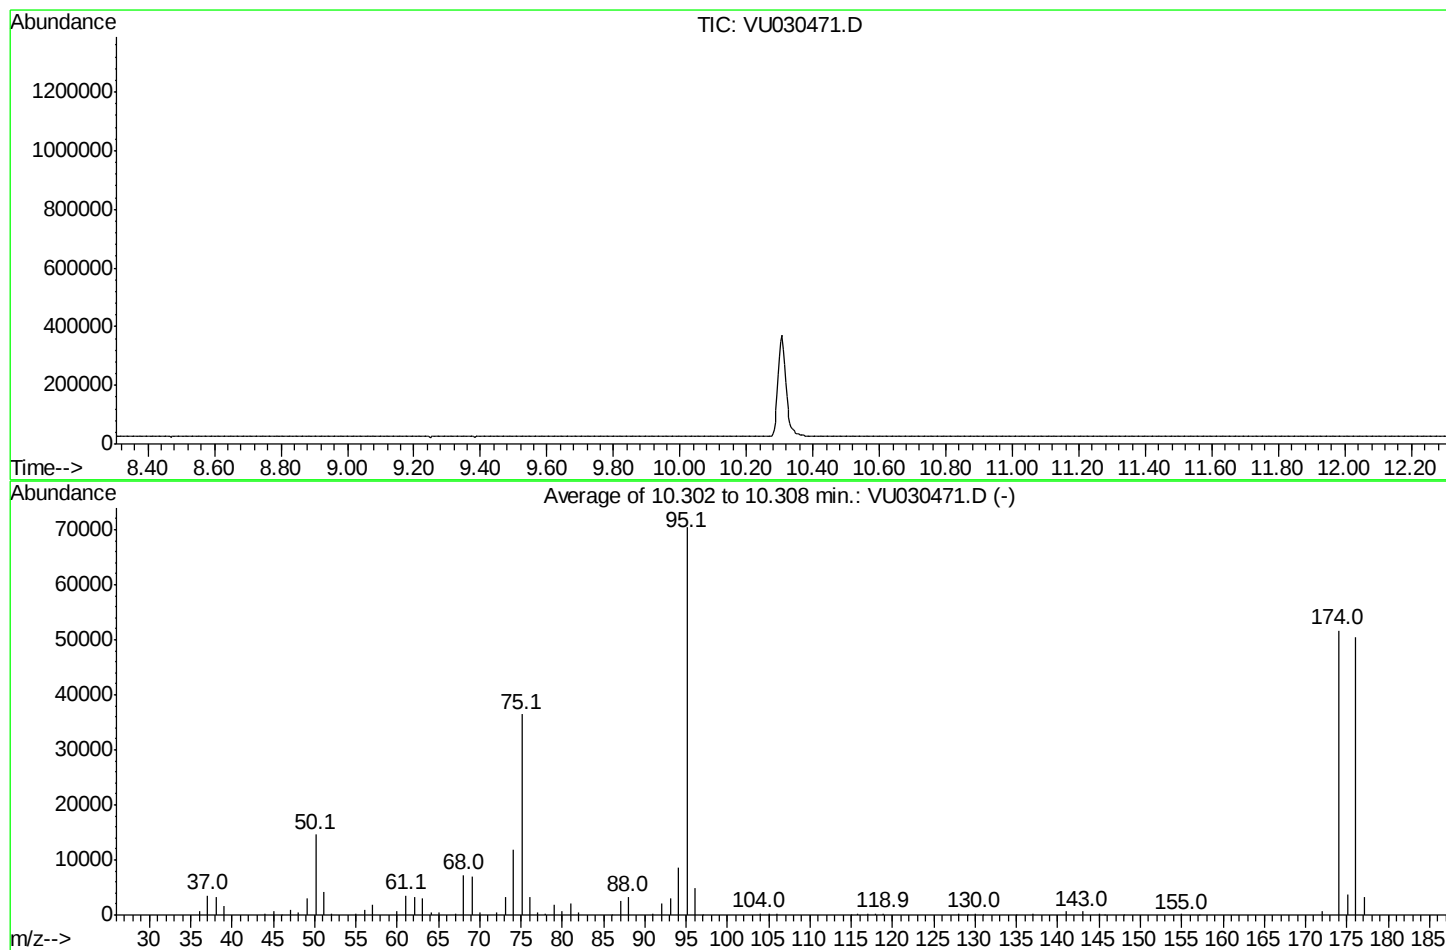

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2854

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.7	14549	PASS
75	95	30	80	51.8	36456	PASS
95	95	100	100	100.0	70432	PASS
96	95	5	9	6.9	4885	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	73.4	51690	PASS
175	174	5	9	7.2	3699	PASS
176	174	95	101	97.5	50421	PASS
177	176	5	9	6.3	3183	PASS

Scan 2854 (10.266 min): VU030471.D
BFB45

m/z	Abundance
40.00	25056.0
44.00	629.0

Instrument :
MSVOA_U
ClientSampleId :
BFB45

m/z	Abundance
36.00	771.0
37.10	3386.0
38.10	3186.0
39.00	1771.0
40.00	24704.0
44.10	908.0
45.00	647.0
46.10	144.0
47.00	989.0
48.00	334.0
49.10	2933.0
50.10	14486.0
51.10	4418.0
52.00	235.0
55.00	177.0
56.00	994.0
57.00	1727.0
60.00	685.0
61.10	3654.0
62.00	3192.0
63.00	2942.0
64.10	489.0
65.00	495.0
67.00	262.0
68.00	6861.0
69.10	6609.0
70.00	520.0
72.00	421.0
73.10	3264.0
74.10	11702.0
75.10	35296.0
76.10	3128.0
77.00	583.0
78.00	322.0
79.00	1906.0
80.00	672.0
81.00	2179.0
82.00	561.0
87.00	2430.0
88.00	3157.0
90.90	214.0
92.10	2241.0
93.10	2964.0
94.10	8232.0
95.10	67848.0
96.10	5100.0
103.90	323.0
105.10	160.0
105.90	269.0
114.90	114.0
115.80	195.0
117.00	279.0
117.90	310.0
119.00	358.0
128.00	171.0
129.00	123.0
130.00	379.0
131.00	101.0
136.90	176.0
140.90	633.0
143.00	660.0
145.00	163.0
147.90	113.0
155.00	127.0
157.10	115.0
172.00	488.0
174.00	48560.0
175.10	3521.0
176.00	47104.0
177.10	2990.0

Instrument :
MSVOA_U
ClientSampleId :
BFB45

m/z	Abundance
36.00	810.0
37.00	3637.0
38.00	3369.0
39.00	1701.0
40.00	24624.0
44.10	870.0
45.00	776.0
46.00	132.0
47.00	1012.0
48.00	397.0
49.10	3098.0
50.10	15072.0
51.10	4372.0
52.00	229.0
54.90	174.0
56.00	1063.0
57.00	1935.0
60.00	773.0
61.10	3726.0
62.10	3460.0
63.10	3103.0
64.10	503.0
65.00	528.0
67.00	273.0
68.10	7599.0
69.10	7100.0
70.00	509.0
72.00	460.0
73.10	3402.0
74.10	12056.0
75.10	37856.0
76.10	3290.0
77.00	477.0
77.90	281.0
79.00	2001.0
80.00	692.0
81.00	2247.0
82.00	503.0
86.00	151.0
87.00	2632.0
88.00	3572.0
91.00	210.0
92.10	2098.0
93.10	3018.0
94.10	8835.0
95.10	72776.0
96.10	5032.0
97.00	129.0
104.00	324.0
105.00	191.0
106.00	273.0
114.90	130.0
115.80	209.0
117.00	319.0
118.00	328.0
118.90	313.0
128.00	202.0
129.00	118.0
130.00	401.0
130.90	121.0
137.00	229.0
140.90	667.0
143.00	693.0
145.00	173.0
145.70	104.0
148.00	118.0
155.00	160.0
157.10	105.0
172.00	621.0
174.00	53232.0
175.10	3793.0
176.00	52128.0
177.00	3238.0

Instrument :
MSVOA_U
ClientSampleId :
BFB45

m/z	Abundance
36.00	775.0
37.00	3531.0
38.00	3188.0
39.00	1550.0
40.00	24528.0
44.10	850.0
45.10	743.0
47.10	1075.0
48.10	481.0
49.10	2846.0
50.10	14089.0
51.10	4071.0
52.00	183.0
54.90	226.0
56.00	1024.0
57.10	1826.0
60.00	763.0
61.10	3263.0
62.10	3282.0
63.10	2906.0
64.10	399.0
65.00	605.0
67.00	236.0
68.10	7495.0
69.10	7262.0
70.00	536.0
72.00	466.0
73.10	3155.0
74.10	11655.0
75.10	36216.0
76.10	3141.0
76.90	390.0
77.80	277.0
79.00	1868.0
80.00	633.0
80.90	2128.0
82.00	447.0
86.00	152.0
87.10	2878.0
88.00	3388.0
91.00	216.0
92.10	1746.0
93.10	2784.0
94.10	8501.0
95.10	70672.0
96.10	4524.0
97.00	141.0
104.00	301.0
105.00	161.0
106.00	250.0
115.80	254.0
117.00	362.0
118.00	289.0
118.80	314.0
128.00	221.0
130.00	292.0
130.90	103.0
134.90	107.0
136.90	203.0
141.00	585.0
143.00	706.0
145.00	174.0
148.00	125.0
155.00	160.0
172.00	745.0
174.00	53280.0
175.10	3783.0
176.00	52032.0
177.00	3321.0

Instrument :
MSVOA_U
ClientSampleId :
BFB45