

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032819\
 Data File : VU030517.D
 Acq On : 28 Mar 2019 16:13
 Operator : JC/SP
 Sample : K2149-07
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF5E9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.399	89	96	106	rBV	230115	231068	14.47%	1.915%
2	1.672	174	181	201	rVB	173414	224724	14.07%	1.863%
3	2.267	357	366	379	rVB	348460	526095	32.95%	4.361%
4	2.505	438	440	445	rBV3	568	589	0.04%	0.005%
5	2.660	484	488	490	rBV	391	273	0.02%	0.002%
6	2.798	529	531	533	rBV	429	237	0.01%	0.002%
7	2.840	533	544	559	rVB2	6745	14768	0.92%	0.122%
8	2.894	559	561	566	rVB2	238	126	0.01%	0.001%
9	3.052	608	610	611	rBV2	186	80	0.01%	0.001%
10	3.084	618	620	621	rBV	237	86	0.01%	0.001%
11	3.142	636	638	640	rBV2	196	121	0.01%	0.001%
12	3.168	643	646	648	rBV2	300	174	0.01%	0.001%
13	3.187	650	652	656	rVB2	378	209	0.01%	0.002%
14	3.287	681	683	684	rBV	236	105	0.01%	0.001%
15	3.328	693	696	699	rVB	231	147	0.01%	0.001%
16	3.357	700	705	708	rBV	348	277	0.02%	0.002%
17	3.415	719	723	725	rBV2	252	186	0.01%	0.002%
18	3.434	725	729	731	rBV2	206	197	0.01%	0.002%
19	3.479	740	743	745	rBV2	191	135	0.01%	0.001%
20	3.495	745	748	752	rVV2	271	241	0.02%	0.002%
21	3.569	768	771	774	rBV	95	66	0.00%	0.001%
22	3.589	774	777	778	rBV2	383	158	0.01%	0.001%
23	3.643	792	794	796	rBV	234	110	0.01%	0.001%
24	3.711	812	815	817	rBV	147	71	0.00%	0.001%
25	3.727	817	820	822	rVB	168	78	0.00%	0.001%
26	3.756	825	829	832	rBV	418	266	0.02%	0.002%
27	3.820	846	849	854	rBV	255	189	0.01%	0.002%
28	3.901	867	874	876	rBV2	227	261	0.02%	0.002%
29	3.920	876	880	882	rVV2	298	206	0.01%	0.002%
30	3.942	886	887	889	rBV	172	70	0.00%	0.001%
31	3.981	897	899	902	rBV2	157	106	0.01%	0.001%
32	4.000	903	905	909	rVB2	360	208	0.01%	0.002%
33	4.026	911	913	914	rBV2	450	120	0.01%	0.001%
34	4.090	931	933	935	rBV2	157	62	0.00%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032819\
 Data File : VU030517.D
 Acq On : 28 Mar 2019 16:13
 Operator : JC/SP
 Sample : K2149-07
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF5E9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

35	4.110	935	939	943	rVB2	255	227	0.01%	0.002%
36	4.129	943	945	947	rBV	199	103	0.01%	0.001%
37	4.174	947	959	990	rBV	163375	444362	27.83%	3.683%
38	4.643	1088	1105	1129	rBV	266397	630039	39.46%	5.223%
39	4.843	1165	1167	1172	rVB2	630	487	0.03%	0.004%
40	4.872	1172	1176	1180	rBV4	1109	1279	0.08%	0.011%
41	4.949	1195	1200	1203	rVB4	880	792	0.05%	0.007%
42	5.026	1222	1224	1227	rBV2	167	133	0.01%	0.001%
43	5.077	1237	1240	1243	rBV2	340	303	0.02%	0.003%
44	5.122	1251	1254	1261	rVB2	200	131	0.01%	0.001%
45	5.151	1261	1263	1267	rVB2	169	119	0.01%	0.001%
46	5.174	1267	1270	1273	rVB2	302	177	0.01%	0.001%
47	5.187	1273	1274	1276	rBV	147	83	0.01%	0.001%
48	5.216	1280	1283	1286	rVB	332	199	0.01%	0.002%
49	5.254	1291	1295	1297	rBV	290	220	0.01%	0.002%
50	5.335	1297	1320	1348	rBV2	535520	1596631	100.00%	13.235%
51	5.733	1441	1444	1445	rBB2	56	68	0.00%	0.001%
52	5.772	1453	1456	1458	rBV2	570	328	0.02%	0.003%
53	5.785	1458	1460	1464	rVB2	490	273	0.02%	0.002%
54	5.881	1477	1490	1519	rBV	475440	963670	60.36%	7.988%
55	6.229	1596	1598	1599	rBV	267	105	0.01%	0.001%
56	6.328	1614	1629	1659	rBV	367908	750945	47.03%	6.225%
57	6.637	1721	1725	1726	rBV2	264	135	0.01%	0.001%
58	6.666	1730	1734	1736	rBV2	448	374	0.02%	0.003%
59	6.749	1758	1760	1763	rBV	145	64	0.00%	0.001%
60	6.804	1775	1777	1781	rBV2	255	183	0.01%	0.002%
61	6.823	1781	1783	1785	rBV	170	100	0.01%	0.001%
62	6.836	1785	1787	1792	rVV	273	174	0.01%	0.001%
63	6.881	1792	1801	1806	rBV4	1295	1774	0.11%	0.015%
64	6.965	1825	1827	1829	rBV	285	116	0.01%	0.001%
65	7.010	1836	1841	1843	rBV2	444	405	0.03%	0.003%
66	7.058	1850	1856	1859	rBV2	319	441	0.03%	0.004%
67	7.129	1876	1878	1881	rBV	320	206	0.01%	0.002%
68	7.167	1885	1890	1895	rBV2	431	481	0.03%	0.004%
69	7.225	1895	1908	1931	rBV	194083	357075	22.36%	2.960%
70	7.499	1992	1993	1996	rVB2	426	185	0.01%	0.002%
71	7.563	1996	2013	2034	rBV	657094	1169403	73.24%	9.694%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU032819\
 Data File : VU030517.D
 Acq On : 28 Mar 2019 16:13
 Operator : JC/SP
 Sample : K2149-07
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF5E9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

72	7.849	2091	2102	2132	rBV	136046	243324	15.24%	2.017%
73	8.048	2160	2164	2166	rBV2	453	432	0.03%	0.004%
74	8.084	2172	2175	2176	rBV	464	244	0.02%	0.002%
75	8.174	2195	2203	2215	rVB2	6574	11100	0.70%	0.092%
76	8.309	2234	2245	2278	rBV2	469847	970626	60.79%	8.046%
77	8.801	2393	2398	2402	rBV2	667	540	0.03%	0.004%
78	8.859	2413	2416	2418	rBV2	412	235	0.01%	0.002%
79	8.894	2425	2427	2431	rVB2	400	256	0.02%	0.002%
80	8.926	2436	2437	2443	rBV2	238	238	0.01%	0.002%
81	9.016	2462	2465	2467	rBV2	255	134	0.01%	0.001%
82	9.087	2474	2487	2516	rBV	692178	1172173	73.42%	9.716%
83	9.286	2547	2549	2550	rBV2	683	281	0.02%	0.002%
84	9.495	2611	2614	2616	rBV2	317	147	0.01%	0.001%
85	9.582	2639	2641	2644	rBV	202	80	0.01%	0.001%
86	9.621	2650	2653	2655	rBV	241	175	0.01%	0.001%
87	9.727	2683	2686	2688	rBV3	240	138	0.01%	0.001%
88	9.781	2695	2703	2705	rBV4	833	882	0.06%	0.007%
89	9.955	2753	2757	2761	rBV3	514	530	0.03%	0.004%
90	10.039	2779	2783	2784	rBV	515	325	0.02%	0.003%
91	10.302	2863	2865	2869	rVB	359	169	0.01%	0.001%
92	10.428	2891	2904	2925	rBV	496009	807982	50.61%	6.698%
93	10.608	2950	2960	2971	rVB5	5581	9904	0.62%	0.082%
94	10.650	2971	2973	2975	rBV	306	135	0.01%	0.001%
95	10.907	3048	3053	3054	rBV	296	252	0.02%	0.002%
96	11.270	3163	3166	3168	rBV2	257	170	0.01%	0.001%
97	11.479	3219	3231	3257	rBV	577911	957685	59.98%	7.939%
98	11.855	3337	3348	3380	rBV	570855	961165	60.20%	7.967%
99	12.762	3627	3630	3634	rBV	684	580	0.04%	0.005%
100	12.881	3665	3667	3670	rBV2	478	279	0.02%	0.002%


Sum of corrected areas: 12063780

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU032819\
Data File : VU030517.D
Acq On : 28 Mar 2019 16:13
Operator : JC/SP
Sample : K2149-07
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF5E9

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

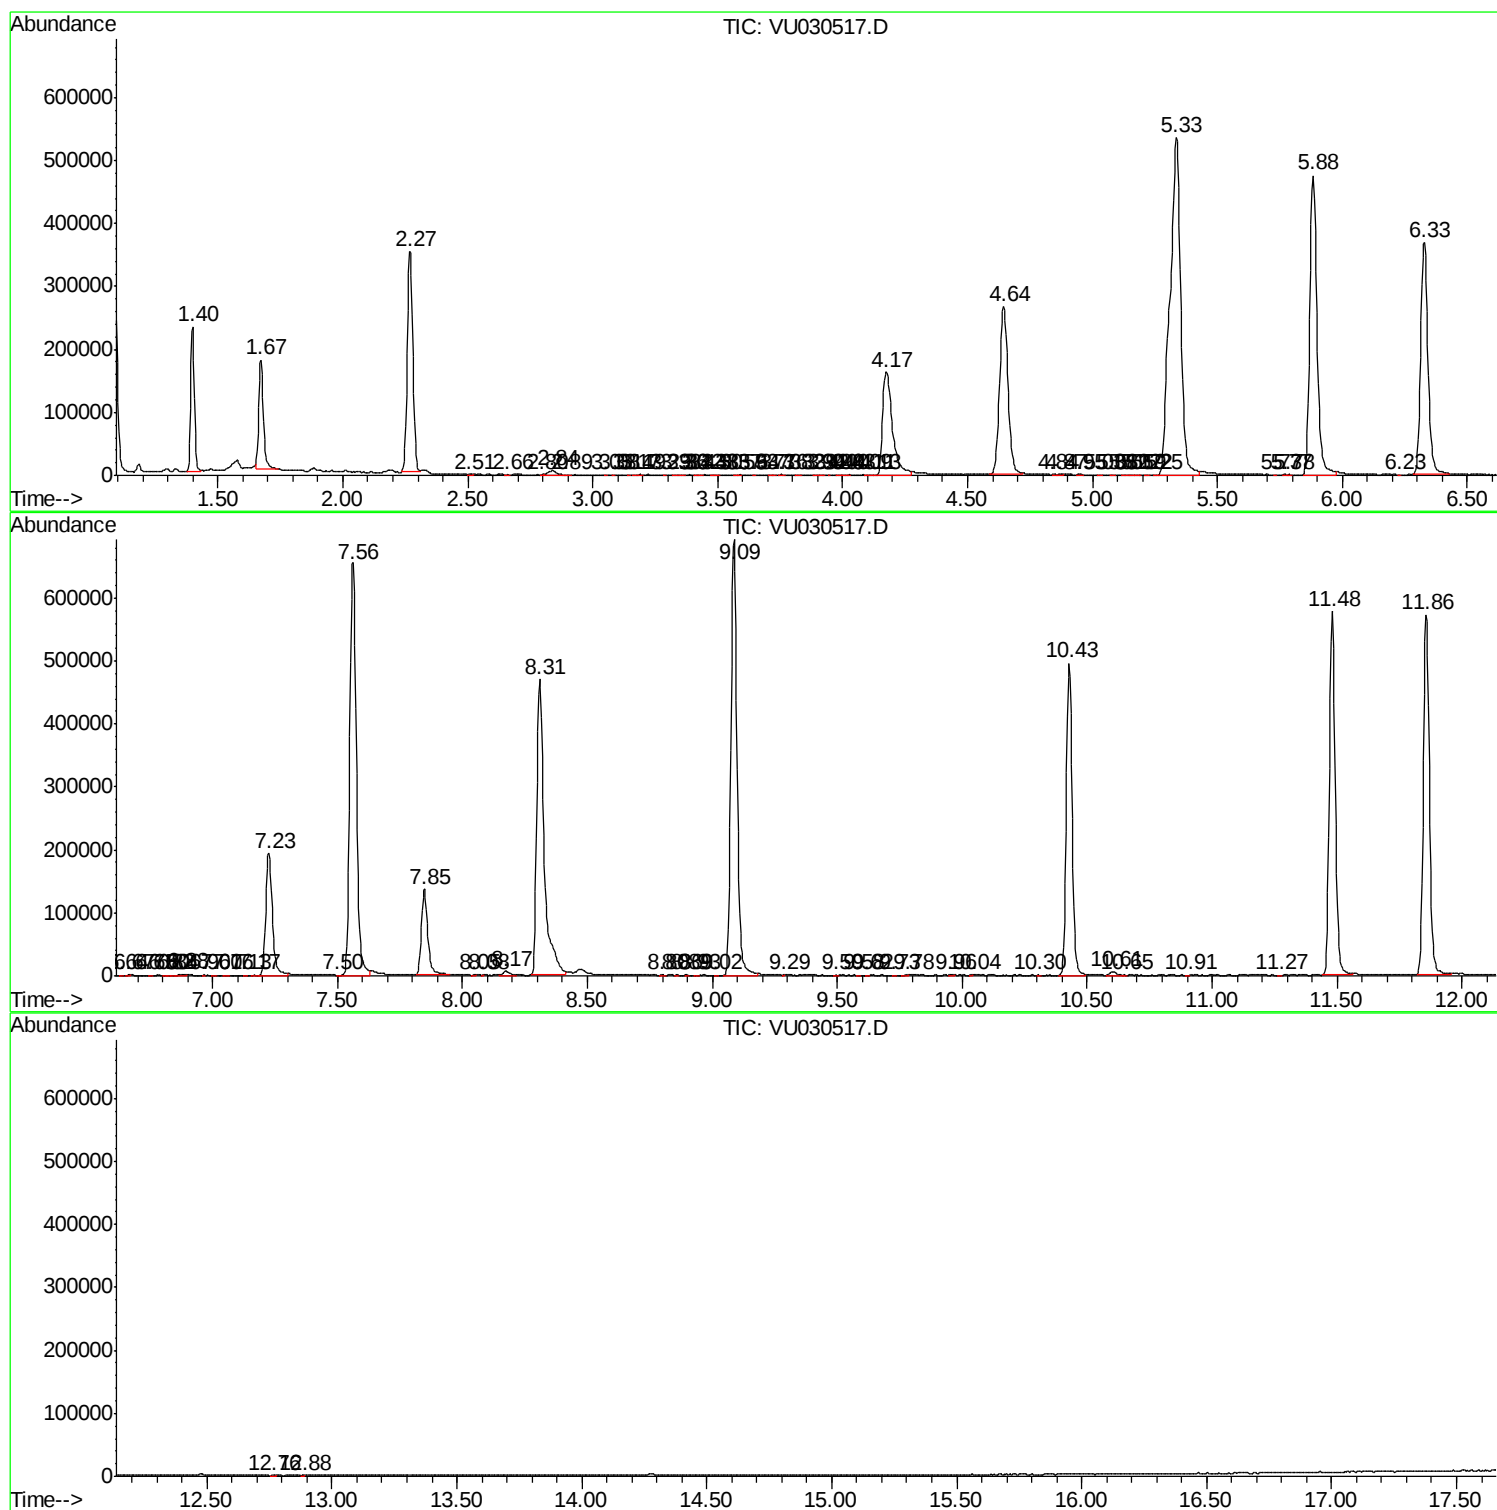

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032819\
Data File : VU030517.D
Acq On : 28 Mar 2019 16:13
Operator : JC/SP
Sample : K2149-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF5E9

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU032819\
Data File : VU030517.D
Acq On : 28 Mar 2019 16:13
Operator : JC/SP
Sample : K2149-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF5E9

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc