


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU032819\
Data File : VU030511.D
Acq On : 28 Mar 2019 13:45
Operator : JC/SP
Sample : BFB46
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB46

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Title : VOC Analysis
Last Update : Fri Mar 29 01:19:16 2019

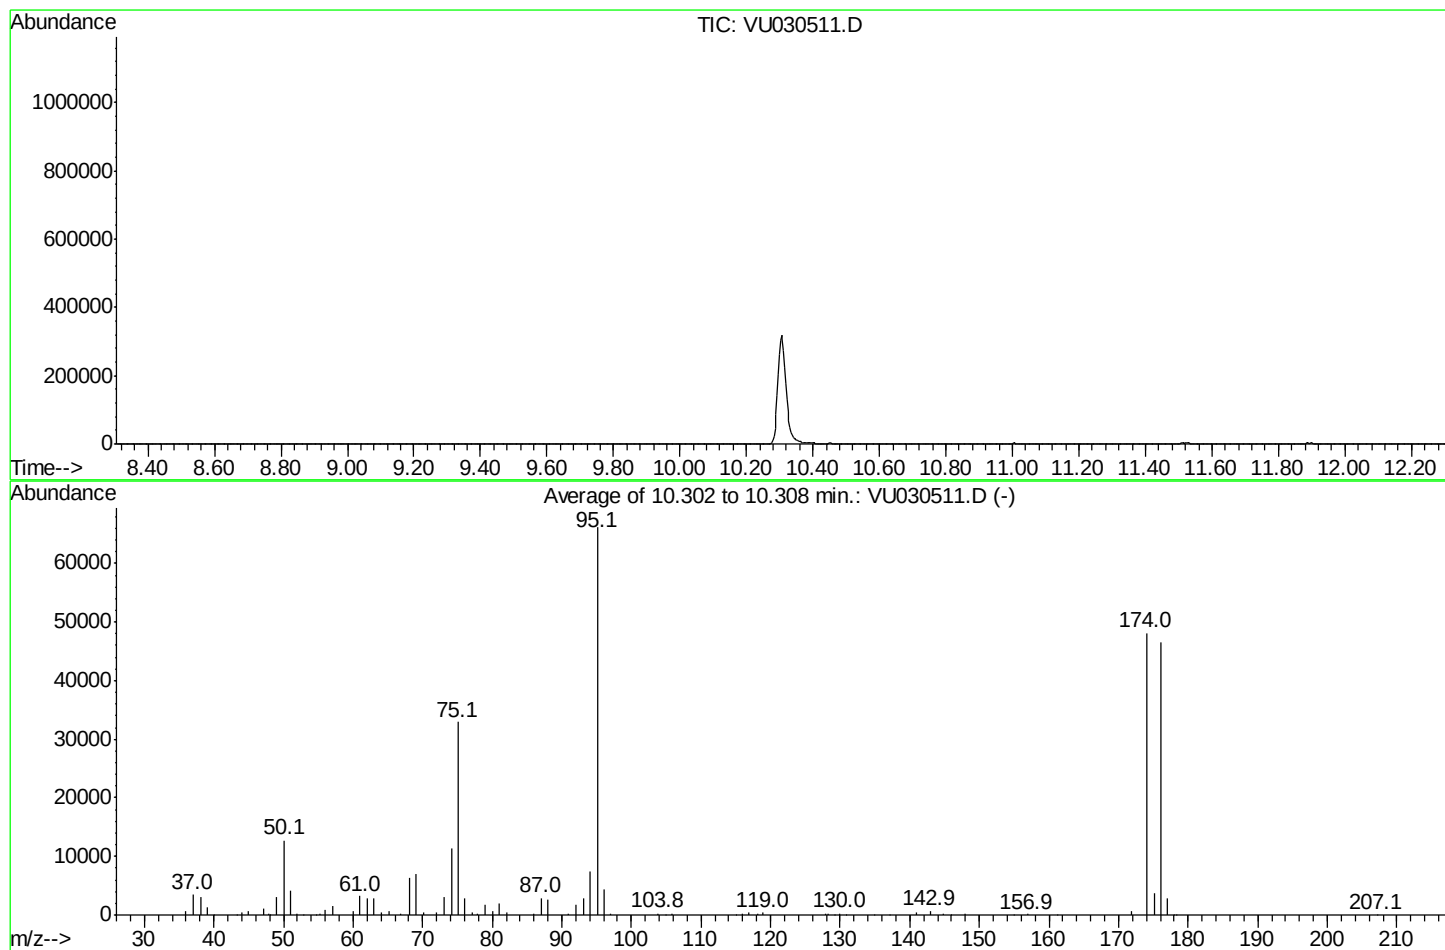

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2854

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.2	12733	PASS
75	95	30	80	49.8	32936	PASS
95	95	100	100	100.0	66160	PASS
96	95	5	9	6.7	4424	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	72.7	48088	PASS
175	174	5	9	7.5	3617	PASS
176	174	95	101	96.7	46482	PASS
177	176	5	9	6.1	2821	PASS

Scan 2854 (10.267 min): VU030511.D
BFB46

m/z	Abundance
40.00	327.0
44.00	631.0

Instrument :
MSVOA_U
ClientSampleId :
BFB46

m/z	Abundance
36.00	676.0
37.00	3514.0
38.00	2959.0
39.00	1272.0
39.90	389.0
43.30	102.0
44.00	947.0
44.90	614.0
47.10	956.0
48.10	266.0
49.00	3082.0
50.10	12381.0
51.10	4063.0
51.90	233.0
52.90	101.0
54.70	144.0
55.20	142.0
56.00	964.0
57.10	1450.0
60.10	648.0
61.00	2942.0
62.10	2775.0
63.00	2753.0
64.00	370.0
65.10	670.0
66.90	207.0
68.10	6364.0
69.10	6736.0
70.00	577.0
72.00	472.0
73.10	2922.0
74.10	11246.0
75.10	32880.0
76.10	2875.0
77.00	478.0
77.80	280.0
78.90	1666.0
80.00	582.0
81.00	1956.0
82.00	489.0
86.00	133.0
87.00	2656.0
88.00	2474.0
90.90	220.0
92.00	1599.0
93.10	2784.0
94.10	7145.0
95.10	64888.0
96.10	4645.0
97.10	136.0
103.90	259.0
104.90	120.0
105.90	195.0
116.00	224.0
116.90	333.0
118.00	191.0
119.00	456.0
127.80	162.0
128.20	158.0
129.10	103.0
130.00	267.0
130.90	119.0
134.80	116.0
137.20	105.0
141.10	494.0
142.90	745.0
144.80	228.0
148.00	155.0
156.90	122.0
171.90	575.0
174.00	46008.0
175.10	3613.0
176.00	45040.0
177.00	2801.0
207.10	118.0

Instrument :
MSVOA_U
ClientSampleId :
BFB46

m/z	Abundance
36.00	701.0
37.00	3508.0
38.10	3139.0
39.00	1386.0
39.90	448.0
43.30	108.0
44.00	978.0
45.00	567.0
47.10	1090.0
47.80	337.0
49.00	3080.0
50.10	13143.0
51.10	4180.0
51.90	166.0
54.80	143.0
55.10	129.0
56.00	1007.0
57.10	1551.0
60.00	667.0
61.00	3324.0
62.10	3015.0
63.00	2955.0
64.10	410.0
65.10	714.0
66.90	281.0
68.10	6471.0
69.10	7242.0
70.10	570.0
72.00	461.0
73.10	3176.0
74.10	11734.0
75.10	33880.0
76.10	2939.0
77.10	447.0
77.80	317.0
78.90	1785.0
80.00	594.0
81.00	2076.0
82.00	477.0
86.00	163.0
87.00	3071.0
88.00	2680.0
90.80	238.0
92.00	1718.0
93.10	2967.0
94.10	7600.0
95.10	68008.0
96.10	4592.0
97.00	127.0
103.80	276.0
104.90	127.0
105.80	201.0
115.00	105.0
116.00	250.0
116.90	389.0
118.00	184.0
119.00	384.0
127.80	208.0
128.20	205.0
129.10	104.0
130.00	227.0
130.90	126.0
137.00	112.0
141.00	524.0
143.00	799.0
144.80	239.0
145.90	112.0
148.00	203.0
156.90	138.0
171.90	551.0
174.00	49488.0
175.10	3668.0
176.00	47856.0
177.10	2877.0
177.90	101.0
207.10	113.0

Instrument :
MSVOA_U
ClientSampleId :
BFB46

m/z	Abundance
36.00	677.0
37.00	3330.0
38.10	3044.0
39.00	1423.0
39.90	449.0
44.00	1001.0
45.00	545.0
47.10	1116.0
47.80	312.0
49.00	2729.0
50.10	12676.0
51.10	4021.0
52.00	120.0
55.20	128.0
56.00	936.0
57.10	1581.0
60.00	670.0
61.00	3293.0
62.10	3030.0
63.00	2806.0
64.10	379.0
65.10	752.0
66.90	289.0
68.10	6028.0
69.10	6986.0
70.10	499.0
72.00	362.0
73.10	3045.0
74.10	11247.0
75.10	32048.0
76.10	2808.0
77.00	428.0
77.80	292.0
78.90	1852.0
80.00	626.0
81.00	2000.0
82.00	434.0
86.00	156.0
87.00	2895.0
88.00	2713.0
90.80	222.0
92.00	1768.0
93.10	2924.0
94.10	7554.0
95.10	65584.0
96.10	4036.0
97.00	104.0
103.80	265.0
105.80	205.0
115.10	107.0
116.00	277.0
116.90	415.0
118.10	209.0
118.90	340.0
127.90	262.0
130.00	213.0
130.90	109.0
136.90	105.0
140.90	576.0
143.00	755.0
144.90	216.0
145.90	104.0
148.00	212.0
155.00	105.0
156.90	117.0
161.10	107.0
171.90	595.0
174.00	48768.0
175.10	3572.0
176.00	46552.0
177.00	2787.0
178.20	117.0

Instrument :
MSVOA_U
ClientSampleId :
BFB46