




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032823\
 Data File : VU053440.D
 Acq On : 28 Mar 2023 17:50
 Operator : JC/MD
 Sample : 02037-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E45F1

Manual IntegrationsAPPROVED

Quant Time: Mar 29 01:13:41 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Mar 29 01:10:06 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 03/31/2023
 Supervised By :Mahesh Dadoda 03/31/2023

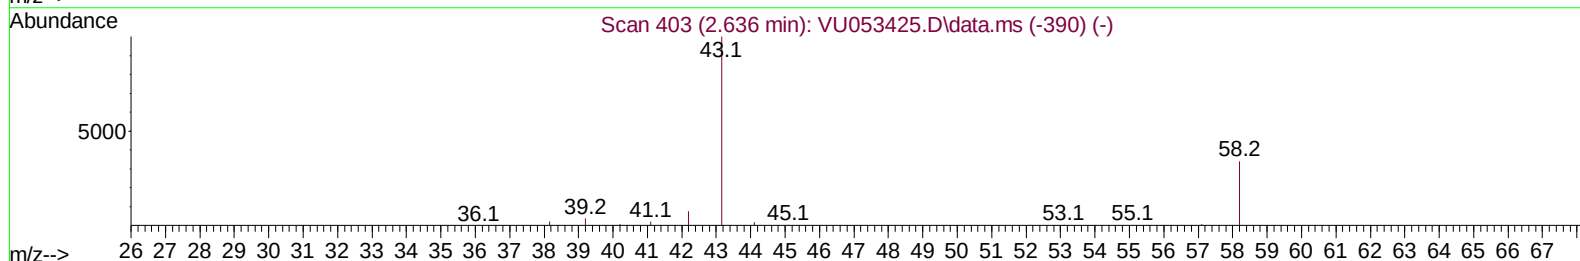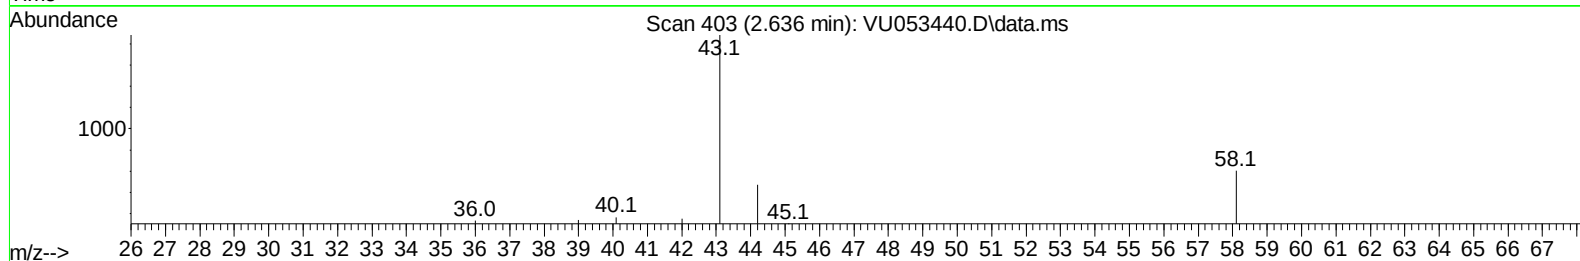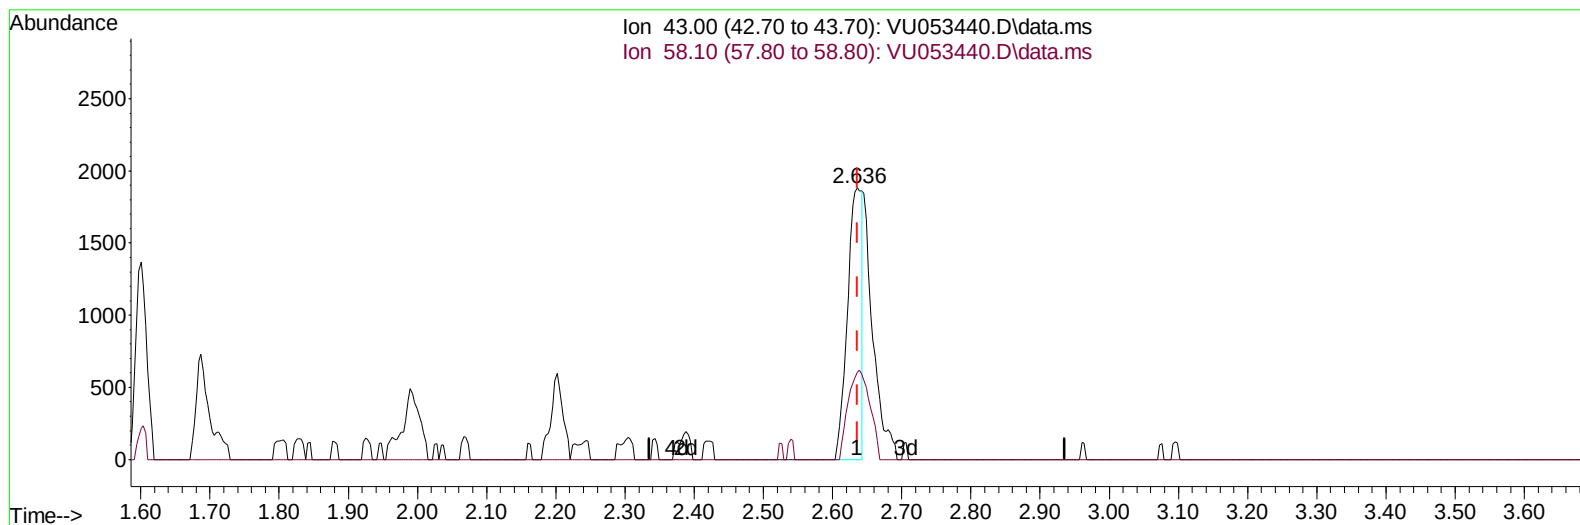

TIC: VU053440.D\data.ms

(13) Acetone (T)

2.636min (-0.000) 2.75 ug/L

response 2702

Ion	Exp%	Act%
43.00	100.00	100.00
58.10	37.50	49.37
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032823\
 Data File : VU053440.D
 Acq On : 28 Mar 2023 17:50
 Operator : JC/MD
 Sample : 02037-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E45F1

Manual IntegrationsAPPROVED

Quant Time: Mar 29 01:13:41 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Mar 29 01:10:06 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 03/31/2023
 Supervised By :Mahesh Dadoda 03/31/2023

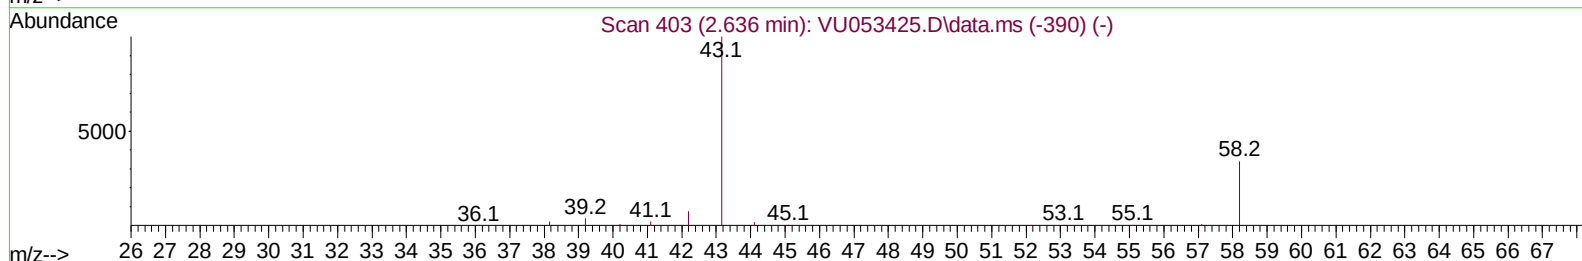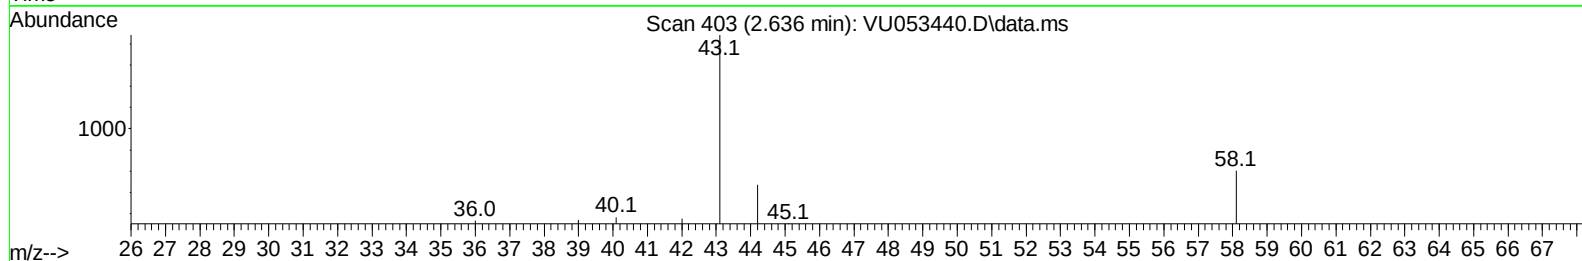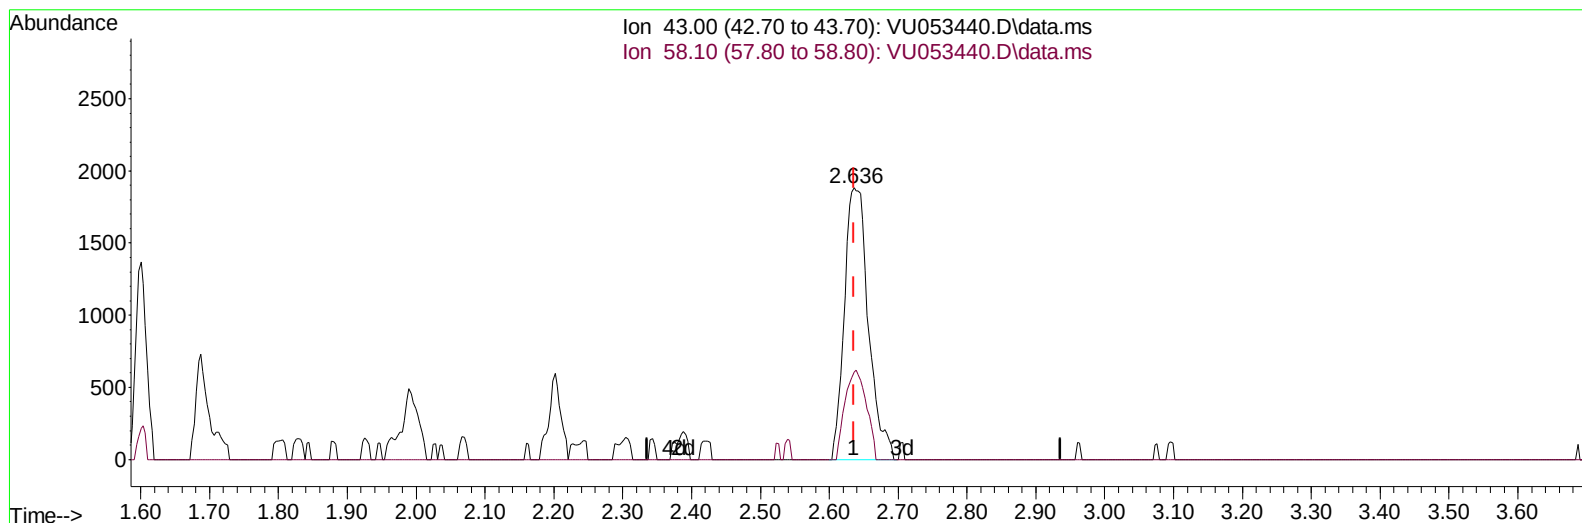

TIC: VU053440.D\data.ms

(13) Acetone (T)

2.636min (-0.000) 4.64 ug/L m

response 4558

Ion	Exp%	Act%
43.00	100.00	100.00
58.10	37.50	29.27
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032823\
 Data File : VU053440.D
 Acq On : 28 Mar 2023 17:50
 Operator : JC/MD
 Sample : 02037-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E45F1

Manual IntegrationsAPPROVED

Quant Time: Mar 29 01:13:41 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Mar 29 01:10:06 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 03/31/2023
 Supervised By :Mahesh Dadoda 03/31/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	6.243	114		201569	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.414	117		189803	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.806	152		90620	50.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.597	65		85499	45.977	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135		Recovery	=	91.960%	
7) Chloroethane-d5	1.912	69		68581	45.594	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130		Recovery	=	91.180%	
11) 1,1-Dichloroethene-d2	2.565	63		107096	33.245	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125		Recovery	=	66.500%	
21) 2-Butanone-d5	4.623	46		104973	121.710	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130		Recovery	=	121.710%	
24) Chloroform-d	5.057	84		137493	44.891	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery	=	89.780%	
26) 1,2-Dichloroethane-d4	5.697	65		93048	48.917	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery	=	97.840%	
32) Benzene-d6	5.722	84		281984	45.804	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery	=	91.600%	
36) 1,2-Dichloropropane-d6	6.684	67		96467	48.551	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120		Recovery	=	97.100%	
41) Toluene-d8	7.893	98		254436	44.391	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120		Recovery	=	88.780%	
43) trans-1,3-Dichloroprop...	8.176	79		42399	43.250	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125		Recovery	=	86.500%	
47) 2-Hexanone-d5	8.629	63		60655	97.644	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130		Recovery	=	97.640%	
56) 1,1,2,2-Tetrachloroeth...	10.751	84		127552	49.556	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120		Recovery	=	99.120%	
66) 1,2-Dichlorobenzene-d4	12.188	152		92027	52.447	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120		Recovery	=	104.900%	
Target Compounds							Qvalue
13) Acetone	2.636	43		4558m	4.640	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032823\
Data File : VU053440.D
Acq On : 28 Mar 2023 17:50
Operator : JC/MD
Sample : 02037-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 3

Instrument :
MSVOA_U
ClientSampleId :
E45F1

Manual IntegrationsAPPROVED

Quant Time: Mar 29 01:13:41 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Mar 29 01:10:06 2023
Response via : Initial Calibration

Reviewed By :Krupa Patel 03/31/2023
Supervised By :Mahesh Dadoda 03/31/2023

