

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032823\
 Data File : VU053430.D
 Acq On : 28 Mar 2023 13:57
 Operator : JC/MD
 Sample : 02085-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COMBO

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

Signal : TIC: VU053430.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	96	rVB	124451	146615	4.40%	1.376%
2	1.912	170	178	198	rVB	95140	135337	4.06%	1.270%
3	2.565	369	381	398	rBV	185636	300562	9.02%	2.821%
4	2.784	446	449	453	rBV2	541	490	0.01%	0.005%
5	2.954	500	502	506	rVB3	443	278	0.01%	0.003%
6	3.041	524	529	536	rBV3	747	929	0.03%	0.009%
7	3.134	552	558	559	rBV2	380	308	0.01%	0.003%
8	3.182	559	573	593	rVB	14085	31337	0.94%	0.294%
9	3.285	603	605	609	rBV2	261	219	0.01%	0.002%
10	3.549	681	687	692	rBV2	419	496	0.01%	0.005%
11	3.581	692	697	703	rBV2	278	312	0.01%	0.003%
12	3.896	791	795	800	rBV2	184	175	0.01%	0.002%
13	3.935	804	807	812	rVV2	343	278	0.01%	0.003%
14	3.964	812	816	820	rVB2	260	227	0.01%	0.002%
15	4.192	884	887	891	rVV	245	145	0.00%	0.001%
16	4.330	925	930	932	rBV2	356	336	0.01%	0.003%
17	4.349	934	936	941	rVV2	328	273	0.01%	0.003%
18	4.391	944	949	952	rVV2	256	273	0.01%	0.003%
19	4.623	1008	1021	1061	rBV2	70827	201009	6.03%	1.886%
20	4.960	1123	1126	1129	rVB2	323	210	0.01%	0.002%
21	4.980	1129	1132	1133	rBV	318	207	0.01%	0.002%
22	5.057	1140	1156	1174	rBV	159868	350585	10.53%	3.290%
23	5.230	1207	1210	1213	rVB2	234	175	0.01%	0.002%
24	5.266	1213	1221	1224	rBV2	197	220	0.01%	0.002%
25	5.385	1256	1258	1263	rBV	203	144	0.00%	0.001%
26	5.420	1263	1269	1271	rVB2	311	306	0.01%	0.003%
27	5.478	1285	1287	1291	rVB	310	150	0.00%	0.001%
28	5.504	1291	1295	1298	rVB2	271	222	0.01%	0.002%
29	5.719	1341	1362	1395	rBV2	321243	896145	26.91%	8.410%
30	6.044	1459	1463	1465	rBV	201	144	0.00%	0.001%
31	6.066	1467	1470	1476	rVV	182	182	0.01%	0.002%
32	6.102	1477	1481	1483	rVV2	205	152	0.00%	0.001%
33	6.118	1483	1486	1490	rVB2	265	190	0.01%	0.002%
34	6.243	1509	1525	1548	rBV	256726	484035	14.53%	4.542%
35	6.417	1576	1579	1582	rVB2	306	190	0.01%	0.002%
36	6.478	1593	1598	1604	rVB3	398	488	0.01%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032823\
 Data File : VU053430.D
 Acq On : 28 Mar 2023 13:57
 Operator : JC/MD
 Sample : 02085-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COMBO

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

37	6.529	1609	1614	1619	rVB3	627	648	0.02%	0.006%
38	6.687	1649	1663	1688	rVB	206159	400502	12.02%	3.758%
39	6.800	1694	1698	1700	rBV2	408	319	0.01%	0.003%
40	6.873	1719	1721	1729	rVB	252	263	0.01%	0.002%
41	7.102	1786	1792	1796	rBV2	200	253	0.01%	0.002%
42	7.269	1838	1844	1848	rVB2	238	261	0.01%	0.002%
43	7.301	1852	1854	1859	rVV2	178	143	0.00%	0.001%
44	7.324	1859	1861	1865	rVV	260	201	0.01%	0.002%
45	7.562	1923	1935	1951	rBV	116913	204463	6.14%	1.919%
46	7.668	1965	1968	1970	rBV2	233	157	0.00%	0.001%
47	7.697	1975	1977	1980	rVB2	540	291	0.01%	0.003%
48	7.748	1989	1993	1999	rBV2	225	338	0.01%	0.003%
49	7.893	2025	2038	2057	rBV	404011	695283	20.87%	6.525%
50	8.031	2079	2081	2086	rVB3	538	382	0.01%	0.004%
51	8.176	2115	2126	2143	rVV	79972	133968	4.02%	1.257%
52	8.301	2162	2165	2168	rVB	351	239	0.01%	0.002%
53	8.468	2213	2217	2220	rBV2	404	411	0.01%	0.004%
54	8.504	2226	2228	2233	rVB	248	153	0.00%	0.001%
55	8.555	2241	2244	2247	rVB2	235	160	0.00%	0.002%
56	8.590	2252	2255	2256	rBV2	323	178	0.01%	0.002%
57	8.629	2256	2267	2302	rVV3	178997	356069	10.69%	3.341%
58	8.835	2329	2331	2336	rVB2	385	238	0.01%	0.002%
59	8.938	2358	2363	2367	rBV	276	315	0.01%	0.003%
60	9.195	2440	2443	2449	rBV	218	215	0.01%	0.002%
61	9.414	2498	2511	2517	rBV	364205	640244	19.22%	6.008%
62	9.568	2556	2559	2562	rVB2	387	241	0.01%	0.002%
63	9.632	2574	2579	2581	rBV	200	201	0.01%	0.002%
64	9.748	2613	2615	2620	rVB2	218	173	0.01%	0.002%
65	9.780	2621	2625	2628	rBV	206	157	0.00%	0.001%
66	9.857	2645	2649	2653	rVB2	228	207	0.01%	0.002%
67	9.947	2673	2677	2680	rVB2	280	201	0.01%	0.002%
68	10.095	2719	2723	2724	rBV2	289	190	0.01%	0.002%
69	10.336	2794	2798	2804	rVB	360	290	0.01%	0.003%
70	10.365	2804	2807	2810	rVB2	211	155	0.00%	0.001%
71	10.407	2816	2820	2822	rBV	208	176	0.01%	0.002%
72	10.446	2830	2832	2836	rVB2	217	145	0.00%	0.001%
73	10.574	2869	2872	2875	rVV2	197	142	0.00%	0.001%
74	10.751	2915	2927	2948	rBV	259877	417281	12.53%	3.916%
75	10.851	2955	2958	2961	rVB2	258	171	0.01%	0.002%
76	11.298	3094	3097	3101	rBV	252	207	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032823\
 Data File : VU053430.D
 Acq On : 28 Mar 2023 13:57
 Operator : JC/MD
 Sample : 02085-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COMBO

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

77	11.391	3123	3126	3129	rBV2	293	208	0.01%	0.002%
78	11.471	3147	3151	3159	rBV3	424	552	0.02%	0.005%
79	11.561	3176	3179	3182	rBV	214	177	0.01%	0.002%
80	11.577	3182	3184	3187	rVV2	273	174	0.01%	0.002%
81	11.677	3211	3215	3219	rBV2	189	190	0.01%	0.002%
82	11.700	3219	3222	3224	rBV2	189	139	0.00%	0.001%
83	11.741	3224	3235	3245	rVV	78652	124097	3.73%	1.165%
84	11.806	3245	3255	3282	rVB2	375609	700994	21.05%	6.578%
85	12.028	3321	3324	3330	rBV2	414	357	0.01%	0.003%
86	12.204	3361	3379	3407	rBV3	1788649	3330736	100.00%	31.257%
87	12.372	3429	3431	3435	rVB2	492	280	0.01%	0.003%
88	12.529	3477	3480	3485	rBV2	255	181	0.01%	0.002%
89	12.642	3512	3515	3519	rBV	266	227	0.01%	0.002%
90	12.680	3524	3527	3532	rVV3	512	387	0.01%	0.004%
91	12.848	3575	3579	3582	rBV2	313	214	0.01%	0.002%
92	12.864	3582	3584	3587	rBV	223	152	0.00%	0.001%
93	13.204	3682	3690	3702	rBV3	9565	16376	0.49%	0.154%
94	13.323	3720	3727	3735	rBV4	2061	2931	0.09%	0.028%
95	13.468	3768	3772	3776	rVB2	352	280	0.01%	0.003%
96	13.548	3794	3797	3804	rBV2	342	455	0.01%	0.004%
97	13.835	3874	3886	3905	rBV	440270	685212	20.57%	6.430%
98	14.085	3960	3964	3972	rVB2	3693	4051	0.12%	0.038%
99	14.323	4026	4038	4059	rBV	204642	327809	9.84%	3.076%
100	15.995	4548	4558	4570	rVB3	32536	50883	1.53%	0.478%




Sum of corrected areas: 10656037

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032823\
Data File : VU053430.D
Acq On : 28 Mar 2023 13:57
Operator : JC/MD
Sample : 02085-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COMBO

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

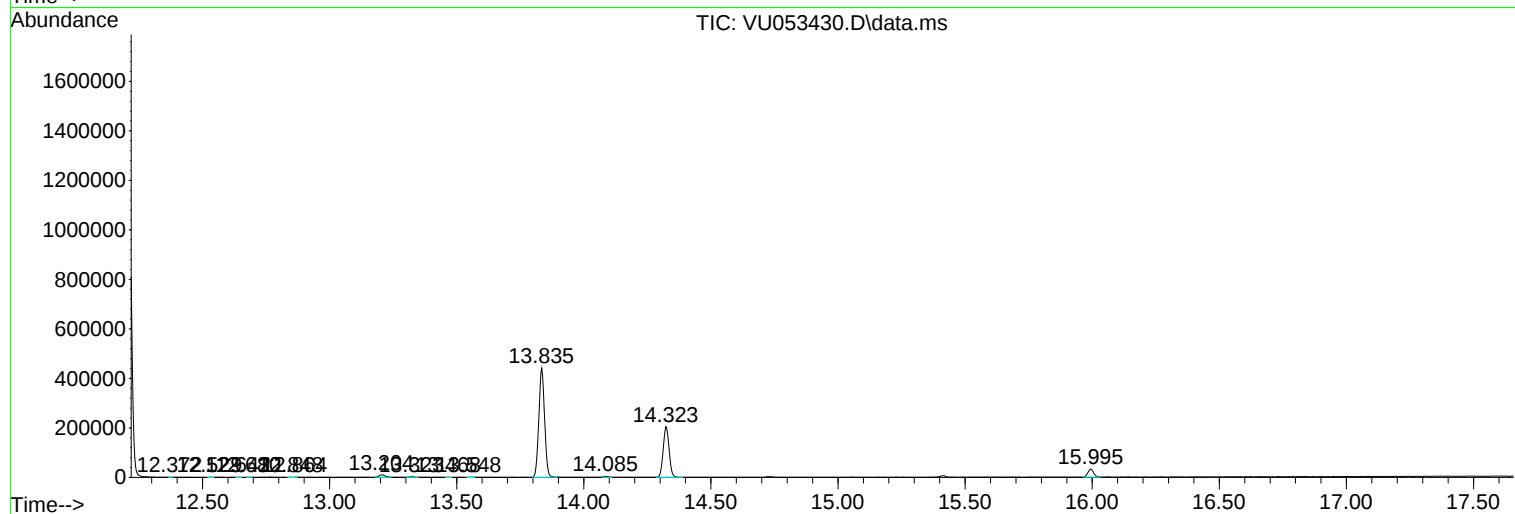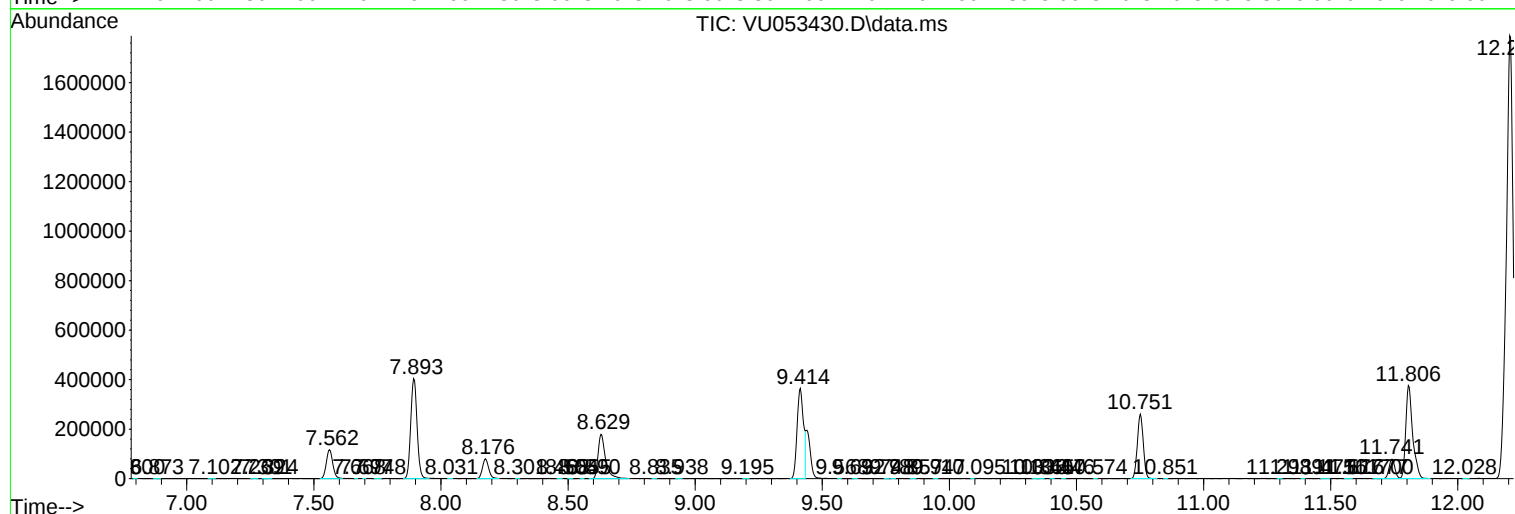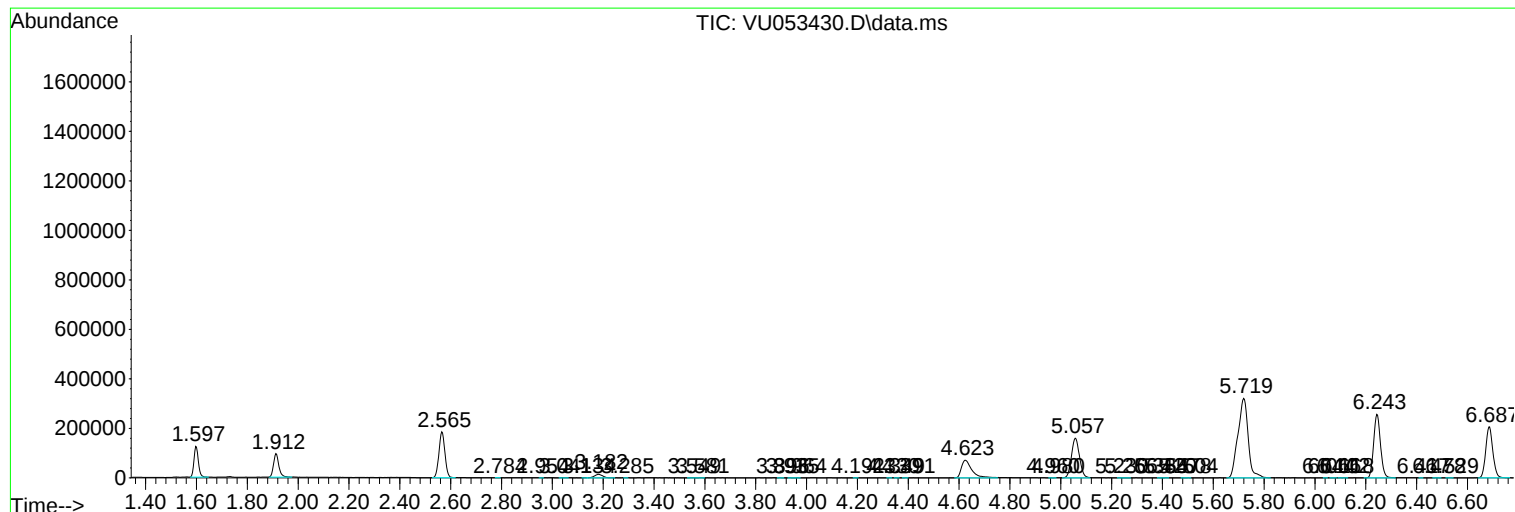

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032823\
Data File : VU053430.D
Acq On : 28 Mar 2023 13:57
Operator : JC/MD
Sample : 02085-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COMB0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032823\
Data File : VU053430.D
Acq On : 28 Mar 2023 13:57
Operator : JC/MD
Sample : 02085-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COMB0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------