

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032823\
 Data File : VU053433.D
 Acq On : 28 Mar 2023 15:07
 Operator : JC/MD
 Sample : 02085-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COMB3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

Signal : TIC: VU053433.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	92	rBV	121013	142234	16.68%	2.194%
2	1.912	170	178	196	rVB	94946	132361	15.52%	2.042%
3	2.565	369	381	398	rBV	180453	296095	34.72%	4.567%
4	2.845	466	468	470	rBV	379	225	0.03%	0.003%
5	2.890	477	482	483	rBV	319	181	0.02%	0.003%
6	3.031	523	526	528	rBV	448	324	0.04%	0.005%
7	3.102	544	548	554	rBV2	436	448	0.05%	0.007%
8	3.182	558	573	590	rBV	15004	34582	4.05%	0.533%
9	3.285	602	605	608	rBV	377	253	0.03%	0.004%
10	3.379	631	634	637	rVB2	265	199	0.02%	0.003%
11	3.481	659	666	669	rVB	394	454	0.05%	0.007%
12	3.507	669	674	679	rBV2	277	304	0.04%	0.005%
13	3.536	679	683	686	rVV	208	233	0.03%	0.004%
14	3.571	690	694	698	rBV	268	226	0.03%	0.003%
15	3.597	698	702	704	rBV	248	198	0.02%	0.003%
16	3.755	746	751	753	rBV2	265	212	0.02%	0.003%
17	3.864	780	785	787	rBV	154	163	0.02%	0.003%
18	3.922	799	803	806	rBV	255	189	0.02%	0.003%
19	3.941	806	809	813	rVB2	303	226	0.03%	0.003%
20	3.967	813	817	819	rBV2	218	148	0.02%	0.002%
21	4.015	828	832	835	rVB2	190	164	0.02%	0.003%
22	4.279	908	914	917	rBV	217	190	0.02%	0.003%
23	4.401	945	952	954	rBV2	259	288	0.03%	0.004%
24	4.481	974	977	982	rVB2	237	175	0.02%	0.003%
25	4.533	990	993	1000	rVB2	194	236	0.03%	0.004%
26	4.626	1004	1022	1047	rBV2	73710	205795	24.13%	3.174%
27	4.919	1110	1113	1115	rBV	213	154	0.02%	0.002%
28	4.980	1130	1132	1137	rBV3	279	276	0.03%	0.004%
29	5.057	1142	1156	1177	rVB	155590	338990	39.75%	5.229%
30	5.186	1194	1196	1202	rVB2	385	266	0.03%	0.004%
31	5.214	1202	1205	1206	rBV2	271	151	0.02%	0.002%
32	5.288	1222	1228	1230	rBV	232	195	0.02%	0.003%
33	5.356	1245	1249	1252	rBV2	212	181	0.02%	0.003%
34	5.423	1265	1270	1274	rBV2	292	334	0.04%	0.005%
35	5.510	1293	1297	1300	rVB	234	189	0.02%	0.003%
36	5.600	1321	1325	1328	rBV	307	210	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032823\
 Data File : VU053433.D
 Acq On : 28 Mar 2023 15:07
 Operator : JC/MD
 Sample : 02085-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COMB3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

37	5.623	1328	1332	1335	rBV2	202	178	0.02%	0.003%
38	5.719	1342	1362	1382	rBV2	317652	852835	100.00%	13.155%
39	5.980	1437	1443	1449	rBV2	315	468	0.05%	0.007%
40	6.147	1491	1495	1500	rVB2	269	219	0.03%	0.003%
41	6.243	1512	1525	1545	rBV	256210	486087	57.00%	7.498%
42	6.488	1596	1601	1604	rVB	494	332	0.04%	0.005%
43	6.517	1604	1610	1611	rBV	477	373	0.04%	0.006%
44	6.687	1646	1663	1684	rBV	198840	391737	45.93%	6.042%
45	6.944	1740	1743	1750	rVB	259	232	0.03%	0.004%
46	6.976	1750	1753	1755	rBV2	234	151	0.02%	0.002%
47	7.028	1767	1769	1774	rVB2	293	199	0.02%	0.003%
48	7.063	1774	1780	1784	rBV	175	198	0.02%	0.003%
49	7.118	1794	1797	1800	rBV	240	181	0.02%	0.003%
50	7.195	1816	1821	1826	rVV2	576	654	0.08%	0.010%
51	7.407	1883	1887	1891	rBV	239	207	0.02%	0.003%
52	7.465	1902	1905	1909	rVB2	291	220	0.03%	0.003%
53	7.510	1914	1919	1922	rVB2	306	243	0.03%	0.004%
54	7.562	1922	1935	1954	rBV	113435	200335	23.49%	3.090%
55	7.793	2004	2007	2011	rVB2	365	221	0.03%	0.003%
56	7.893	2025	2038	2067	rBV	397120	684277	80.24%	10.555%
57	8.082	2094	2097	2099	rBV2	227	158	0.02%	0.002%
58	8.118	2103	2108	2110	rBV	232	168	0.02%	0.003%
59	8.176	2114	2126	2148	rBV	76841	131864	15.46%	2.034%
60	8.275	2154	2157	2160	rVB2	310	204	0.02%	0.003%
61	8.324	2165	2172	2175	rBV2	246	403	0.05%	0.006%
62	8.439	2199	2208	2211	rBV	242	317	0.04%	0.005%
63	8.629	2250	2267	2295	rBV2	185202	374415	43.90%	5.775%
64	8.880	2342	2345	2351	rVB3	296	268	0.03%	0.004%
65	8.912	2351	2355	2359	rBV2	250	240	0.03%	0.004%
66	8.947	2364	2366	2371	rVB	226	167	0.02%	0.003%
67	9.037	2392	2394	2399	rBV	169	171	0.02%	0.003%
68	9.095	2408	2412	2415	rBV	222	207	0.02%	0.003%
69	9.317	2475	2481	2484	rVB2	193	238	0.03%	0.004%
70	9.336	2485	2487	2492	rVB	223	150	0.02%	0.002%
71	9.414	2498	2511	2538	rBV	350265	588307	68.98%	9.074%
72	9.545	2551	2552	2558	rVB	306	152	0.02%	0.002%
73	9.574	2558	2561	2565	rVB3	364	239	0.03%	0.004%
74	9.600	2565	2569	2572	rBV2	312	234	0.03%	0.004%
75	9.658	2584	2587	2592	rBV	180	182	0.02%	0.003%
76	10.098	2720	2724	2727	rVV2	238	167	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032823\
 Data File : VU053433.D
 Acq On : 28 Mar 2023 15:07
 Operator : JC/MD
 Sample : 02085-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COMB3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

77	10.121	2727	2731	2734	rVB	297	280	0.03%	0.004%
78	10.291	2776	2784	2789	rBV2	363	515	0.06%	0.008%
79	10.401	2816	2818	2826	rVB	283	199	0.02%	0.003%
80	10.436	2826	2829	2831	rBV	336	256	0.03%	0.004%
81	10.751	2915	2927	2950	rVB	262804	420627	49.32%	6.488%
82	10.880	2965	2967	2970	rBV	366	161	0.02%	0.002%
83	10.941	2981	2986	2987	rBV	185	165	0.02%	0.003%
84	11.285	3090	3093	3098	rBV2	325	298	0.03%	0.005%
85	11.468	3146	3150	3155	rVB2	207	193	0.02%	0.003%
86	11.500	3155	3160	3164	rBV2	407	360	0.04%	0.006%
87	11.642	3201	3204	3211	rVB2	242	258	0.03%	0.004%
88	11.674	3211	3214	3217	rBV	320	241	0.03%	0.004%
89	11.745	3232	3236	3241	rVB2	646	503	0.06%	0.008%
90	11.806	3241	3255	3274	rBV	357977	565858	66.35%	8.728%
91	12.082	3332	3341	3354	rBV6	1657	4044	0.47%	0.062%
92	12.188	3361	3374	3396	rBV	364755	602624	70.66%	9.295%
93	12.732	3537	3543	3547	rBV	354	280	0.03%	0.004%
94	12.767	3547	3554	3559	rBV3	985	1372	0.16%	0.021%
95	12.815	3565	3569	3574	rBV2	357	365	0.04%	0.006%
96	12.957	3611	3613	3615	rBV2	261	157	0.02%	0.002%
97	13.259	3705	3707	3711	rVB2	335	169	0.02%	0.003%
98	13.841	3882	3888	3902	rVB7	3550	5927	0.69%	0.091%
99	14.034	3946	3948	3951	rBV	395	310	0.04%	0.005%
100	14.330	4033	4040	4048	rBV6	1800	3277	0.38%	0.051%




Sum of corrected areas: 6483086

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032823\
Data File : VU053433.D
Acq On : 28 Mar 2023 15:07
Operator : JC/MD
Sample : 02085-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COMB3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

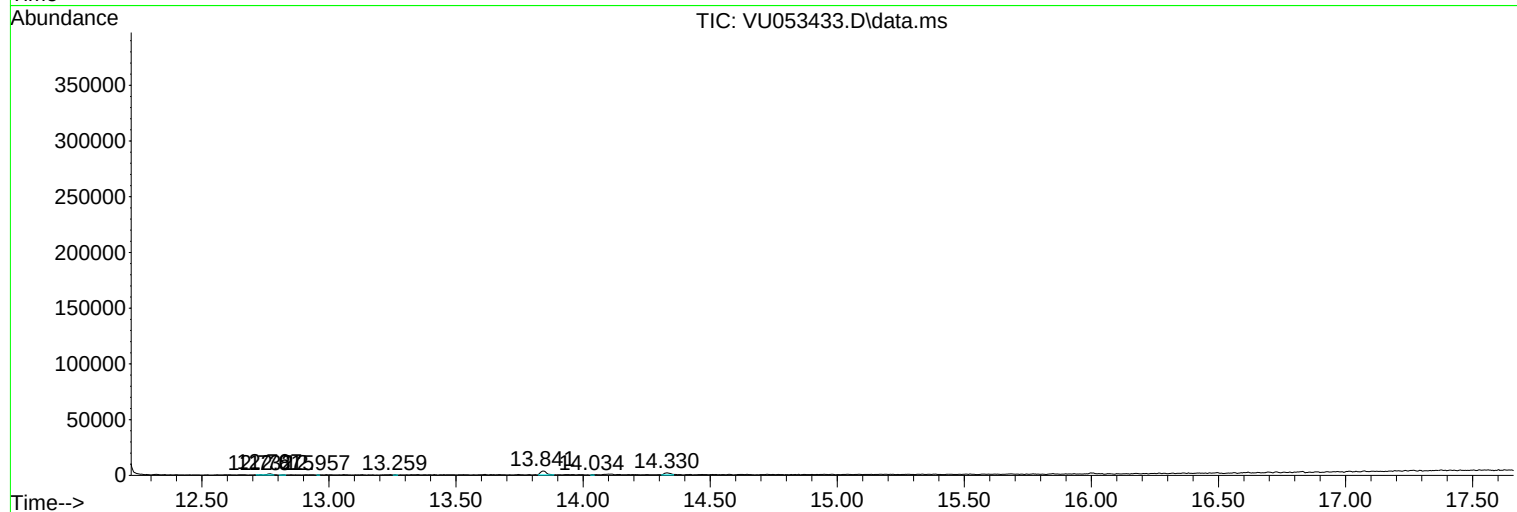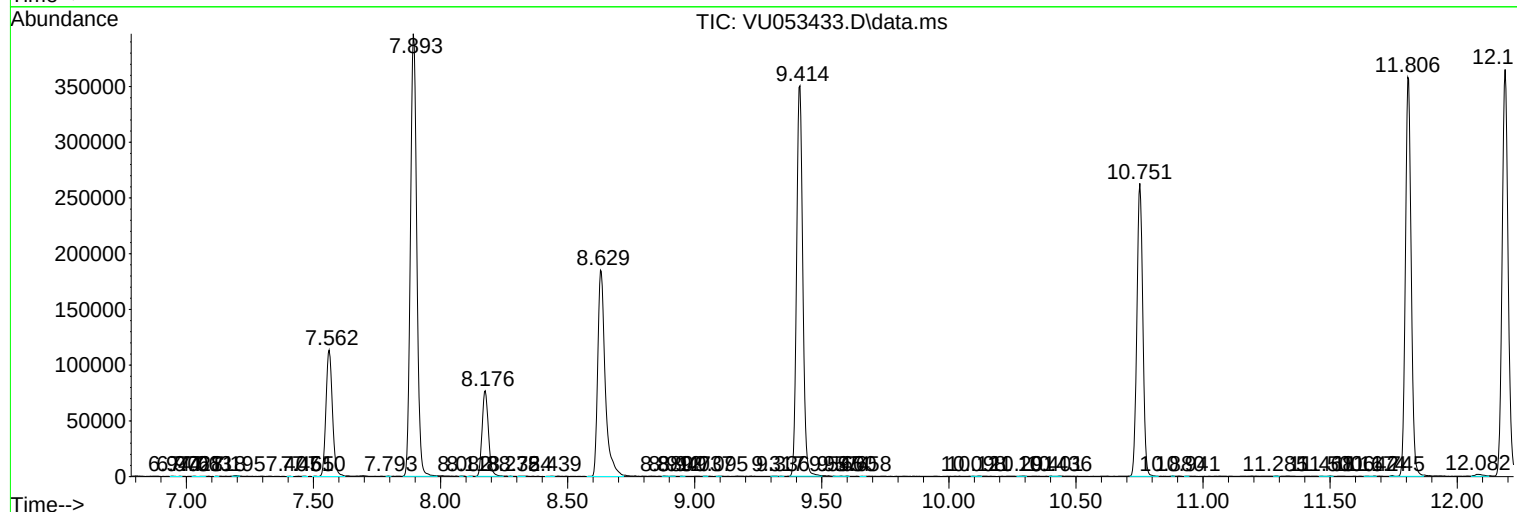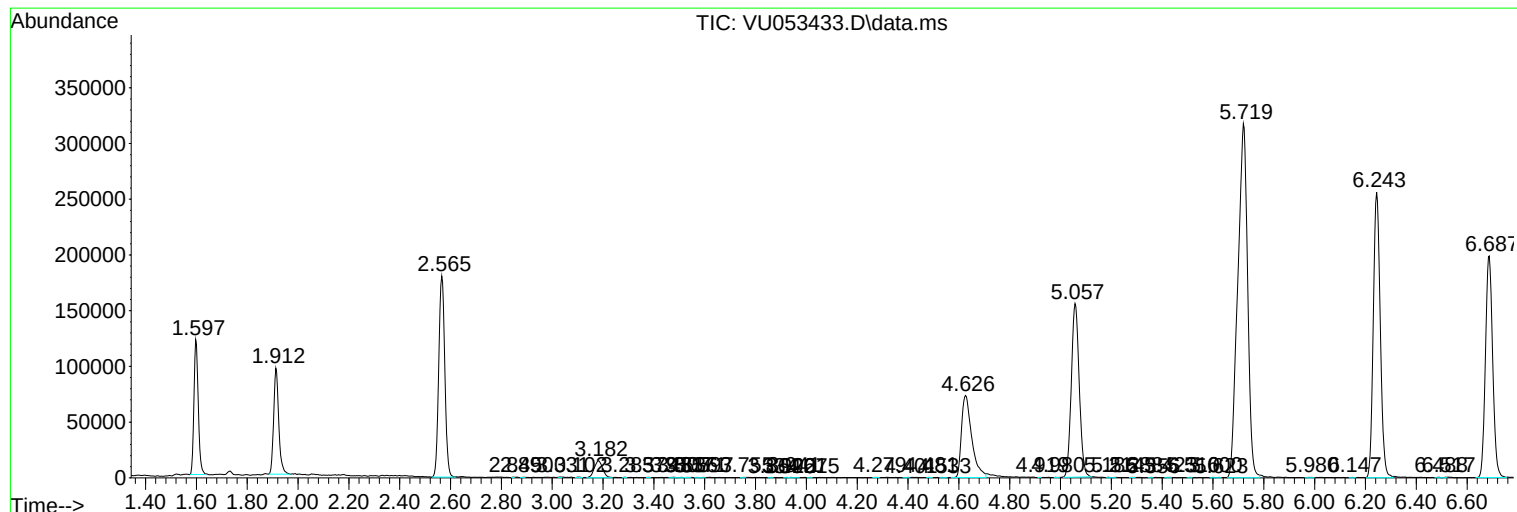

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032823\
Data File : VU053433.D
Acq On : 28 Mar 2023 15:07
Operator : JC/MD
Sample : 02085-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COMB3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032823\
Data File : VU053433.D
Acq On : 28 Mar 2023 15:07
Operator : JC/MD
Sample : 02085-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0MB3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------