

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032823\
 Data File : VU053435.D
 Acq On : 28 Mar 2023 15:53
 Operator : JC/MD
 Sample : 02037-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E45E7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

Signal : TIC: VU053435.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	96	rVB	96351	112530	14.80%	1.877%
2	1.912	171	178	192	rVB	81163	111174	14.62%	1.854%
3	2.565	370	381	395	rBV	149897	239447	31.48%	3.993%
4	2.829	459	463	467	rBV3	333	343	0.05%	0.006%
5	3.035	521	527	528	rBV3	663	559	0.07%	0.009%
6	3.176	567	571	577	rBV2	667	963	0.13%	0.016%
7	3.247	589	593	595	rBV	213	166	0.02%	0.003%
8	3.324	615	617	623	rBV	313	201	0.03%	0.003%
9	3.350	623	625	627	rBV2	372	235	0.03%	0.004%
10	3.533	678	682	684	rBV2	220	176	0.02%	0.003%
11	3.568	688	693	696	rVB3	326	269	0.04%	0.004%
12	3.613	704	707	713	rVB2	287	305	0.04%	0.005%
13	3.645	713	717	722	rBV2	329	327	0.04%	0.005%
14	3.684	726	729	733	rBV2	248	204	0.03%	0.003%
15	3.761	750	753	759	rBV2	354	288	0.04%	0.005%
16	4.012	827	831	836	rBV2	265	316	0.04%	0.005%
17	4.131	862	868	871	rBV	260	251	0.03%	0.004%
18	4.256	902	907	909	rBV	203	211	0.03%	0.004%
19	4.295	915	919	923	rBV2	242	232	0.03%	0.004%
20	4.324	923	928	931	rVV2	318	284	0.04%	0.005%
21	4.417	952	957	960	rBV	166	177	0.02%	0.003%
22	4.472	970	974	979	rBV	259	252	0.03%	0.004%
23	4.497	979	982	986	rBV2	181	178	0.02%	0.003%
24	4.533	990	993	996	rBV2	253	179	0.02%	0.003%
25	4.626	1010	1022	1054	rBV	62525	178743	23.50%	2.981%
26	5.057	1140	1156	1178	rBV	141850	311421	40.95%	5.193%
27	5.256	1214	1218	1223	rVB2	208	192	0.03%	0.003%
28	5.350	1244	1247	1252	rBV2	193	231	0.03%	0.004%
29	5.404	1261	1264	1268	rVB2	205	197	0.03%	0.003%
30	5.462	1275	1282	1285	rBV2	270	356	0.05%	0.006%
31	5.555	1308	1311	1316	rVB	245	207	0.03%	0.003%
32	5.581	1316	1319	1325	rVB2	220	221	0.03%	0.004%
33	5.719	1341	1362	1386	rBV2	277505	760568	100.00%	12.684%
34	5.896	1415	1417	1422	rVB2	379	191	0.03%	0.003%
35	5.919	1422	1424	1427	rBV2	396	290	0.04%	0.005%
36	6.031	1455	1459	1463	rBV2	228	255	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032823\
 Data File : VU053435.D
 Acq On : 28 Mar 2023 15:53
 Operator : JC/MD
 Sample : 02037-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E45E7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

37	6.243	1511	1525	1547	rBV	267399	511403	67.24%	8.528%
38	6.523	1608	1612	1613	rBV2	791	460	0.06%	0.008%
39	6.575	1625	1628	1630	rBV	215	162	0.02%	0.003%
40	6.687	1648	1663	1687	rBV	184522	356272	46.84%	5.941%
41	6.899	1724	1729	1735	rVB2	268	355	0.05%	0.006%
42	6.970	1748	1751	1757	rVB	232	212	0.03%	0.004%
43	6.999	1757	1760	1762	rBV2	400	247	0.03%	0.004%
44	7.124	1797	1799	1803	rVB2	286	190	0.02%	0.003%
45	7.179	1812	1816	1817	rBV	416	291	0.04%	0.005%
46	7.317	1855	1859	1862	rBV	228	205	0.03%	0.003%
47	7.349	1865	1869	1876	rBV2	191	236	0.03%	0.004%
48	7.433	1890	1895	1898	rBV2	228	254	0.03%	0.004%
49	7.491	1910	1913	1916	rBV	247	176	0.02%	0.003%
50	7.562	1923	1935	1952	rBV	78959	136958	18.01%	2.284%
51	7.690	1971	1975	1976	rBV2	472	294	0.04%	0.005%
52	7.771	1997	2000	2005	rBV	246	228	0.03%	0.004%
53	7.838	2015	2021	2025	rBV2	296	343	0.05%	0.006%
54	7.893	2025	2038	2061	rBV	341273	589408	77.50%	9.829%
55	8.076	2093	2095	2099	rVB	283	163	0.02%	0.003%
56	8.124	2106	2110	2114	rBV2	312	268	0.04%	0.004%
57	8.176	2114	2126	2145	rBV2	52344	90894	11.95%	1.516%
58	8.542	2234	2240	2242	rBV	230	183	0.02%	0.003%
59	8.629	2255	2267	2296	rBV3	174604	349893	46.00%	5.835%
60	8.928	2357	2360	2364	rVB2	329	211	0.03%	0.004%
61	9.208	2443	2447	2450	rBV2	225	220	0.03%	0.004%
62	9.414	2498	2511	2540	rBV	371070	645884	84.92%	10.771%
63	9.552	2551	2554	2558	rVB3	294	176	0.02%	0.003%
64	9.574	2558	2561	2562	rBV	279	165	0.02%	0.003%
65	9.623	2573	2576	2580	rBV	244	169	0.02%	0.003%
66	9.661	2585	2588	2591	rBV2	246	201	0.03%	0.003%
67	9.706	2599	2602	2608	rVB3	304	234	0.03%	0.004%
68	9.764	2616	2620	2624	rBV2	199	207	0.03%	0.003%
69	9.787	2624	2627	2632	rVB	212	178	0.02%	0.003%
70	9.832	2638	2641	2647	rVB2	280	301	0.04%	0.005%
71	9.925	2665	2670	2673	rBV	250	251	0.03%	0.004%
72	9.944	2673	2676	2681	rBV	237	179	0.02%	0.003%
73	10.089	2717	2721	2725	rVB2	331	236	0.03%	0.004%
74	10.115	2725	2729	2731	rBV	243	175	0.02%	0.003%
75	10.324	2788	2794	2799	rBV2	336	459	0.06%	0.008%
76	10.510	2847	2852	2854	rBV	265	189	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032823\
 Data File : VU053435.D
 Acq On : 28 Mar 2023 15:53
 Operator : JC/MD
 Sample : 02037-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E45E7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

77	10.751	2914	2927	2947	rBV	253048	403010	52.99%	6.721%
78	10.980	2993	2998	3002	rBV2	261	230	0.03%	0.004%
79	11.134	3042	3046	3051	rBV2	212	206	0.03%	0.003%
80	11.414	3129	3133	3136	rBV2	273	248	0.03%	0.004%
81	11.436	3136	3140	3143	rVV	270	201	0.03%	0.003%
82	11.465	3146	3149	3153	rVV2	307	256	0.03%	0.004%
83	11.652	3204	3207	3213	rBV	250	162	0.02%	0.003%
84	11.745	3230	3236	3244	rVB5	1901	2528	0.33%	0.042%
85	11.806	3244	3255	3275	rBV	351306	590798	77.68%	9.852%
86	12.079	3331	3340	3346	rBV5	1607	2926	0.38%	0.049%
87	12.189	3362	3374	3397	rBV	331398	560743	73.73%	9.351%
88	12.295	3404	3407	3411	rBV3	822	604	0.08%	0.010%
89	12.536	3479	3482	3486	rBV	222	221	0.03%	0.004%
90	12.600	3499	3502	3507	rVB2	255	208	0.03%	0.003%
91	12.899	3592	3595	3599	rBV2	462	327	0.04%	0.005%
92	13.105	3656	3659	3662	rBV	337	200	0.03%	0.003%
93	13.243	3700	3702	3705	rBV	404	262	0.03%	0.004%
94	13.301	3717	3720	3721	rBV	358	183	0.02%	0.003%
95	13.841	3878	3888	3899	rBV2	10344	16593	2.18%	0.277%
96	14.237	4005	4011	4015	rBV2	561	731	0.10%	0.012%
97	14.285	4022	4026	4029	rBV3	331	277	0.04%	0.005%
98	14.330	4034	4040	4049	rVB3	3055	4257	0.56%	0.071%
99	14.446	4073	4076	4078	rBV	651	401	0.05%	0.007%
100	14.848	4199	4201	4202	rBV	472	213	0.03%	0.004%




Sum of corrected areas: 5996454

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032823\
Data File : VU053435.D
Acq On : 28 Mar 2023 15:53
Operator : JC/MD
Sample : 02037-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E45E7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

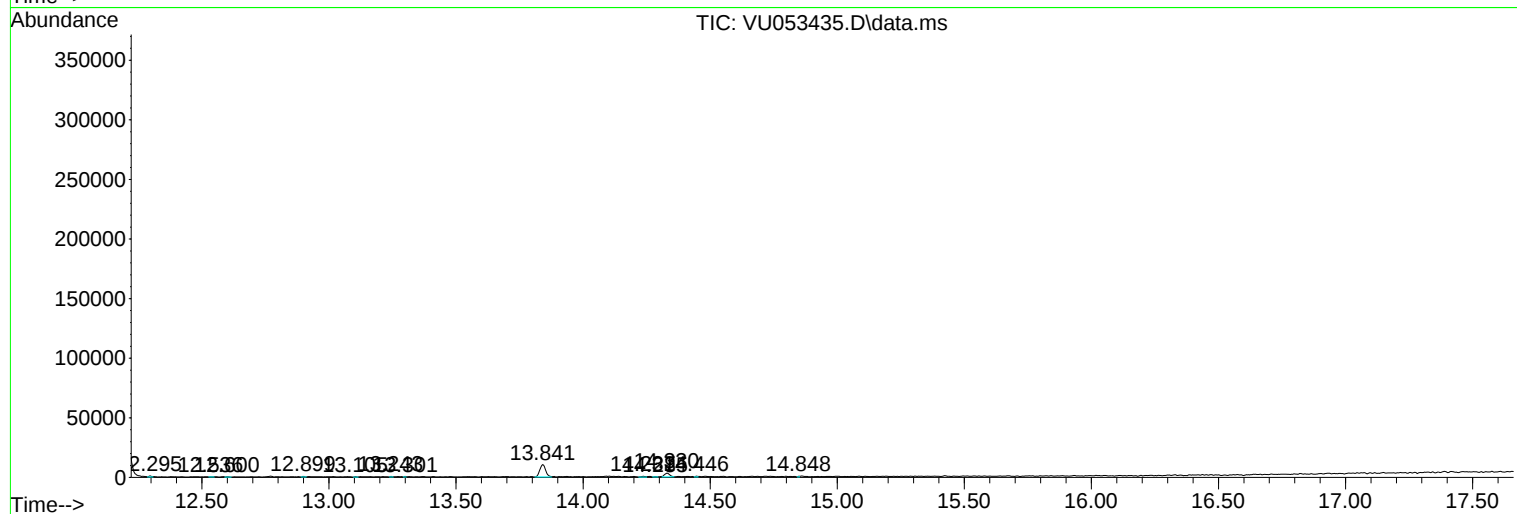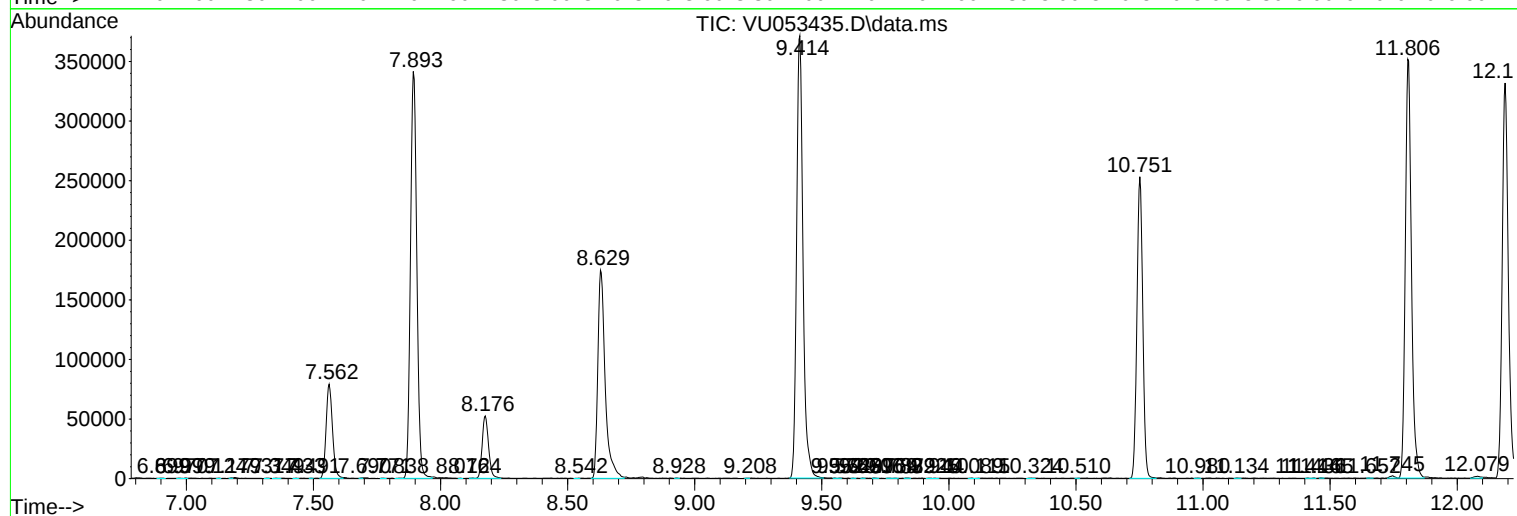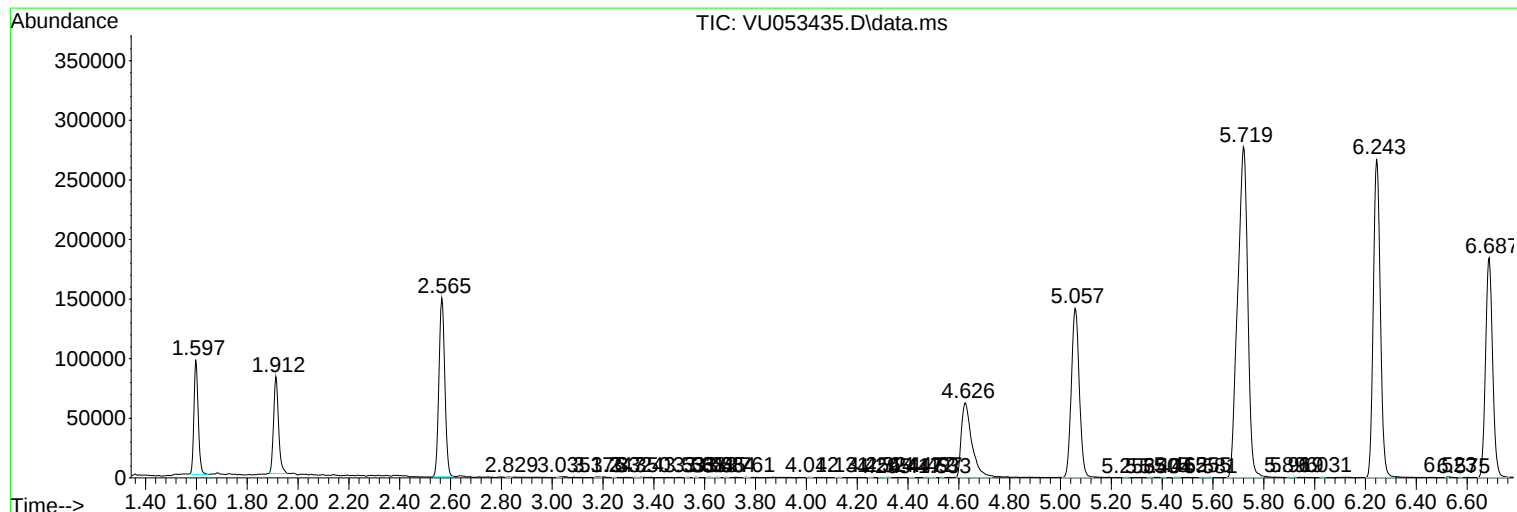

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032823\
Data File : VU053435.D
Acq On : 28 Mar 2023 15:53
Operator : JC/MD
Sample : 02037-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E45E7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032823\
Data File : VU053435.D
Acq On : 28 Mar 2023 15:53
Operator : JC/MD
Sample : 02037-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E45E7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------