

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032823\
 Data File : VU053436.D
 Acq On : 28 Mar 2023 16:17
 Operator : JC/MD
 Sample : 02037-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E45E8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

Signal : TIC: VU053436.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	74	80	91	rVB	91742	106406	13.99%	1.806%
2	1.912	171	178	197	rVB	81259	109895	14.45%	1.865%
3	2.565	369	381	396	rBV	146644	237597	31.25%	4.032%
4	3.234	586	589	597	rVB	279	222	0.03%	0.004%
5	3.269	598	600	605	rBV	297	180	0.02%	0.003%
6	3.436	649	652	654	rBV	290	222	0.03%	0.004%
7	3.469	659	662	665	rBV	243	188	0.02%	0.003%
8	3.665	719	723	725	rBV	329	280	0.04%	0.005%
9	3.790	758	762	764	rBV2	244	170	0.02%	0.003%
10	4.079	847	852	856	rBV2	332	323	0.04%	0.005%
11	4.231	895	899	903	rBV2	220	176	0.02%	0.003%
12	4.379	942	945	948	rBV2	209	203	0.03%	0.003%
13	4.469	971	973	977	rVV2	241	168	0.02%	0.003%
14	4.536	991	994	998	rVB2	174	174	0.02%	0.003%
15	4.626	1010	1022	1047	rBV	63565	175737	23.11%	2.982%
16	5.002	1133	1139	1141	rVV	210	256	0.03%	0.004%
17	5.057	1141	1156	1179	rVV	142850	312941	41.16%	5.310%
18	5.256	1207	1218	1220	rBV2	314	482	0.06%	0.008%
19	5.494	1288	1292	1297	rBV	320	283	0.04%	0.005%
20	5.526	1299	1302	1305	rBV2	208	167	0.02%	0.003%
21	5.594	1318	1323	1325	rBV2	241	234	0.03%	0.004%
22	5.719	1341	1362	1387	rBV2	276064	760344	100.00%	12.902%
23	5.867	1405	1408	1412	rVB	378	305	0.04%	0.005%
24	5.893	1413	1416	1419	rBV	288	174	0.02%	0.003%
25	5.915	1420	1423	1425	rBV3	334	228	0.03%	0.004%
26	5.967	1436	1439	1444	rVV3	322	284	0.04%	0.005%
27	5.996	1444	1448	1455	rVB2	321	207	0.03%	0.004%
28	6.047	1460	1464	1469	rBV2	199	195	0.03%	0.003%
29	6.099	1477	1480	1483	rBV2	301	229	0.03%	0.004%
30	6.153	1495	1497	1499	rBV2	320	201	0.03%	0.003%
31	6.243	1510	1525	1546	rBV	261175	493805	64.94%	8.379%
32	6.417	1575	1579	1583	rVB2	469	390	0.05%	0.007%
33	6.443	1583	1587	1588	rBV	272	164	0.02%	0.003%
34	6.533	1608	1615	1617	rBV5	979	1009	0.13%	0.017%
35	6.597	1631	1635	1638	rBV2	378	266	0.03%	0.005%
36	6.616	1638	1641	1645	rVB2	415	257	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032823\
 Data File : VU053436.D
 Acq On : 28 Mar 2023 16:17
 Operator : JC/MD
 Sample : 02037-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E45E8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

37	6.687	1649	1663	1687	rBV	183964	360530	47.42%	6.118%
38	6.793	1693	1696	1697	rBV	355	185	0.02%	0.003%
39	6.925	1734	1737	1741	rVB2	268	168	0.02%	0.003%
40	6.973	1750	1752	1758	rVB	233	183	0.02%	0.003%
41	7.015	1758	1765	1771	rVB2	281	371	0.05%	0.006%
42	7.063	1771	1780	1782	rBV	264	329	0.04%	0.006%
43	7.134	1796	1802	1805	rBV2	298	321	0.04%	0.005%
44	7.189	1812	1819	1822	rBV5	808	1039	0.14%	0.018%
45	7.276	1843	1846	1849	rBV	273	178	0.02%	0.003%
46	7.301	1851	1854	1858	rVB2	377	289	0.04%	0.005%
47	7.439	1893	1897	1901	rVB	260	235	0.03%	0.004%
48	7.562	1923	1935	1949	rBV	76951	133778	17.59%	2.270%
49	7.893	2025	2038	2060	rBV	340950	586553	77.14%	9.953%
50	8.060	2084	2090	2094	rVB3	383	411	0.05%	0.007%
51	8.089	2094	2099	2103	rBV2	475	308	0.04%	0.005%
52	8.176	2115	2126	2144	rVV	52550	90978	11.97%	1.544%
53	8.324	2168	2172	2174	rVB2	242	170	0.02%	0.003%
54	8.417	2198	2201	2206	rBV	251	202	0.03%	0.003%
55	8.491	2221	2224	2230	rVB	314	324	0.04%	0.005%
56	8.523	2230	2234	2238	rBV	269	190	0.02%	0.003%
57	8.552	2238	2243	2246	rBV3	467	387	0.05%	0.007%
58	8.571	2247	2249	2255	rVB2	175	187	0.02%	0.003%
59	8.629	2255	2267	2299	rBV2	178021	367798	48.37%	6.241%
60	8.851	2332	2336	2338	rBV	364	277	0.04%	0.005%
61	8.964	2367	2371	2376	rBV2	311	357	0.05%	0.006%
62	9.144	2423	2427	2431	rBV	242	176	0.02%	0.003%
63	9.414	2498	2511	2531	rBV	361050	609381	80.15%	10.341%
64	9.690	2593	2597	2598	rBV	238	201	0.03%	0.003%
65	9.886	2655	2658	2663	rVV2	227	243	0.03%	0.004%
66	9.944	2672	2676	2678	rBV	274	159	0.02%	0.003%
67	10.018	2695	2699	2701	rBV	270	214	0.03%	0.004%
68	10.192	2748	2753	2757	rBV2	285	324	0.04%	0.005%
69	10.304	2784	2788	2790	rBV	227	159	0.02%	0.003%
70	10.381	2809	2812	2817	rVB2	240	204	0.03%	0.003%
71	10.420	2821	2824	2829	rVB	218	213	0.03%	0.004%
72	10.504	2847	2850	2854	rVB	268	164	0.02%	0.003%
73	10.578	2870	2873	2875	rBV	192	166	0.02%	0.003%
74	10.642	2889	2893	2895	rBV2	368	323	0.04%	0.005%
75	10.751	2915	2927	2945	rBV	255359	408448	53.72%	6.931%
76	11.089	3030	3032	3035	rBV2	287	160	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032823\
 Data File : VU053436.D
 Acq On : 28 Mar 2023 16:17
 Operator : JC/MD
 Sample : 02037-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E45E8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

77	11.240	3076	3079	3082	rVB	324	205	0.03%	0.003%
78	11.385	3121	3124	3129	rVB2	250	209	0.03%	0.004%
79	11.471	3149	3151	3158	rVB	283	256	0.03%	0.004%
80	11.594	3186	3189	3192	rBV	323	176	0.02%	0.003%
81	11.690	3214	3219	3223	rBV3	589	625	0.08%	0.011%
82	11.709	3223	3225	3229	rVV	387	208	0.03%	0.004%
83	11.806	3244	3255	3276	rBV	351523	569562	74.91%	9.665%
84	12.002	3311	3316	3320	rBV2	229	261	0.03%	0.004%
85	12.079	3331	3340	3347	rBV8	2033	3707	0.49%	0.063%
86	12.188	3362	3374	3395	rBV	321399	536129	70.51%	9.098%
87	12.362	3425	3428	3432	rBV2	215	213	0.03%	0.004%
88	12.690	3527	3530	3532	rBV	323	205	0.03%	0.003%
89	12.729	3540	3542	3548	rVB	381	284	0.04%	0.005%
90	12.767	3548	3554	3563	rBV3	816	1315	0.17%	0.022%
91	12.844	3575	3578	3582	rVB	334	186	0.02%	0.003%
92	12.870	3582	3586	3587	rBV	195	173	0.02%	0.003%
93	12.886	3587	3591	3592	rBV2	1400	856	0.11%	0.015%
94	13.034	3634	3637	3640	rBV	339	188	0.02%	0.003%
95	13.626	3817	3821	3825	rBV2	289	297	0.04%	0.005%
96	13.777	3865	3868	3871	rBV2	379	290	0.04%	0.005%
97	13.841	3881	3888	3899	rVB6	3953	6252	0.82%	0.106%
98	13.925	3911	3914	3920	rBV2	382	302	0.04%	0.005%
99	14.163	3985	3988	3991	rBV	320	252	0.03%	0.004%
100	14.426	4066	4070	4071	rBV	449	281	0.04%	0.005%




Sum of corrected areas: 5893077

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032823\
Data File : VU053436.D
Acq On : 28 Mar 2023 16:17
Operator : JC/MD
Sample : 02037-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E45E8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

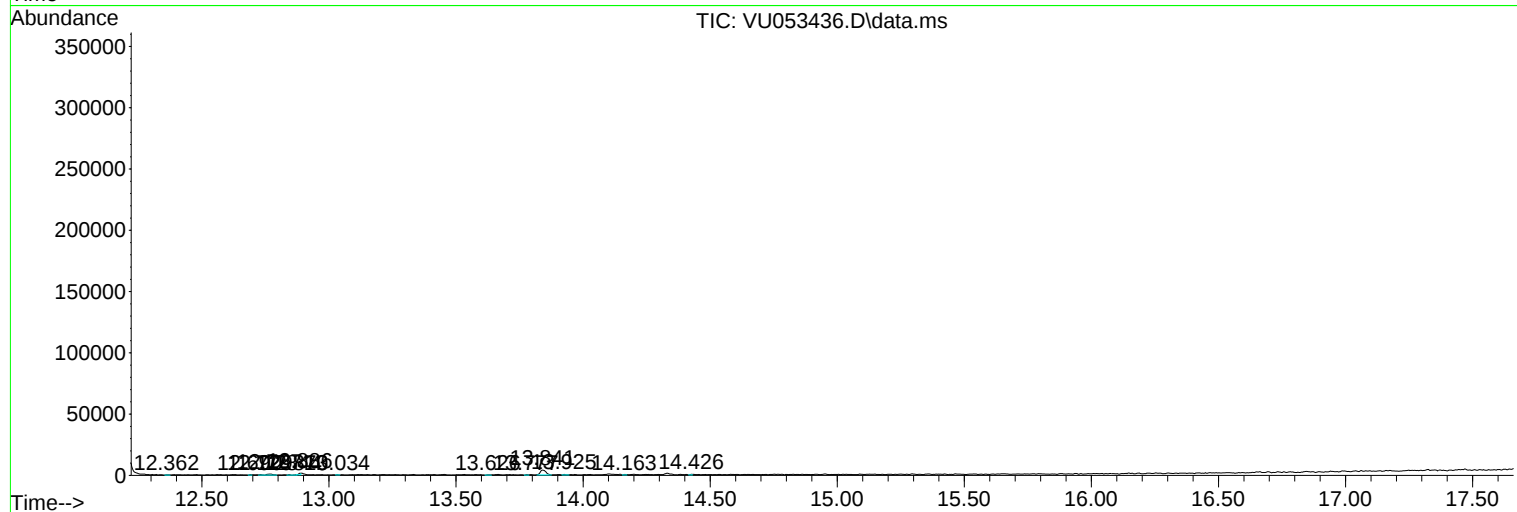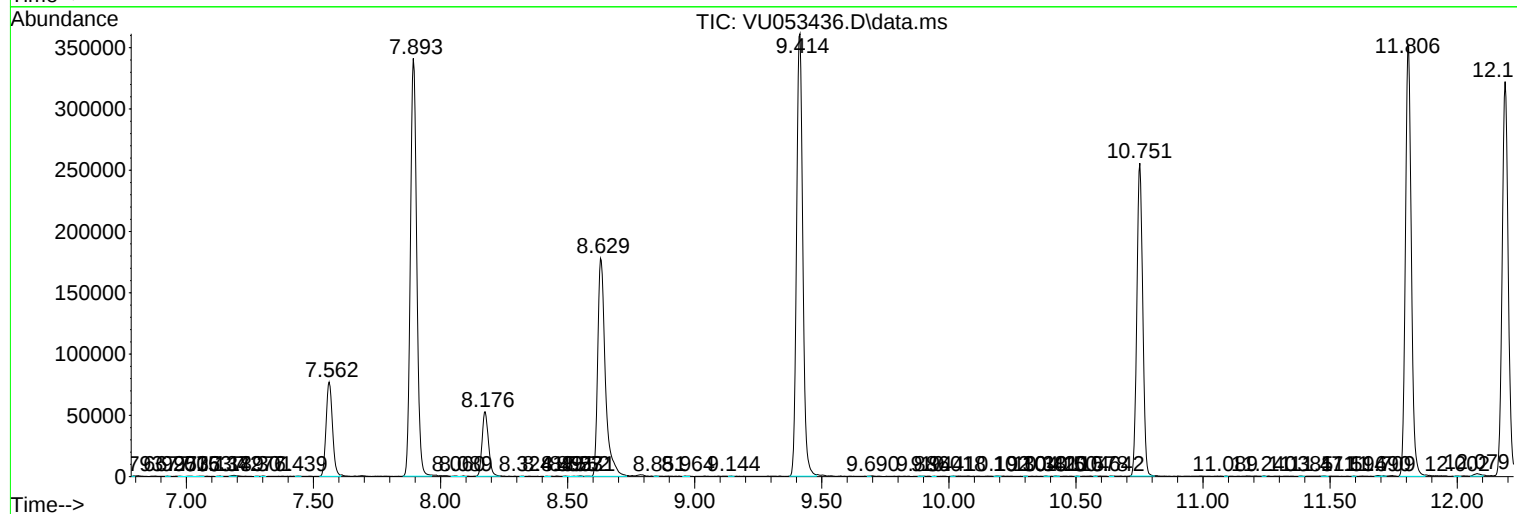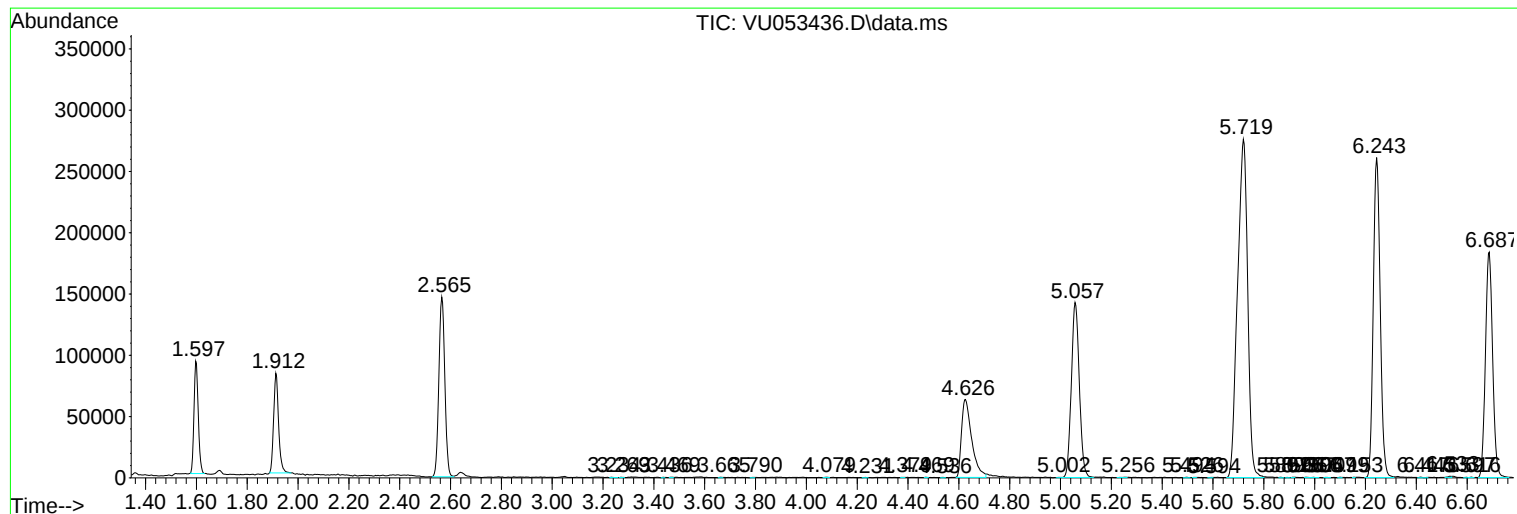

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032823\
Data File : VU053436.D
Acq On : 28 Mar 2023 16:17
Operator : JC/MD
Sample : 02037-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E45E8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032823\
Data File : VU053436.D
Acq On : 28 Mar 2023 16:17
Operator : JC/MD
Sample : 02037-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E45E8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------