

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032823\
 Data File : VU053438.D
 Acq On : 28 Mar 2023 17:04
 Operator : JC/MD
 Sample : 02037-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E45E9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

Signal : TIC: VU053438.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	97	rVB	115374	136562	16.52%	2.213%
2	1.913	171	178	193	rVB	89244	122669	14.84%	1.988%
3	2.565	369	381	399	rBV	177313	282226	34.13%	4.574%
4	3.212	579	582	586	rBV2	207	156	0.02%	0.003%
5	3.240	587	591	594	rVB	255	178	0.02%	0.003%
6	3.292	605	607	612	rVB2	163	129	0.02%	0.002%
7	3.327	612	618	619	rBV	202	200	0.02%	0.003%
8	3.478	662	665	668	rVB	292	159	0.02%	0.003%
9	3.501	668	672	673	rBV	209	152	0.02%	0.002%
10	3.546	682	686	688	rBV	150	139	0.02%	0.002%
11	3.591	697	700	704	rVB2	457	285	0.03%	0.005%
12	4.157	871	876	878	rBV	331	335	0.04%	0.005%
13	4.253	901	906	910	rVB2	265	288	0.03%	0.005%
14	4.314	923	925	932	rVB2	331	221	0.03%	0.004%
15	4.375	940	944	949	rBV2	336	307	0.04%	0.005%
16	4.475	971	975	979	rBV	288	268	0.03%	0.004%
17	4.623	1009	1021	1053	rBV	64336	172457	20.86%	2.795%
18	4.912	1108	1111	1115	rBV2	372	279	0.03%	0.005%
19	4.993	1133	1136	1140	rBV2	228	221	0.03%	0.004%
20	5.057	1140	1156	1179	rBV	148784	327674	39.63%	5.310%
21	5.186	1193	1196	1201	rBV2	259	198	0.02%	0.003%
22	5.260	1215	1219	1221	rBV	182	167	0.02%	0.003%
23	5.311	1232	1235	1238	rBV	276	202	0.02%	0.003%
24	5.507	1293	1296	1299	rBV2	241	219	0.03%	0.004%
25	5.543	1305	1307	1312	rVB2	211	179	0.02%	0.003%
26	5.649	1337	1340	1342	rBV2	230	160	0.02%	0.003%
27	5.719	1342	1362	1390	rVV3	305727	826848	100.00%	13.400%
28	5.835	1396	1398	1402	rVB	427	190	0.02%	0.003%
29	5.935	1427	1429	1434	rVB	362	234	0.03%	0.004%
30	5.964	1434	1438	1439	rBV	167	132	0.02%	0.002%
31	5.970	1439	1440	1448	rVB2	279	213	0.03%	0.003%
32	6.031	1457	1459	1462	rBV2	216	143	0.02%	0.002%
33	6.083	1471	1475	1477	rBV2	161	134	0.02%	0.002%
34	6.137	1490	1492	1495	rBV	193	148	0.02%	0.002%
35	6.244	1512	1525	1548	rVV	244504	458320	55.43%	7.427%
36	6.517	1608	1610	1612	rBV2	548	306	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032823\
 Data File : VU053438.D
 Acq On : 28 Mar 2023 17:04
 Operator : JC/MD
 Sample : 02037-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E45E9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

37	6.584	1628	1631	1633	rBV	199	130	0.02%	0.002%
38	6.684	1649	1662	1687	rBV	196815	381759	46.17%	6.187%
39	6.938	1738	1741	1747	rVB	206	183	0.02%	0.003%
40	6.977	1747	1753	1754	rBV	185	151	0.02%	0.002%
41	7.080	1781	1785	1789	rBV	306	334	0.04%	0.005%
42	7.153	1803	1808	1811	rBV	202	195	0.02%	0.003%
43	7.189	1811	1819	1820	rBV3	515	545	0.07%	0.009%
44	7.260	1837	1841	1845	rVV2	180	174	0.02%	0.003%
45	7.282	1845	1848	1851	rVB2	200	139	0.02%	0.002%
46	7.401	1882	1885	1887	rBV	241	139	0.02%	0.002%
47	7.440	1894	1897	1901	rVB2	217	141	0.02%	0.002%
48	7.472	1904	1907	1912	rVB2	194	199	0.02%	0.003%
49	7.501	1912	1916	1918	rBV2	295	206	0.02%	0.003%
50	7.562	1923	1935	1955	rBV	107660	190155	23.00%	3.082%
51	7.780	1998	2003	2005	rBV2	260	204	0.02%	0.003%
52	7.893	2023	2038	2058	rBV	377888	655725	79.30%	10.627%
53	8.089	2096	2099	2101	rBV	221	154	0.02%	0.002%
54	8.173	2114	2125	2152	rBV	74427	128241	15.51%	2.078%
55	8.462	2212	2215	2217	rVB	274	157	0.02%	0.003%
56	8.481	2217	2221	2223	rVB	274	171	0.02%	0.003%
57	8.523	2232	2234	2237	rVB	249	134	0.02%	0.002%
58	8.542	2237	2240	2244	rBV2	245	231	0.03%	0.004%
59	8.629	2256	2267	2297	rBV3	180055	359062	43.43%	5.819%
60	8.835	2328	2331	2335	rVB2	451	364	0.04%	0.006%
61	8.922	2354	2358	2361	rBV2	227	203	0.02%	0.003%
62	9.054	2394	2399	2405	rBV	361	405	0.05%	0.007%
63	9.137	2422	2425	2430	rBV	244	199	0.02%	0.003%
64	9.333	2484	2486	2490	rVB2	265	154	0.02%	0.002%
65	9.414	2498	2511	2536	rBV	335129	564280	68.24%	9.145%
66	9.613	2569	2573	2576	rBV2	217	157	0.02%	0.003%
67	9.661	2585	2588	2591	rVB2	225	137	0.02%	0.002%
68	9.755	2611	2617	2620	rBV2	206	228	0.03%	0.004%
69	9.790	2626	2628	2630	rBV	206	139	0.02%	0.002%
70	9.845	2640	2645	2647	rBV2	233	198	0.02%	0.003%
71	10.067	2711	2714	2718	rBV	282	225	0.03%	0.004%
72	10.102	2722	2725	2728	rBV	370	226	0.03%	0.004%
73	10.163	2741	2744	2746	rBV2	208	141	0.02%	0.002%
74	10.214	2757	2760	2763	rBV	262	185	0.02%	0.003%
75	10.301	2785	2787	2790	rBV	161	141	0.02%	0.002%
76	10.391	2812	2815	2818	rBV2	173	137	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032823\
 Data File : VU053438.D
 Acq On : 28 Mar 2023 17:04
 Operator : JC/MD
 Sample : 02037-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E45E9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

77	10.517	2851	2854	2859	rBV2	195	161	0.02%	0.003%
78	10.751	2912	2927	2942	rBV	256763	410422	49.64%	6.651%
79	10.829	2949	2951	2953	rBV	365	173	0.02%	0.003%
80	10.915	2976	2978	2981	rBV2	234	166	0.02%	0.003%
81	10.976	2995	2997	3000	rVB	301	185	0.02%	0.003%
82	11.134	3041	3046	3050	rBV2	332	347	0.04%	0.006%
83	11.298	3094	3097	3101	rBV2	246	186	0.02%	0.003%
84	11.472	3147	3151	3153	rBV	347	233	0.03%	0.004%
85	11.587	3184	3187	3191	rVB2	269	209	0.03%	0.003%
86	11.632	3198	3201	3204	rBV	298	172	0.02%	0.003%
87	11.739	3228	3234	3242	rVB6	1927	2534	0.31%	0.041%
88	11.806	3243	3255	3280	rBV	340691	546184	66.06%	8.851%
89	12.005	3315	3317	3319	rVB	307	143	0.02%	0.002%
90	12.189	3362	3374	3393	rBV	359074	585632	70.83%	9.491%
91	12.349	3421	3424	3432	rVB2	345	488	0.06%	0.008%
92	12.388	3432	3436	3438	rBV2	372	261	0.03%	0.004%
93	12.825	3570	3572	3577	rVB	256	149	0.02%	0.002%
94	13.163	3673	3677	3683	rBV3	379	473	0.06%	0.008%
95	13.452	3762	3767	3769	rBV	354	308	0.04%	0.005%
96	13.510	3781	3785	3788	rBV	326	322	0.04%	0.005%
97	13.841	3883	3888	3898	rVB4	1768	2471	0.30%	0.040%
98	13.886	3898	3902	3905	rBV2	330	258	0.03%	0.004%
99	13.957	3922	3924	3928	rBV2	262	222	0.03%	0.004%
100	14.198	3996	3999	4001	rBV	280	144	0.02%	0.002%


Sum of corrected areas: 6170589

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032823\
Data File : VU053438.D
Acq On : 28 Mar 2023 17:04
Operator : JC/MD
Sample : 02037-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E45E9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

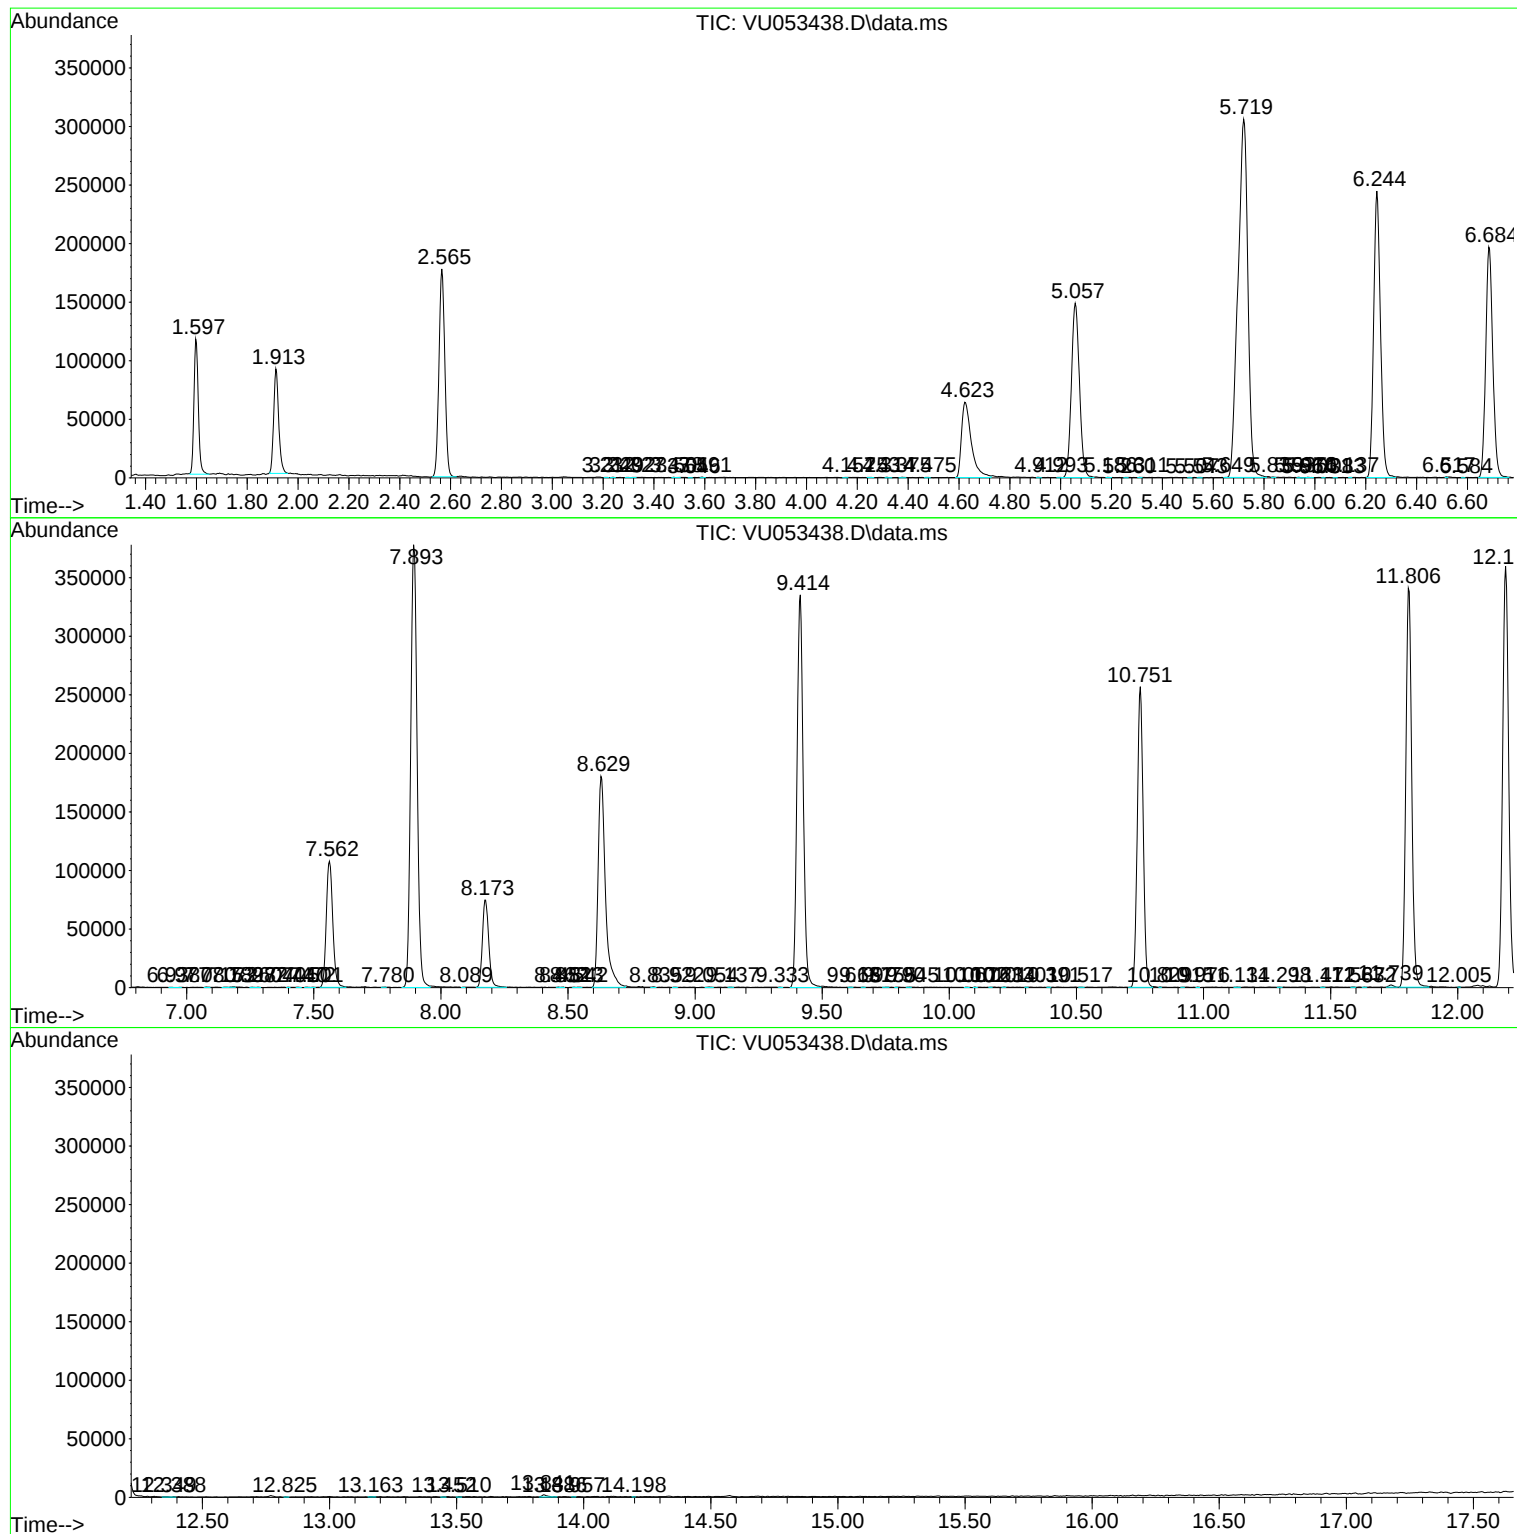

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032823\
Data File : VU053438.D
Acq On : 28 Mar 2023 17:04
Operator : JC/MD
Sample : 02037-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E45E9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032823\
Data File : VU053438.D
Acq On : 28 Mar 2023 17:04
Operator : JC/MD
Sample : 02037-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E45E9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------