

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032823\
 Data File : VU053439.D
 Acq On : 28 Mar 2023 17:27
 Operator : JC/MD
 Sample : 02037-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E45F0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M

Title : VOC Analysis

Signal : TIC: VU053439.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	42	45	50	rBV	798	844	0.10%	0.013%
2	1.597	72	80	92	rBV	117029	138174	16.33%	2.180%
3	1.912	169	178	195	rBV	95210	131797	15.57%	2.080%
4	2.565	369	381	395	rBV	176472	285530	33.74%	4.506%
5	2.790	448	451	453	rBV2	337	199	0.02%	0.003%
6	2.874	473	477	482	rVB2	370	363	0.04%	0.006%
7	2.916	487	490	494	rBV	353	211	0.02%	0.003%
8	2.938	495	497	501	rBV	203	172	0.02%	0.003%
9	3.009	517	519	521	rVV	262	180	0.02%	0.003%
10	3.044	524	530	536	rVV3	1017	1163	0.14%	0.018%
11	3.076	537	540	544	rVB2	345	206	0.02%	0.003%
12	3.195	574	577	583	rVB	492	399	0.05%	0.006%
13	3.375	630	633	638	rBV2	266	281	0.03%	0.004%
14	3.578	692	696	701	rVB2	208	256	0.03%	0.004%
15	3.620	705	709	714	rVV	245	214	0.03%	0.003%
16	3.668	720	724	728	rVB	359	302	0.04%	0.005%
17	3.877	786	789	794	rBV	303	274	0.03%	0.004%
18	4.102	854	859	861	rBV	213	184	0.02%	0.003%
19	4.478	972	976	979	rBV	232	185	0.02%	0.003%
20	4.565	994	1003	1006	rBV	426	557	0.07%	0.009%
21	4.626	1007	1022	1048	rBV	67203	178347	21.07%	2.814%
22	4.870	1092	1098	1100	rBV2	278	285	0.03%	0.004%
23	4.896	1104	1106	1112	rVB2	216	184	0.02%	0.003%
24	5.057	1141	1156	1178	rVV	152640	334310	39.50%	5.275%
25	5.311	1231	1235	1240	rBV2	330	296	0.03%	0.005%
26	5.398	1260	1262	1269	rVB2	268	212	0.03%	0.003%
27	5.436	1269	1274	1280	rVB2	266	340	0.04%	0.005%
28	5.719	1341	1362	1389	rBV2	309377	846327	100.00%	13.355%
29	6.038	1456	1461	1463	rBV	355	309	0.04%	0.005%
30	6.166	1497	1501	1503	rVB	251	172	0.02%	0.003%
31	6.243	1508	1525	1543	rBV	250011	472496	55.83%	7.456%
32	6.520	1608	1611	1618	rVB4	658	738	0.09%	0.012%
33	6.687	1648	1663	1686	rBV	198749	390949	46.19%	6.169%
34	6.790	1692	1695	1697	rBV2	323	193	0.02%	0.003%
35	6.809	1697	1701	1705	rVB3	426	349	0.04%	0.006%
36	6.903	1727	1730	1735	rVB	210	215	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032823\
 Data File : VU053439.D
 Acq On : 28 Mar 2023 17:27
 Operator : JC/MD
 Sample : 02037-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E45F0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

37	6.967	1747	1750	1753	rVB	291	179	0.02%	0.003%
38	7.018	1762	1766	1769	rVV2	187	185	0.02%	0.003%
39	7.192	1814	1820	1825	rVV4	839	955	0.11%	0.015%
40	7.317	1855	1859	1864	rVB	347	242	0.03%	0.004%
41	7.398	1878	1884	1889	rBV2	264	306	0.04%	0.005%
42	7.446	1894	1899	1904	rBV	362	314	0.04%	0.005%
43	7.481	1907	1910	1913	rBV	210	171	0.02%	0.003%
44	7.562	1922	1935	1959	rBV	110009	196484	23.22%	3.100%
45	7.648	1959	1962	1965	rVB	231	175	0.02%	0.003%
46	7.693	1970	1976	1982	rBV3	747	865	0.10%	0.014%
47	7.809	2007	2012	2015	rBV2	244	266	0.03%	0.004%
48	7.893	2024	2038	2062	rBV	389262	667815	78.91%	10.538%
49	8.176	2114	2126	2143	rVV	76959	131660	15.56%	2.078%
50	8.433	2203	2206	2211	rBV2	191	187	0.02%	0.003%
51	8.459	2211	2214	2216	rBV2	295	221	0.03%	0.003%
52	8.558	2242	2245	2250	rBV	250	181	0.02%	0.003%
53	8.629	2256	2267	2298	rBV3	187843	374139	44.21%	5.904%
54	8.790	2312	2317	2323	rVB2	357	307	0.04%	0.005%
55	8.816	2323	2325	2328	rBV	320	186	0.02%	0.003%
56	8.944	2362	2365	2368	rBV	295	196	0.02%	0.003%
57	9.025	2386	2390	2396	rBV2	264	334	0.04%	0.005%
58	9.173	2433	2436	2441	rVB2	240	199	0.02%	0.003%
59	9.218	2447	2450	2455	rBV2	273	261	0.03%	0.004%
60	9.253	2455	2461	2465	rVV	303	290	0.03%	0.005%
61	9.414	2496	2511	2533	rBV	349047	578295	68.33%	9.125%
62	9.758	2615	2618	2620	rVB	262	177	0.02%	0.003%
63	9.980	2683	2687	2692	rBV	259	252	0.03%	0.004%
64	10.172	2744	2747	2750	rBV2	266	183	0.02%	0.003%
65	10.217	2756	2761	2764	rBV2	241	235	0.03%	0.004%
66	10.237	2765	2767	2773	rVV2	285	294	0.03%	0.005%
67	10.401	2815	2818	2824	rVB2	226	170	0.02%	0.003%
68	10.433	2824	2828	2831	rBV2	228	210	0.02%	0.003%
69	10.751	2914	2927	2945	rVV	266014	425380	50.26%	6.712%
70	10.832	2949	2952	2955	rVB2	369	196	0.02%	0.003%
71	10.886	2966	2969	2978	rVB3	288	366	0.04%	0.006%
72	10.938	2978	2985	2988	rBV2	316	397	0.05%	0.006%
73	11.121	3039	3042	3046	rBV2	282	218	0.03%	0.003%
74	11.201	3062	3067	3073	rBV2	235	371	0.04%	0.006%
75	11.269	3085	3088	3092	rVB2	270	210	0.02%	0.003%
76	11.333	3104	3108	3111	rBV	323	209	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032823\
 Data File : VU053439.D
 Acq On : 28 Mar 2023 17:27
 Operator : JC/MD
 Sample : 02037-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E45F0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

77	11.745	3233	3236	3242	rVB3	821	776	0.09%	0.012%
78	11.806	3242	3255	3274	rBV	351619	560693	66.25%	8.848%
79	12.037	3324	3327	3329	rBV	324	205	0.02%	0.003%
80	12.079	3329	3340	3354	rVV6	1947	4766	0.56%	0.075%
81	12.188	3361	3374	3388	rBV	360729	592159	69.97%	9.344%
82	12.275	3399	3401	3405	rVB3	458	316	0.04%	0.005%
83	12.452	3452	3456	3458	rBV2	210	203	0.02%	0.003%
84	12.507	3469	3473	3476	rBV2	229	187	0.02%	0.003%
85	12.770	3546	3555	3558	rVV2	1142	1552	0.18%	0.024%
86	13.237	3697	3700	3703	rBV2	323	205	0.02%	0.003%
87	13.565	3799	3802	3806	rBV	280	213	0.03%	0.003%
88	13.809	3873	3878	3880	rBV2	236	234	0.03%	0.004%
89	13.848	3885	3890	3900	rVB3	942	1223	0.14%	0.019%
90	13.941	3917	3919	3923	rBV	211	193	0.02%	0.003%
91	14.024	3943	3945	3949	rBV2	319	217	0.03%	0.003%
92	14.114	3965	3973	3978	rBV4	747	1224	0.14%	0.019%
93	14.156	3982	3986	3988	rVB	354	219	0.03%	0.003%
94	14.266	4017	4020	4022	rVB	330	177	0.02%	0.003%
95	14.359	4046	4049	4054	rBV	265	211	0.02%	0.003%
96	14.458	4075	4080	4082	rBV2	428	409	0.05%	0.006%
97	14.629	4131	4133	4136	rVB2	379	223	0.03%	0.004%
98	14.774	4175	4178	4180	rBV2	291	183	0.02%	0.003%
99	15.031	4254	4258	4259	rBV2	427	353	0.04%	0.006%
100	16.037	4567	4571	4572	rBV2	755	584	0.07%	0.009%




Sum of corrected areas: 6337219

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032823\
Data File : VU053439.D
Acq On : 28 Mar 2023 17:27
Operator : JC/MD
Sample : 02037-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E45F0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

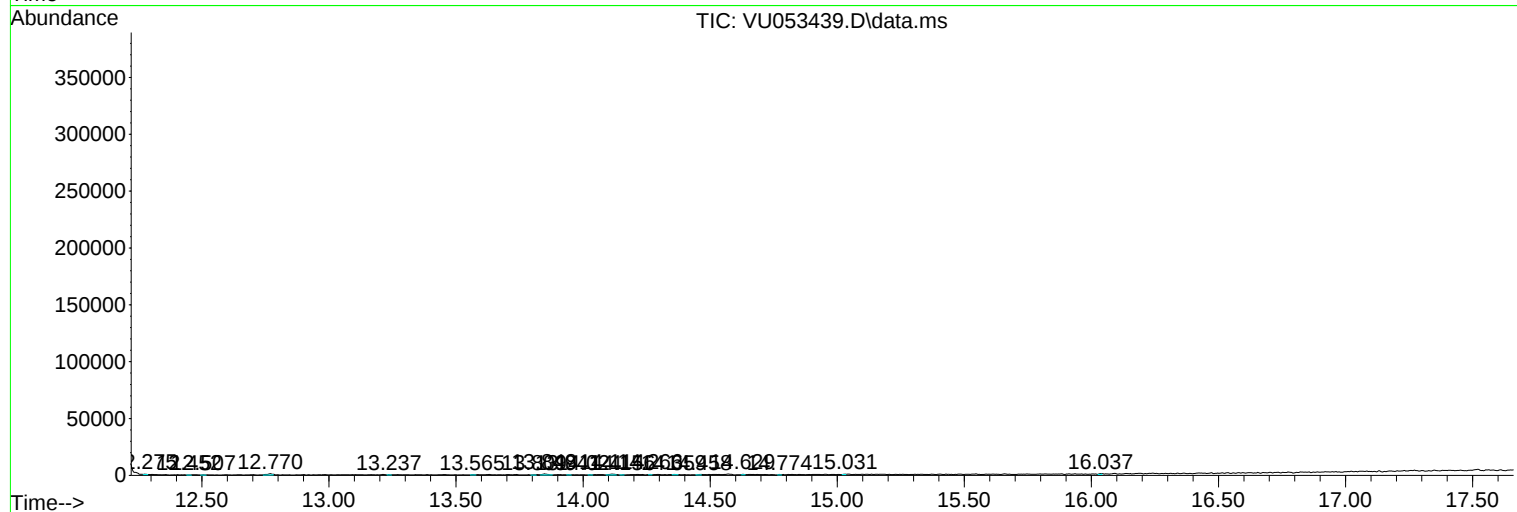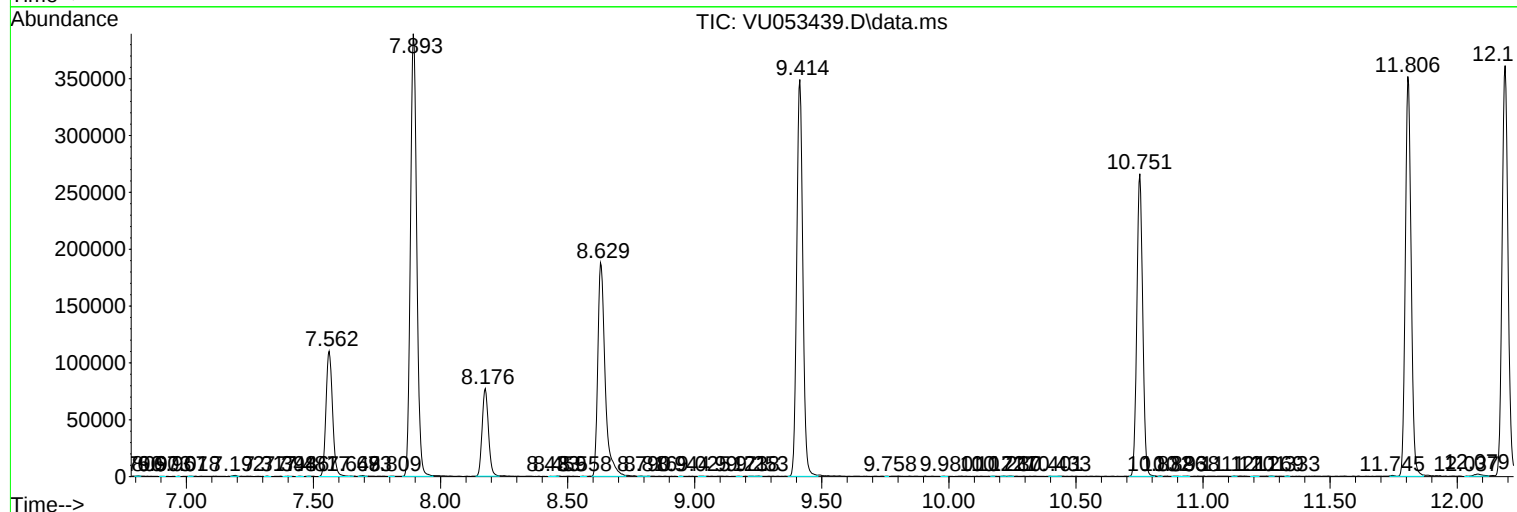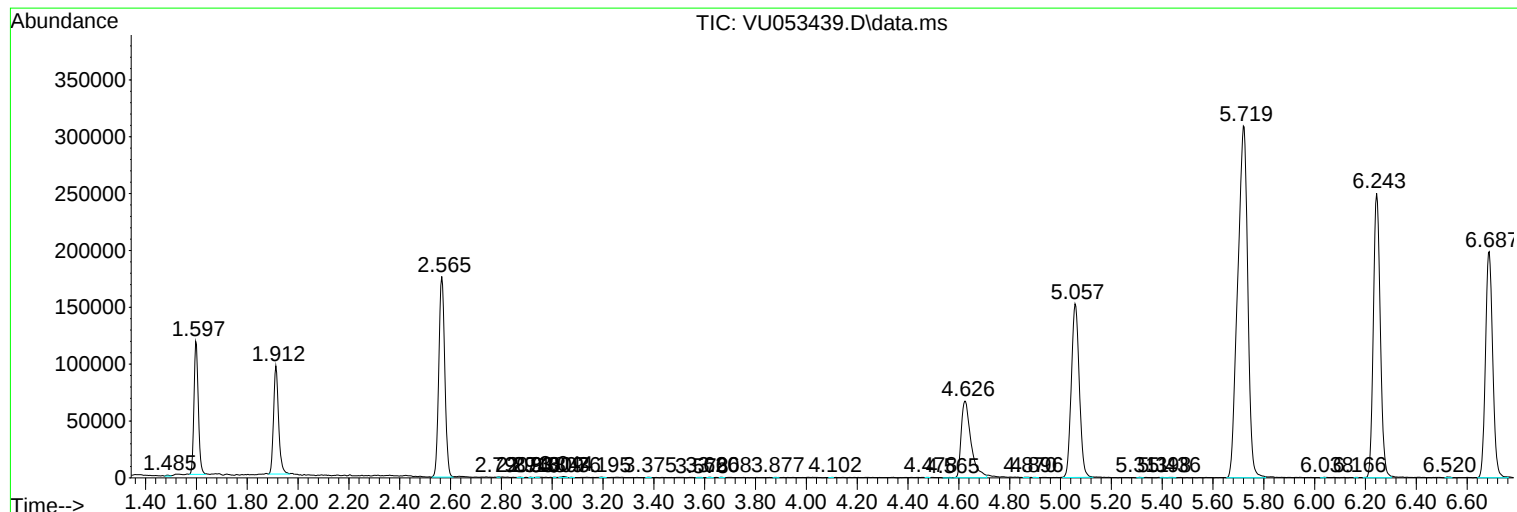

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032823\
Data File : VU053439.D
Acq On : 28 Mar 2023 17:27
Operator : JC/MD
Sample : 02037-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E45F0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032823\
Data File : VU053439.D
Acq On : 28 Mar 2023 17:27
Operator : JC/MD
Sample : 02037-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E45F0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------