

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032823\
 Data File : VU053440.D
 Acq On : 28 Mar 2023 17:50
 Operator : JC/MD
 Sample : 02037-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E45F1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

Signal : TIC: VU053440.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	96	rVB	119606	140894	16.67%	2.229%
2	1.912	171	178	192	rVB	93807	125359	14.83%	1.983%
3	2.565	369	381	395	rBV	183643	293872	34.77%	4.649%
4	2.732	427	433	437	rBV2	484	469	0.06%	0.007%
5	2.960	498	504	507	rBV	529	443	0.05%	0.007%
6	2.993	511	514	517	rBV2	270	211	0.02%	0.003%
7	3.038	526	528	529	rBV	527	246	0.03%	0.004%
8	3.076	538	540	544	rVB	301	230	0.03%	0.004%
9	3.140	556	560	562	rBV	209	145	0.02%	0.002%
10	3.176	565	571	573	rBV2	499	540	0.06%	0.009%
11	3.276	600	602	604	rVB2	333	152	0.02%	0.002%
12	3.372	630	632	639	rVV	236	298	0.04%	0.005%
13	3.623	706	710	716	rBV3	371	368	0.04%	0.006%
14	3.677	724	727	729	rBV	296	201	0.02%	0.003%
15	3.748	746	749	754	rBV2	202	223	0.03%	0.004%
16	3.845	775	779	782	rBV	365	305	0.04%	0.005%
17	4.272	907	912	917	rVB2	266	374	0.04%	0.006%
18	4.317	925	926	929	rBV2	272	189	0.02%	0.003%
19	4.407	951	954	959	rBV	223	167	0.02%	0.003%
20	4.433	959	962	965	rBV	249	233	0.03%	0.004%
21	4.623	1009	1021	1057	rBV	64360	170753	20.20%	2.701%
22	4.835	1084	1087	1090	rBV2	325	214	0.03%	0.003%
23	4.954	1121	1124	1127	rVB2	301	191	0.02%	0.003%
24	5.057	1140	1156	1182	rBV2	153423	336351	39.80%	5.321%
25	5.176	1189	1193	1198	rVB2	256	248	0.03%	0.004%
26	5.202	1198	1201	1204	rBV3	338	300	0.04%	0.005%
27	5.288	1224	1228	1231	rBV2	174	143	0.02%	0.002%
28	5.639	1332	1337	1341	rVB2	230	198	0.02%	0.003%
29	5.719	1341	1362	1387	rBV2	311969	845206	100.00%	13.371%
30	5.912	1420	1422	1425	rBV2	251	159	0.02%	0.003%
31	5.970	1434	1440	1444	rBV2	204	213	0.03%	0.003%
32	6.034	1458	1460	1463	rVB	310	217	0.03%	0.003%
33	6.128	1483	1489	1491	rBV3	406	435	0.05%	0.007%
34	6.243	1511	1525	1549	rBV	255924	478496	56.61%	7.570%
35	6.455	1587	1591	1596	rBV2	358	286	0.03%	0.005%
36	6.529	1609	1614	1616	rBV3	422	435	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032823\
 Data File : VU053440.D
 Acq On : 28 Mar 2023 17:50
 Operator : JC/MD
 Sample : 02037-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E45F1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

37	6.613	1638	1640	1645	rBV2	242	164	0.02%	0.003%
38	6.687	1649	1663	1683	rBV	197832	388763	46.00%	6.150%
39	6.800	1695	1698	1699	rBV	254	148	0.02%	0.002%
40	6.890	1724	1726	1729	rBV	281	203	0.02%	0.003%
41	7.060	1775	1779	1785	rVB2	248	256	0.03%	0.004%
42	7.105	1785	1793	1797	rBV2	194	333	0.04%	0.005%
43	7.160	1806	1810	1812	rBV2	270	222	0.03%	0.004%
44	7.285	1843	1849	1851	rBV2	251	231	0.03%	0.004%
45	7.317	1856	1859	1864	rVB2	263	257	0.03%	0.004%
46	7.410	1885	1888	1895	rBV2	287	285	0.03%	0.005%
47	7.562	1921	1935	1954	rVV	110313	194644	23.03%	3.079%
48	7.726	1983	1986	1987	rBV2	209	145	0.02%	0.002%
49	7.751	1991	1994	1997	rBV2	195	159	0.02%	0.003%
50	7.816	2011	2014	2017	rVB	270	199	0.02%	0.003%
51	7.893	2025	2038	2058	rBV	391460	669616	79.23%	10.593%
52	8.066	2090	2092	2096	rVB	296	151	0.02%	0.002%
53	8.176	2111	2126	2148	rBV	77106	130653	15.46%	2.067%
54	8.365	2180	2185	2188	rBV2	316	263	0.03%	0.004%
55	8.414	2197	2200	2203	rVB2	239	148	0.02%	0.002%
56	8.478	2213	2220	2223	rVB2	677	632	0.07%	0.010%
57	8.513	2228	2231	2233	rBV2	176	150	0.02%	0.002%
58	8.555	2240	2244	2252	rVB2	315	375	0.04%	0.006%
59	8.629	2252	2267	2299	rBV2	182006	362569	42.90%	5.736%
60	8.787	2310	2316	2319	rBV3	969	1062	0.13%	0.017%
61	8.880	2340	2345	2346	rVB	227	161	0.02%	0.003%
62	8.938	2361	2363	2369	rVB	232	143	0.02%	0.002%
63	8.996	2379	2381	2389	rVB	356	195	0.02%	0.003%
64	9.041	2390	2395	2398	rBV	375	356	0.04%	0.006%
65	9.188	2438	2441	2446	rVB2	235	220	0.03%	0.003%
66	9.214	2446	2449	2451	rBV	356	261	0.03%	0.004%
67	9.269	2463	2466	2467	rBV	254	149	0.02%	0.002%
68	9.356	2490	2493	2498	rVB	181	162	0.02%	0.003%
69	9.414	2498	2511	2534	rBV	345026	583724	69.06%	9.234%
70	9.587	2563	2565	2567	rBV2	399	173	0.02%	0.003%
71	9.690	2590	2597	2598	rBV3	571	480	0.06%	0.008%
72	9.799	2627	2631	2635	rBV	269	239	0.03%	0.004%
73	9.828	2636	2640	2644	rVV2	256	218	0.03%	0.003%
74	9.922	2665	2669	2673	rVV2	249	246	0.03%	0.004%
75	10.041	2700	2706	2710	rBV2	233	290	0.03%	0.005%
76	10.163	2740	2744	2746	rBV	189	153	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032823\
 Data File : VU053440.D
 Acq On : 28 Mar 2023 17:50
 Operator : JC/MD
 Sample : 02037-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E45F1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

77	10.240	2763	2768	2771	rBV2	313	276	0.03%	0.004%
78	10.259	2771	2774	2779	rVB	242	172	0.02%	0.003%
79	10.330	2792	2796	2798	rBV	182	157	0.02%	0.002%
80	10.500	2846	2849	2854	rVV2	284	325	0.04%	0.005%
81	10.751	2914	2927	2945	rVV	255919	411598	48.70%	6.511%
82	10.931	2979	2983	2985	rBV	187	158	0.02%	0.002%
83	11.012	3003	3008	3013	rVB2	236	341	0.04%	0.005%
84	11.076	3026	3028	3032	rBV	207	182	0.02%	0.003%
85	11.095	3032	3034	3037	rVV	335	197	0.02%	0.003%
86	11.185	3055	3062	3064	rBV2	247	334	0.04%	0.005%
87	11.375	3113	3121	3129	rBV3	1318	1616	0.19%	0.026%
88	11.687	3215	3218	3221	rBV2	235	194	0.02%	0.003%
89	11.806	3243	3255	3274	rBV	354402	563465	66.67%	8.914%
90	11.999	3311	3315	3319	rVB2	286	250	0.03%	0.004%
91	12.076	3331	3339	3342	rBV5	2536	3324	0.39%	0.053%
92	12.188	3362	3374	3391	rBV	367636	598892	70.86%	9.474%
93	12.330	3414	3418	3421	rBV3	506	442	0.05%	0.007%
94	12.455	3454	3457	3462	rBV2	269	310	0.04%	0.005%
95	12.593	3497	3500	3503	rBV2	315	192	0.02%	0.003%
96	12.973	3615	3618	3619	rBV2	375	198	0.02%	0.003%
97	13.192	3683	3686	3689	rBV	270	248	0.03%	0.004%
98	13.269	3708	3710	3714	rBV	321	182	0.02%	0.003%
99	14.359	4047	4049	4052	rBV2	298	182	0.02%	0.003%
100	14.494	4087	4091	4095	rBV3	425	421	0.05%	0.007%




Sum of corrected areas: 6321218

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032823\
Data File : VU053440.D
Acq On : 28 Mar 2023 17:50
Operator : JC/MD
Sample : 02037-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E45F1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

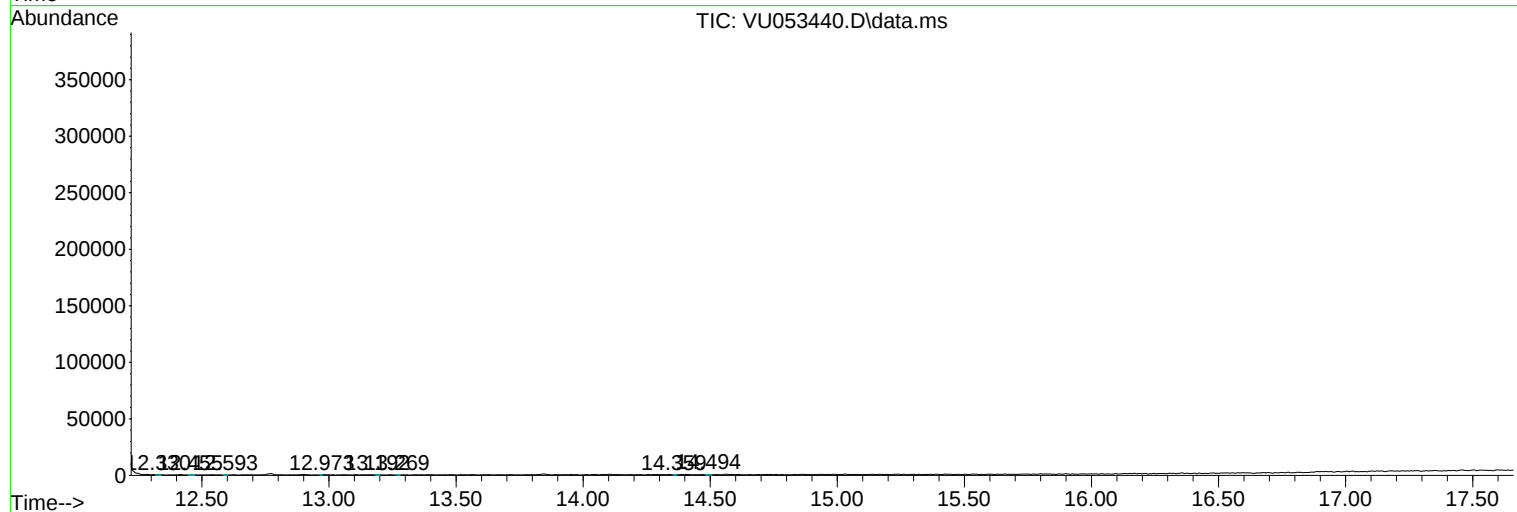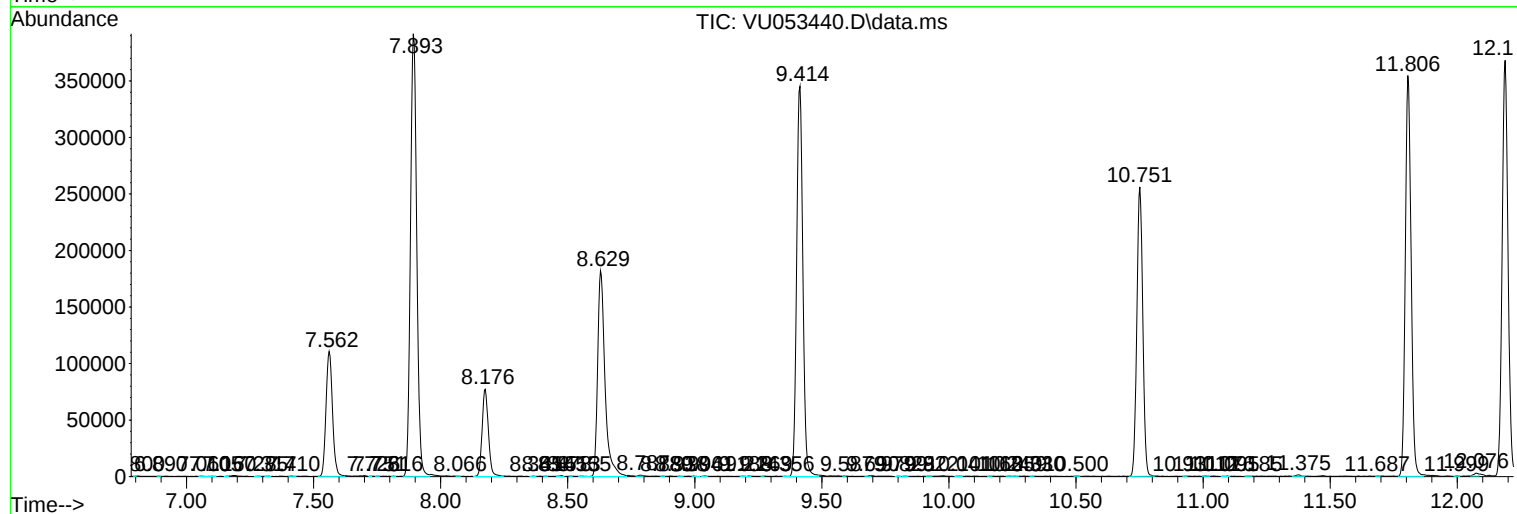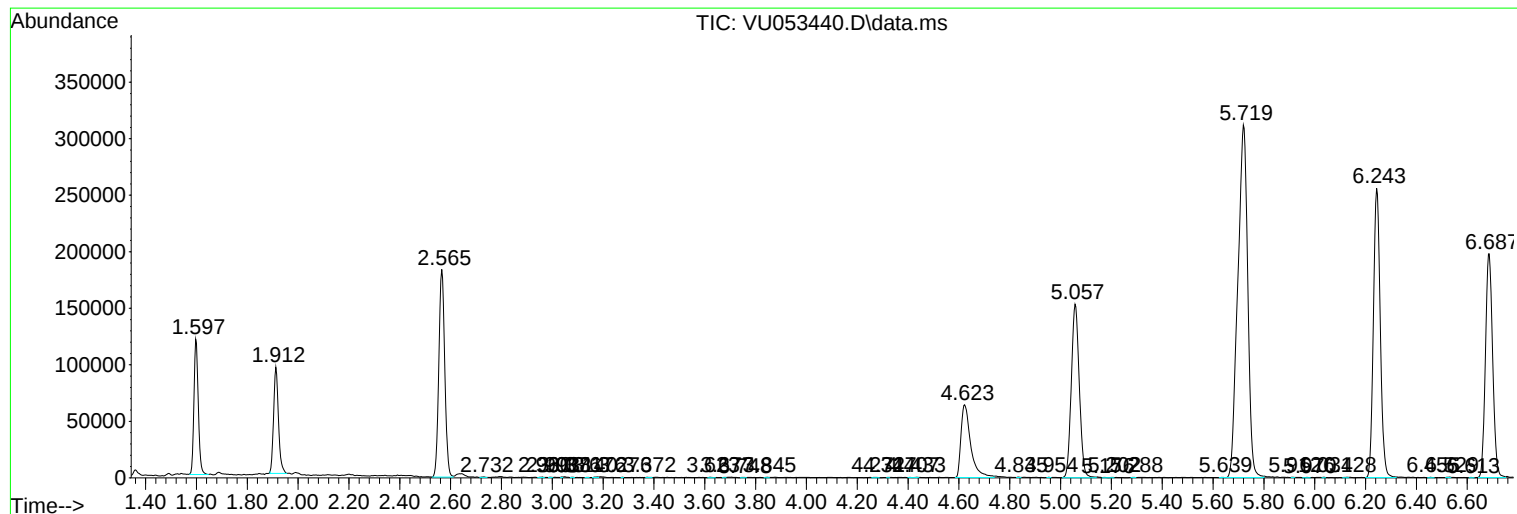

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032823\
Data File : VU053440.D
Acq On : 28 Mar 2023 17:50
Operator : JC/MD
Sample : 02037-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E45F1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032823\
Data File : VU053440.D
Acq On : 28 Mar 2023 17:50
Operator : JC/MD
Sample : 02037-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E45F1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------