

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032823\
 Data File : VU053443.D
 Acq On : 28 Mar 2023 19:01
 Operator : JC/MD
 Sample : 02054-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYF61

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

Signal : TIC: VU053443.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	95	rVB	123795	144681	16.52%	2.196%
2	1.912	171	178	196	rVB	97733	133310	15.23%	2.024%
3	2.565	369	381	397	rBV	187161	303603	34.67%	4.609%
4	2.758	439	441	446	rBV	267	228	0.03%	0.003%
5	2.896	481	484	486	rBV2	298	210	0.02%	0.003%
6	3.118	550	553	557	rBV2	264	188	0.02%	0.003%
7	3.179	561	572	574	rBV3	677	997	0.11%	0.015%
8	3.324	615	617	620	rBV2	187	102	0.01%	0.002%
9	3.523	674	679	682	rBV	311	268	0.03%	0.004%
10	3.584	696	698	700	rBV2	226	130	0.01%	0.002%
11	3.655	717	720	723	rBV	240	142	0.02%	0.002%
12	3.954	809	813	815	rBV	230	169	0.02%	0.003%
13	4.002	825	828	830	rBV	189	125	0.01%	0.002%
14	4.137	866	870	873	rBV2	249	192	0.02%	0.003%
15	4.289	914	917	920	rVB	361	216	0.02%	0.003%
16	4.318	924	926	929	rBV	179	125	0.01%	0.002%
17	4.350	933	936	938	rBV	161	130	0.01%	0.002%
18	4.462	968	971	974	rBV	182	119	0.01%	0.002%
19	4.581	1004	1008	1009	rBV	238	150	0.02%	0.002%
20	4.623	1009	1021	1050	rBV	69907	178622	20.40%	2.711%
21	4.938	1116	1119	1121	rBV2	203	131	0.01%	0.002%
22	4.986	1130	1134	1136	rBV2	298	256	0.03%	0.004%
23	5.057	1140	1156	1182	rVV	161503	352981	40.31%	5.358%
24	5.202	1198	1201	1204	rVB3	335	244	0.03%	0.004%
25	5.311	1231	1235	1242	rBV2	213	302	0.03%	0.005%
26	5.343	1242	1245	1246	rBV2	273	112	0.01%	0.002%
27	5.398	1258	1262	1268	rBV2	140	202	0.02%	0.003%
28	5.498	1290	1293	1297	rBV	278	215	0.02%	0.003%
29	5.604	1324	1326	1331	rVB2	221	167	0.02%	0.003%
30	5.719	1341	1362	1384	rVV2	323303	875575	100.00%	13.291%
31	5.964	1435	1438	1441	rVB2	162	105	0.01%	0.002%
32	5.983	1441	1444	1446	rBV2	301	179	0.02%	0.003%
33	6.028	1456	1458	1461	rBV2	206	128	0.01%	0.002%
34	6.044	1461	1463	1468	rVB2	187	124	0.01%	0.002%
35	6.099	1478	1480	1483	rVV2	207	132	0.02%	0.002%
36	6.115	1483	1485	1488	rVB2	296	155	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032823\
 Data File : VU053443.D
 Acq On : 28 Mar 2023 19:01
 Operator : JC/MD
 Sample : 02054-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYF61

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

37	6.137	1488	1492	1493	rBV	172	112	0.01%	0.002%
38	6.243	1512	1525	1551	rVV	259946	490326	56.00%	7.443%
39	6.462	1591	1593	1596	rBV2	159	108	0.01%	0.002%
40	6.536	1603	1616	1627	rVB2	3256	6447	0.74%	0.098%
41	6.591	1627	1633	1635	rBV2	409	404	0.05%	0.006%
42	6.684	1648	1662	1681	rBV	206048	401689	45.88%	6.098%
43	6.932	1737	1739	1740	rBV	257	107	0.01%	0.002%
44	6.996	1753	1759	1764	rBV2	377	504	0.06%	0.008%
45	7.044	1770	1774	1781	rVB	179	169	0.02%	0.003%
46	7.089	1781	1788	1791	rBV2	270	286	0.03%	0.004%
47	7.250	1836	1838	1841	rVB2	221	120	0.01%	0.002%
48	7.456	1897	1902	1904	rBV	199	181	0.02%	0.003%
49	7.562	1922	1935	1961	rVV	114925	204643	23.37%	3.106%
50	7.690	1967	1975	1976	rBV3	561	501	0.06%	0.008%
51	7.813	2011	2013	2017	rBV2	122	106	0.01%	0.002%
52	7.893	2022	2038	2056	rBV	409924	702041	80.18%	10.657%
53	8.022	2075	2078	2079	rBV2	360	203	0.02%	0.003%
54	8.176	2114	2126	2149	rBV	78685	135681	15.50%	2.060%
55	8.542	2237	2240	2243	rVB	239	138	0.02%	0.002%
56	8.575	2248	2250	2254	rVB2	175	104	0.01%	0.002%
57	8.629	2254	2267	2296	rBV2	186822	370172	42.28%	5.619%
58	8.835	2328	2331	2334	rBV	196	116	0.01%	0.002%
59	8.874	2340	2343	2346	rBV2	353	224	0.03%	0.003%
60	8.996	2378	2381	2384	rBV2	215	191	0.02%	0.003%
61	9.047	2393	2397	2398	rBV	245	147	0.02%	0.002%
62	9.157	2429	2431	2435	rVV2	166	107	0.01%	0.002%
63	9.211	2445	2448	2452	rBV	209	155	0.02%	0.002%
64	9.311	2473	2479	2480	rBV2	275	227	0.03%	0.003%
65	9.414	2498	2511	2538	rBV	359187	595875	68.06%	9.045%
66	9.610	2571	2572	2575	rBV	233	105	0.01%	0.002%
67	9.649	2581	2584	2588	rBV	198	158	0.02%	0.002%
68	9.739	2609	2612	2614	rVB2	253	135	0.02%	0.002%
69	9.796	2627	2630	2633	rBV	255	206	0.02%	0.003%
70	10.012	2695	2697	2699	rBV	242	116	0.01%	0.002%
71	10.121	2728	2731	2732	rBV	219	99	0.01%	0.002%
72	10.195	2750	2754	2758	rBV2	260	280	0.03%	0.004%
73	10.443	2828	2831	2833	rBV	184	149	0.02%	0.002%
74	10.636	2889	2891	2894	rBV	195	122	0.01%	0.002%
75	10.751	2913	2927	2943	rBV	270002	434869	49.67%	6.601%
76	10.886	2964	2969	2970	rBV2	658	497	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032823\
 Data File : VU053443.D
 Acq On : 28 Mar 2023 19:01
 Operator : JC/MD
 Sample : 02054-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYF61

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

77	10.954	2988	2990	2994	rVB2	219	160	0.02%	0.002%
78	10.989	2998	3001	3005	rVB2	355	216	0.02%	0.003%
79	11.076	3022	3028	3030	rBV	176	195	0.02%	0.003%
80	11.182	3058	3061	3062	rBV2	285	157	0.02%	0.002%
81	11.465	3141	3149	3161	rBV	8165	12097	1.38%	0.184%
82	11.578	3176	3184	3189	rBV2	318	440	0.05%	0.007%
83	11.726	3225	3230	3234	rBV2	222	266	0.03%	0.004%
84	11.806	3243	3255	3276	rBV	355862	581412	66.40%	8.826%
85	12.009	3314	3318	3321	rBV2	373	372	0.04%	0.006%
86	12.063	3331	3335	3336	rBV	302	221	0.03%	0.003%
87	12.189	3362	3374	3395	rBV	385994	623599	71.22%	9.466%
88	12.298	3406	3408	3411	rBV2	317	136	0.02%	0.002%
89	12.568	3486	3492	3502	rVB3	2675	3676	0.42%	0.056%
90	12.648	3514	3517	3521	rBV2	262	213	0.02%	0.003%
91	12.880	3583	3589	3593	rBV3	438	548	0.06%	0.008%
92	12.973	3610	3618	3623	rBV3	1566	2075	0.24%	0.031%
93	13.105	3657	3659	3667	rVB2	428	429	0.05%	0.007%
94	13.291	3712	3717	3726	rVB2	1267	1504	0.17%	0.023%
95	13.449	3758	3766	3782	rBV6	2737	4827	0.55%	0.073%
96	13.783	3867	3870	3875	rBV2	560	499	0.06%	0.008%
97	14.156	3982	3986	3987	rBV	546	307	0.04%	0.005%
98	14.224	4004	4007	4009	rBV	408	198	0.02%	0.003%
99	14.652	4138	4140	4142	rBV2	488	287	0.03%	0.004%
100	15.410	4369	4376	4388	rBV	6879	11275	1.29%	0.171%




Sum of corrected areas: 6587644

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032823\
Data File : VU053443.D
Acq On : 28 Mar 2023 19:01
Operator : JC/MD
Sample : 02054-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYF61

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

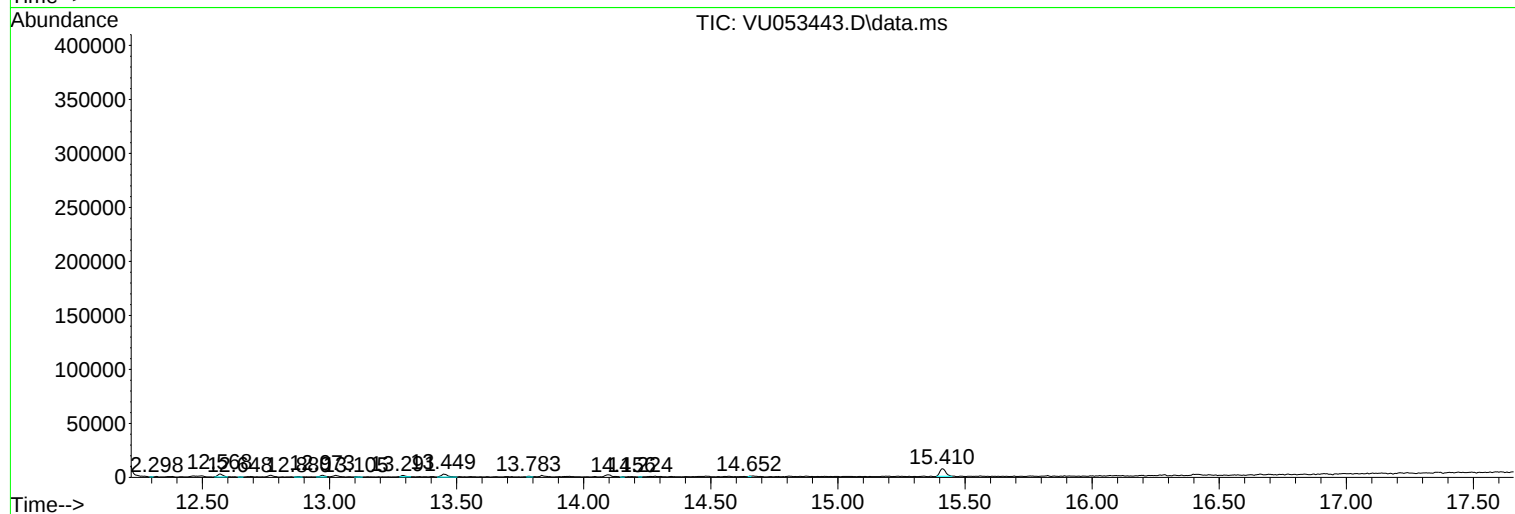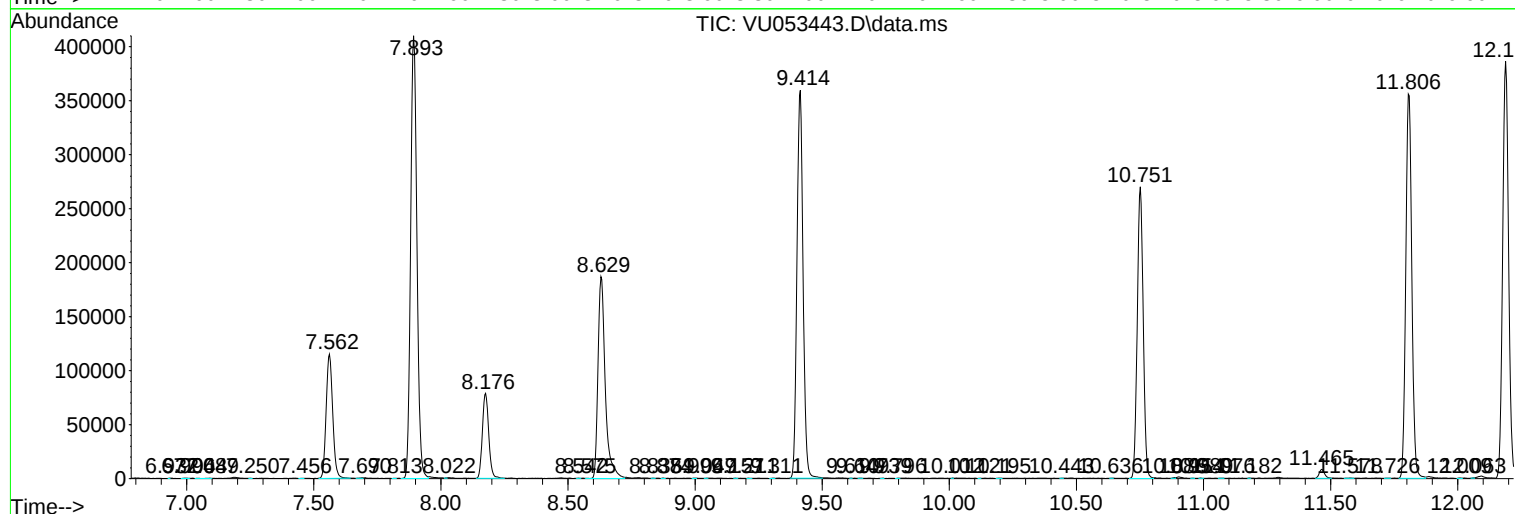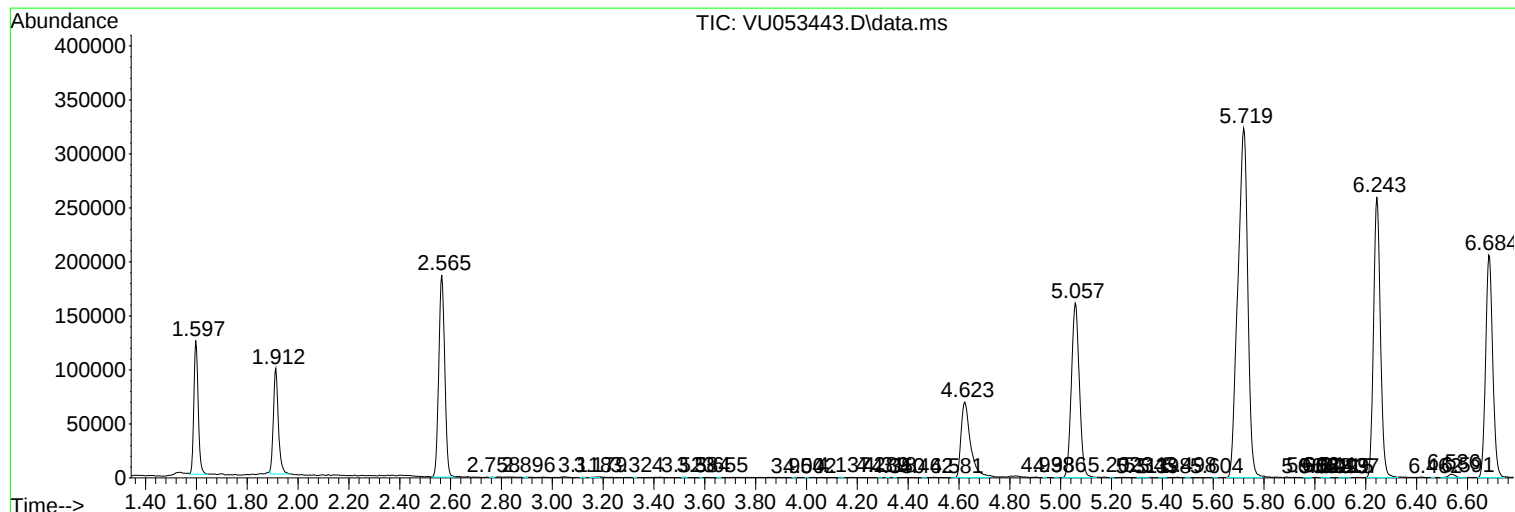

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032823\
Data File : VU053443.D
Acq On : 28 Mar 2023 19:01
Operator : JC/MD
Sample : 02054-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYF61

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032823\
Data File : VU053443.D
Acq On : 28 Mar 2023 19:01
Operator : JC/MD
Sample : 02054-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYF61

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------