

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032823\
 Data File : VU053445.D
 Acq On : 28 Mar 2023 19:48
 Operator : JC/MD
 Sample : 02054-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYF63

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

Signal : TIC: VU053445.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	95	rVB	114647	135931	16.27%	2.104%
2	1.913	170	178	197	rVB	92183	129683	15.52%	2.007%
3	2.565	370	381	397	rVB	177746	286164	34.25%	4.429%
4	2.948	497	500	501	rBV	386	251	0.03%	0.004%
5	3.141	558	560	563	rBV2	224	152	0.02%	0.002%
6	3.263	594	598	600	rBV	220	183	0.02%	0.003%
7	3.285	603	605	612	rVV2	266	211	0.03%	0.003%
8	3.356	624	627	631	rVB	283	187	0.02%	0.003%
9	3.379	632	634	639	rVB2	209	190	0.02%	0.003%
10	3.514	669	676	679	rBV2	343	412	0.05%	0.006%
11	3.536	679	683	686	rVB	247	197	0.02%	0.003%
12	3.578	693	696	700	rVB	234	193	0.02%	0.003%
13	3.601	700	703	708	rBV2	202	188	0.02%	0.003%
14	3.707	734	736	743	rVB2	220	180	0.02%	0.003%
15	3.784	756	760	761	rBV	298	214	0.03%	0.003%
16	4.019	829	833	834	rBV	243	159	0.02%	0.002%
17	4.028	834	836	841	rVV2	248	162	0.02%	0.003%
18	4.064	842	847	852	rVV2	331	321	0.04%	0.005%
19	4.137	867	870	873	rVB2	259	197	0.02%	0.003%
20	4.166	873	879	881	rBV	259	197	0.02%	0.003%
21	4.256	903	907	909	rBV	270	206	0.02%	0.003%
22	4.343	932	934	937	rVB2	355	178	0.02%	0.003%
23	4.369	937	942	948	rBV	150	199	0.02%	0.003%
24	4.398	948	951	954	rBV2	250	179	0.02%	0.003%
25	4.482	970	977	983	rBV2	272	364	0.04%	0.006%
26	4.523	988	990	997	rVB2	204	194	0.02%	0.003%
27	4.555	997	1000	1002	rBV2	235	189	0.02%	0.003%
28	4.623	1010	1021	1053	rBV	64733	169032	20.23%	2.616%
29	5.057	1139	1156	1179	rBV	149617	331497	39.68%	5.130%
30	5.272	1221	1223	1227	rBV2	262	185	0.02%	0.003%
31	5.324	1233	1239	1241	rBV	223	205	0.02%	0.003%
32	5.359	1246	1250	1258	rBV2	318	484	0.06%	0.007%
33	5.472	1282	1285	1287	rBV	305	172	0.02%	0.003%
34	5.597	1320	1324	1326	rBV2	284	242	0.03%	0.004%
35	5.719	1341	1362	1390	rBV2	304002	835488	100.00%	12.930%
36	5.919	1419	1424	1426	rBV	335	198	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032823\
 Data File : VU053445.D
 Acq On : 28 Mar 2023 19:48
 Operator : JC/MD
 Sample : 02054-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYF63

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

37	5.996	1445	1448	1452	rVB2	269	192	0.02%	0.003%
38	6.041	1458	1462	1464	rBV2	304	221	0.03%	0.003%
39	6.163	1498	1500	1502	rBV	239	151	0.02%	0.002%
40	6.244	1512	1525	1547	rBV	249511	471118	56.39%	7.291%
41	6.539	1603	1617	1638	rBV2	109593	206231	24.68%	3.192%
42	6.613	1638	1640	1643	rVB3	493	209	0.03%	0.003%
43	6.687	1647	1663	1687	rBV	195131	386213	46.23%	5.977%
44	6.806	1695	1700	1706	rVB3	486	605	0.07%	0.009%
45	6.944	1738	1743	1744	rBV2	267	205	0.02%	0.003%
46	7.195	1810	1821	1829	rBV4	781	1243	0.15%	0.019%
47	7.231	1829	1832	1836	rVB2	222	171	0.02%	0.003%
48	7.369	1869	1875	1880	rBV2	291	484	0.06%	0.007%
49	7.420	1885	1891	1894	rVB2	275	286	0.03%	0.004%
50	7.562	1921	1935	1957	rBV	109006	192726	23.07%	2.983%
51	7.694	1973	1976	1980	rBV2	551	367	0.04%	0.006%
52	7.751	1991	1994	1997	rBV2	217	171	0.02%	0.003%
53	7.819	2012	2015	2022	rBV	326	416	0.05%	0.006%
54	7.893	2025	2038	2060	rBV	386436	666729	79.80%	10.318%
55	8.054	2084	2088	2091	rVB4	501	350	0.04%	0.005%
56	8.073	2091	2094	2096	rBV2	239	175	0.02%	0.003%
57	8.128	2108	2111	2113	rBV2	216	163	0.02%	0.003%
58	8.176	2115	2126	2145	rVV2	77058	129568	15.51%	2.005%
59	8.343	2175	2178	2181	rBV2	274	179	0.02%	0.003%
60	8.433	2201	2206	2207	rVB2	241	149	0.02%	0.002%
61	8.452	2208	2212	2215	rBV2	299	194	0.02%	0.003%
62	8.507	2224	2229	2233	rVB	358	343	0.04%	0.005%
63	8.533	2233	2237	2240	rBV2	200	177	0.02%	0.003%
64	8.629	2255	2267	2303	rBV2	178612	355591	42.56%	5.503%
65	8.973	2371	2374	2377	rBV	228	213	0.03%	0.003%
66	9.047	2394	2397	2401	rVB	250	175	0.02%	0.003%
67	9.298	2469	2475	2476	rBV	180	152	0.02%	0.002%
68	9.414	2498	2511	2533	rBV	350567	577972	69.18%	8.944%
69	9.690	2594	2597	2603	rVB2	282	241	0.03%	0.004%
70	9.761	2617	2619	2624	rVB	296	231	0.03%	0.004%
71	9.790	2624	2628	2631	rBV2	225	187	0.02%	0.003%
72	9.841	2641	2644	2647	rBV	226	166	0.02%	0.003%
73	9.931	2669	2672	2676	rBV	173	167	0.02%	0.003%
74	10.208	2755	2758	2760	rBV	250	182	0.02%	0.003%
75	10.359	2802	2805	2811	rVB	298	269	0.03%	0.004%
76	10.385	2811	2813	2816	rBV2	228	161	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032823\
 Data File : VU053445.D
 Acq On : 28 Mar 2023 19:48
 Operator : JC/MD
 Sample : 02054-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EYF63

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

77	10.501	2846	2849	2855	rVB	185	175	0.02%	0.003%
78	10.623	2885	2887	2890	rVB2	309	185	0.02%	0.003%
79	10.710	2911	2914	2915	rVV	278	184	0.02%	0.003%
80	10.751	2915	2927	2951	rVB	259725	416742	49.88%	6.449%
81	10.845	2951	2956	2959	rBV	260	229	0.03%	0.004%
82	11.031	3010	3014	3020	rVB2	359	388	0.05%	0.006%
83	11.301	3091	3098	3103	rVB2	382	438	0.05%	0.007%
84	11.349	3110	3113	3115	rBV2	258	176	0.02%	0.003%
85	11.468	3143	3150	3158	rBV2	1944	2877	0.34%	0.045%
86	11.517	3162	3165	3169	rVV2	204	167	0.02%	0.003%
87	11.806	3243	3255	3272	rBV	350098	556073	66.56%	8.606%
88	12.189	3361	3374	3396	rBV	360964	590879	70.72%	9.144%
89	12.462	3455	3459	3463	rBV2	316	348	0.04%	0.005%
90	12.648	3513	3517	3520	rBV	291	264	0.03%	0.004%
91	12.767	3550	3554	3560	rVB2	596	692	0.08%	0.011%
92	12.886	3588	3591	3594	rVB	299	158	0.02%	0.002%
93	13.018	3629	3632	3633	rBV	304	173	0.02%	0.003%
94	13.115	3659	3662	3666	rVB	294	224	0.03%	0.003%
95	13.381	3743	3745	3748	rBV	255	173	0.02%	0.003%
96	13.796	3869	3874	3877	rBV2	472	477	0.06%	0.007%
97	14.076	3955	3961	3962	rBV	291	259	0.03%	0.004%
98	14.417	4061	4067	4071	rBV3	499	635	0.08%	0.010%
99	14.500	4088	4093	4095	rBV3	370	337	0.04%	0.005%
100	14.652	4136	4140	4143	rBV	459	425	0.05%	0.007%




Sum of corrected areas: 6461805

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032823\
Data File : VU053445.D
Acq On : 28 Mar 2023 19:48
Operator : JC/MD
Sample : 02054-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYF63

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

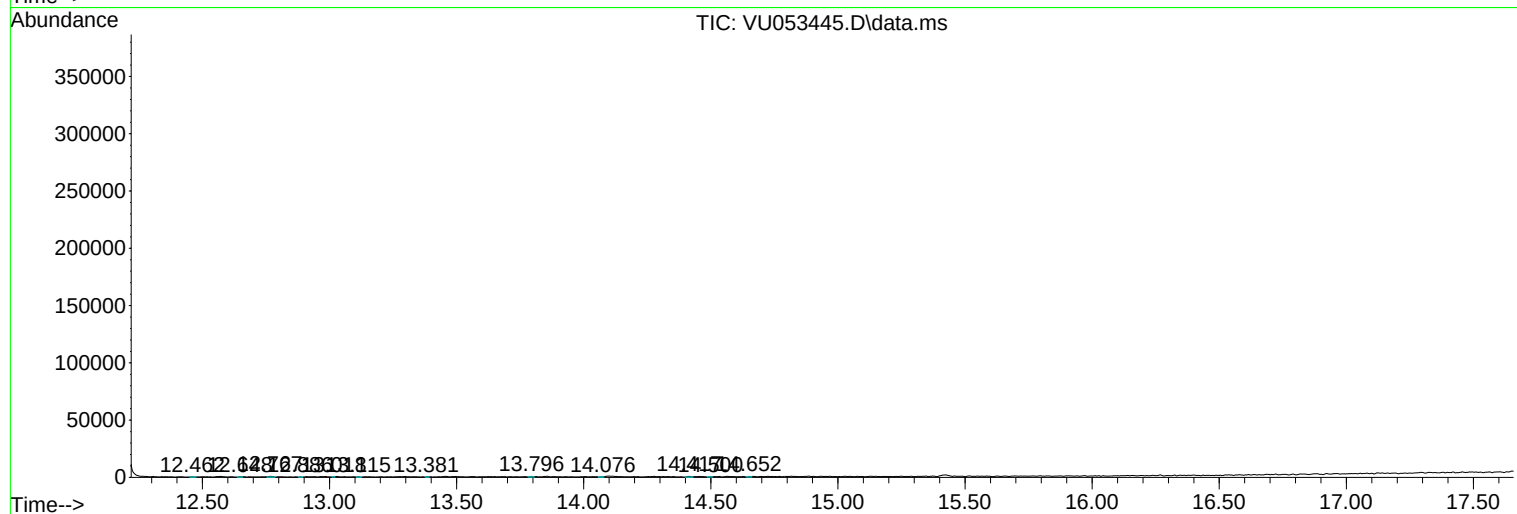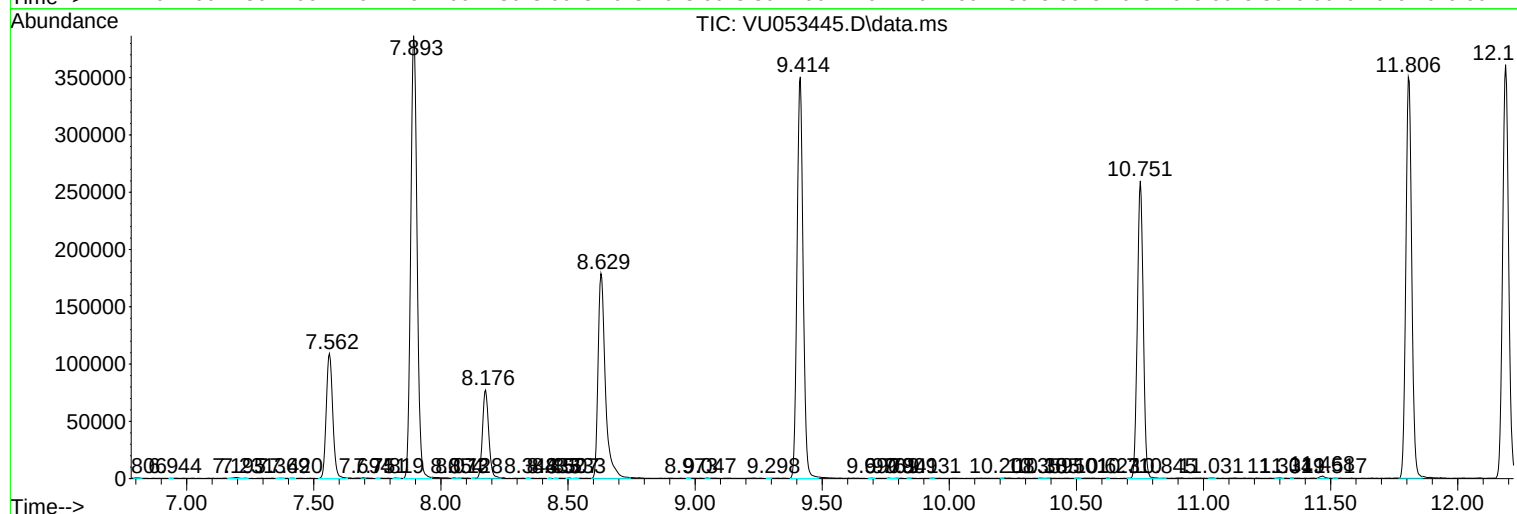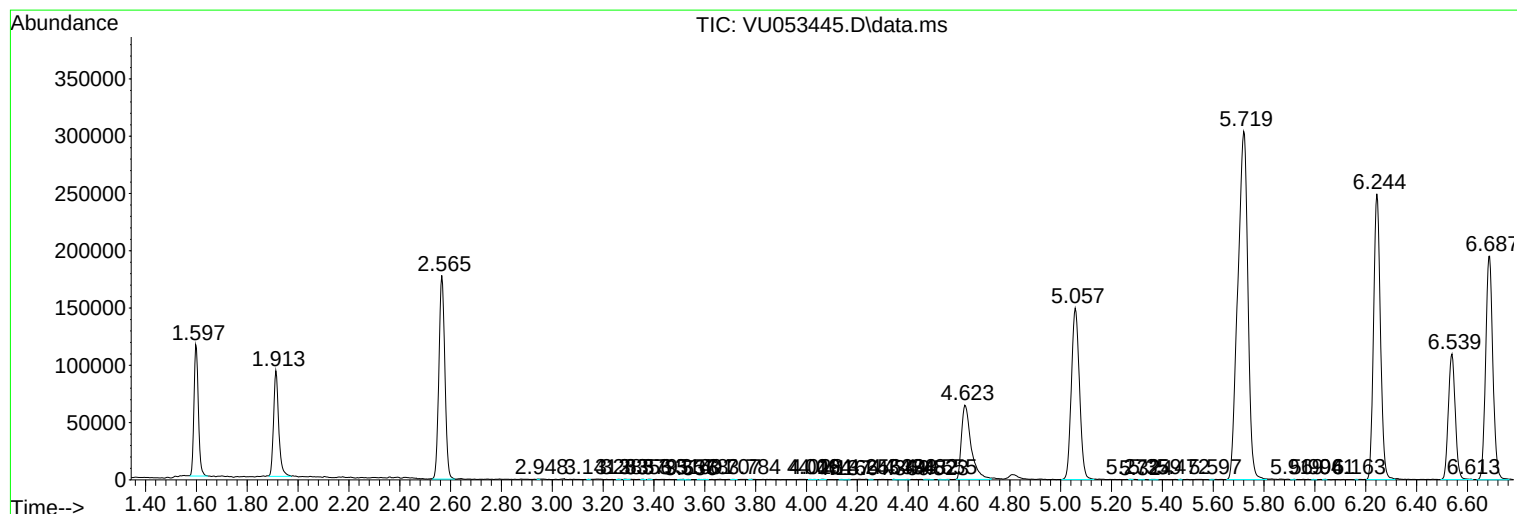

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032823\
Data File : VU053445.D
Acq On : 28 Mar 2023 19:48
Operator : JC/MD
Sample : 02054-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYF63

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032823\
Data File : VU053445.D
Acq On : 28 Mar 2023 19:48
Operator : JC/MD
Sample : 02054-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EYF63

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------