

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032823\
 Data File : VU053450.D
 Acq On : 28 Mar 2023 22:09
 Operator : JC/MD
 Sample : 02085-01DL 4X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COMB0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

Signal : TIC: VU053450.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	99	rVB	113321	135159	10.99%	1.829%
2	1.912	171	178	195	rVB	90040	123493	10.04%	1.671%
3	2.565	369	381	395	rBV	179484	288609	23.46%	3.905%
4	2.912	486	489	490	rBV	385	203	0.02%	0.003%
5	3.009	517	519	522	rBV2	273	183	0.01%	0.002%
6	3.041	522	529	545	rVB7	2390	4906	0.40%	0.066%
7	3.108	545	550	554	rBV	220	228	0.02%	0.003%
8	3.179	562	572	587	rVB2	4692	9548	0.78%	0.129%
9	3.343	619	623	624	rBV2	634	466	0.04%	0.006%
10	3.385	633	636	642	rVB3	216	243	0.02%	0.003%
11	3.414	642	645	647	rBV2	392	231	0.02%	0.003%
12	3.678	723	727	729	rBV2	219	169	0.01%	0.002%
13	3.961	811	815	820	rBV2	335	255	0.02%	0.003%
14	4.086	852	854	860	rVB2	202	186	0.02%	0.003%
15	4.414	952	956	960	rVB2	316	210	0.02%	0.003%
16	4.494	977	981	985	rBV2	260	217	0.02%	0.003%
17	4.539	992	995	1000	rVB2	303	225	0.02%	0.003%
18	4.575	1002	1006	1009	rBV2	216	156	0.01%	0.002%
19	4.626	1009	1022	1046	rBV	66900	182248	14.81%	2.466%
20	4.980	1127	1132	1134	rBV2	359	275	0.02%	0.004%
21	5.057	1138	1156	1176	rBV	154147	336479	27.35%	4.552%
22	5.195	1197	1199	1203	rVB2	271	170	0.01%	0.002%
23	5.285	1225	1227	1231	rVB	405	249	0.02%	0.003%
24	5.321	1231	1238	1240	rBV	244	272	0.02%	0.004%
25	5.382	1253	1257	1261	rVB	477	372	0.03%	0.005%
26	5.417	1265	1268	1278	rVB2	406	595	0.05%	0.008%
27	5.539	1304	1306	1311	rVB2	254	213	0.02%	0.003%
28	5.571	1311	1316	1318	rBV2	183	156	0.01%	0.002%
29	5.719	1339	1362	1394	rBV2	308829	847089	68.86%	11.460%
30	6.243	1511	1525	1551	rBV	252000	478291	38.88%	6.471%
31	6.494	1600	1603	1607	rVB	303	204	0.02%	0.003%
32	6.533	1607	1615	1618	rBV3	1287	1605	0.13%	0.022%
33	6.684	1648	1662	1684	rBV2	197104	386112	31.39%	5.224%
34	6.796	1695	1697	1698	rBV	470	162	0.01%	0.002%
35	6.864	1715	1718	1721	rBV2	272	244	0.02%	0.003%
36	7.009	1759	1763	1764	rBV	196	154	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032823\
 Data File : VU053450.D
 Acq On : 28 Mar 2023 22:09
 Operator : JC/MD
 Sample : 02085-01DL 4X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COMB0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

37	7.076	1781	1784	1787	rBV2	199	164	0.01%	0.002%
38	7.311	1850	1857	1858	rBV	241	172	0.01%	0.002%
39	7.468	1902	1906	1910	rBV2	261	275	0.02%	0.004%
40	7.562	1919	1935	1954	rBV	111200	196699	15.99%	2.661%
41	7.681	1967	1972	1975	rBV2	412	404	0.03%	0.005%
42	7.732	1984	1988	1991	rBV	204	218	0.02%	0.003%
43	7.790	1999	2006	2007	rBV	637	626	0.05%	0.008%
44	7.893	2022	2038	2074	rBV	393016	675116	54.88%	9.134%
45	8.089	2094	2099	2101	rBV	244	202	0.02%	0.003%
46	8.105	2101	2104	2107	rBV2	231	226	0.02%	0.003%
47	8.176	2114	2126	2148	rBV	75541	131966	10.73%	1.785%
48	8.279	2155	2158	2164	rVB3	576	378	0.03%	0.005%
49	8.324	2169	2172	2177	rBV2	248	188	0.02%	0.003%
50	8.359	2177	2183	2186	rBV2	235	220	0.02%	0.003%
51	8.433	2202	2206	2208	rBV2	214	162	0.01%	0.002%
52	8.507	2224	2229	2232	rVB2	250	244	0.02%	0.003%
53	8.552	2237	2243	2250	rVB3	942	1259	0.10%	0.017%
54	8.629	2256	2267	2299	rBV2	186352	367723	29.89%	4.975%
55	8.925	2354	2359	2363	rBV4	554	611	0.05%	0.008%
56	9.018	2386	2388	2391	rBV	220	153	0.01%	0.002%
57	9.034	2391	2393	2401	rVB2	288	319	0.03%	0.004%
58	9.070	2401	2404	2406	rBV2	264	180	0.01%	0.002%
59	9.166	2430	2434	2440	rVB2	278	274	0.02%	0.004%
60	9.221	2446	2451	2455	rBV2	285	286	0.02%	0.004%
61	9.259	2459	2463	2467	rBV	190	188	0.02%	0.003%
62	9.414	2498	2511	2537	rBV	352871	660597	53.70%	8.937%
63	9.562	2553	2557	2558	rBV	973	708	0.06%	0.010%
64	9.639	2578	2581	2589	rVB2	222	244	0.02%	0.003%
65	9.687	2591	2596	2597	rBV	882	692	0.06%	0.009%
66	10.012	2694	2697	2701	rVB2	258	222	0.02%	0.003%
67	10.108	2718	2727	2739	rVV6	1560	2869	0.23%	0.039%
68	10.237	2764	2767	2772	rVB2	304	250	0.02%	0.003%
69	10.285	2772	2782	2784	rBV2	358	400	0.03%	0.005%
70	10.481	2837	2843	2851	rVB4	909	1363	0.11%	0.018%
71	10.539	2855	2861	2864	rBV	210	259	0.02%	0.004%
72	10.587	2873	2876	2879	rBV	256	163	0.01%	0.002%
73	10.751	2913	2927	2943	rBV	261245	417355	33.93%	5.646%
74	10.877	2962	2966	2968	rBV	250	191	0.02%	0.003%
75	10.986	2998	3000	3009	rVV2	243	276	0.02%	0.004%
76	11.041	3013	3017	3020	rBV	274	277	0.02%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032823\
 Data File : VU053450.D
 Acq On : 28 Mar 2023 22:09
 Operator : JC/MD
 Sample : 02085-01DL 4X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COMB0DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

77	11.086	3027	3031	3039	rVB2	1137	1299	0.11%	0.018%
78	11.153	3048	3052	3055	rVB2	194	162	0.01%	0.002%
79	11.198	3063	3066	3070	rBV3	201	166	0.01%	0.002%
80	11.394	3124	3127	3129	rBV	247	156	0.01%	0.002%
81	11.465	3143	3149	3158	rVB2	2136	2726	0.22%	0.037%
82	11.529	3166	3169	3175	rBV2	279	275	0.02%	0.004%
83	11.571	3178	3182	3184	rBV2	216	153	0.01%	0.002%
84	11.687	3214	3218	3220	rBV	311	230	0.02%	0.003%
85	11.742	3225	3235	3244	rBV2	19294	30553	2.48%	0.413%
86	11.806	3244	3255	3277	rVB	361057	610343	49.61%	8.257%
87	12.198	3361	3377	3406	rBV2	507129	1230215	100.00%	16.644%
88	12.941	3601	3608	3609	rBV	233	273	0.02%	0.004%
89	12.970	3614	3617	3620	rBV	384	245	0.02%	0.003%
90	13.140	3667	3670	3673	rBV2	275	226	0.02%	0.003%
91	13.217	3688	3694	3703	rVB7	4321	6077	0.49%	0.082%
92	13.298	3717	3719	3722	rBV2	400	194	0.02%	0.003%
93	13.629	3819	3822	3824	rBV	254	171	0.01%	0.002%
94	13.835	3876	3886	3904	rBV3	93347	148674	12.09%	2.011%
95	13.909	3907	3909	3912	rBV	269	158	0.01%	0.002%
96	13.963	3923	3926	3929	rVB	258	179	0.01%	0.002%
97	14.086	3956	3964	3974	rBV	7905	11678	0.95%	0.158%
98	14.327	4028	4039	4052	rBV2	47707	75201	6.11%	1.017%
99	14.513	4094	4097	4103	rBV2	440	503	0.04%	0.007%
100	15.995	4552	4558	4570	rVB5	5341	7871	0.64%	0.106%




Sum of corrected areas: 7391424

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032823\
Data File : VU053450.D
Acq On : 28 Mar 2023 22:09
Operator : JC/MD
Sample : 02085-01DL 4X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COMB0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

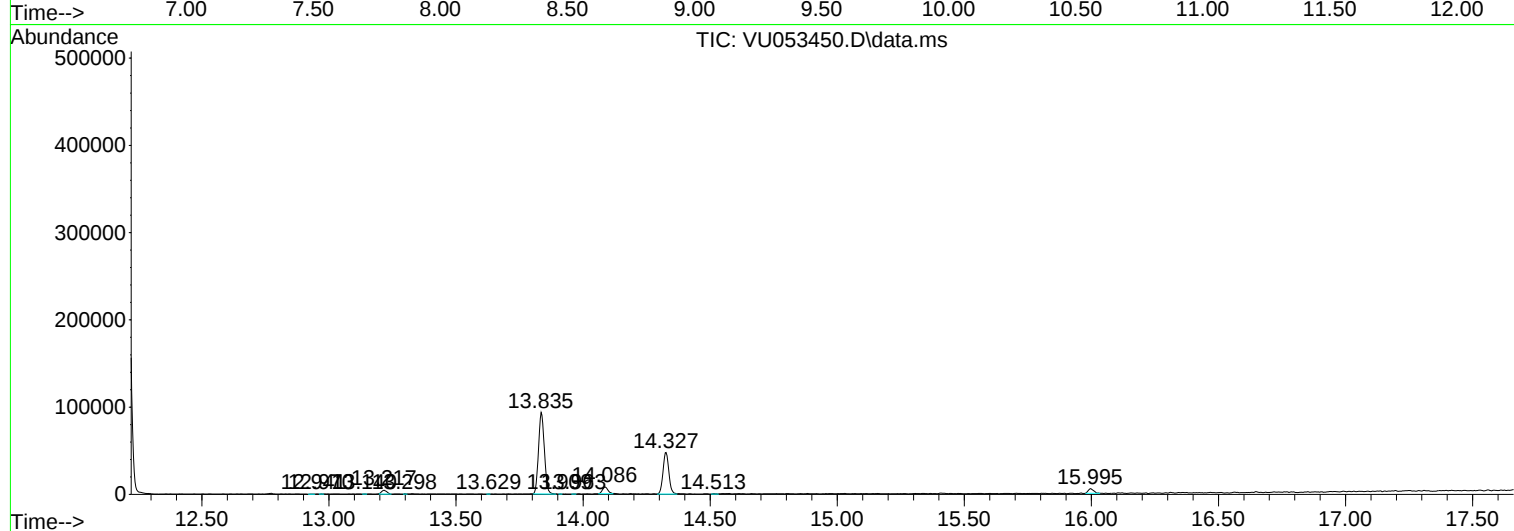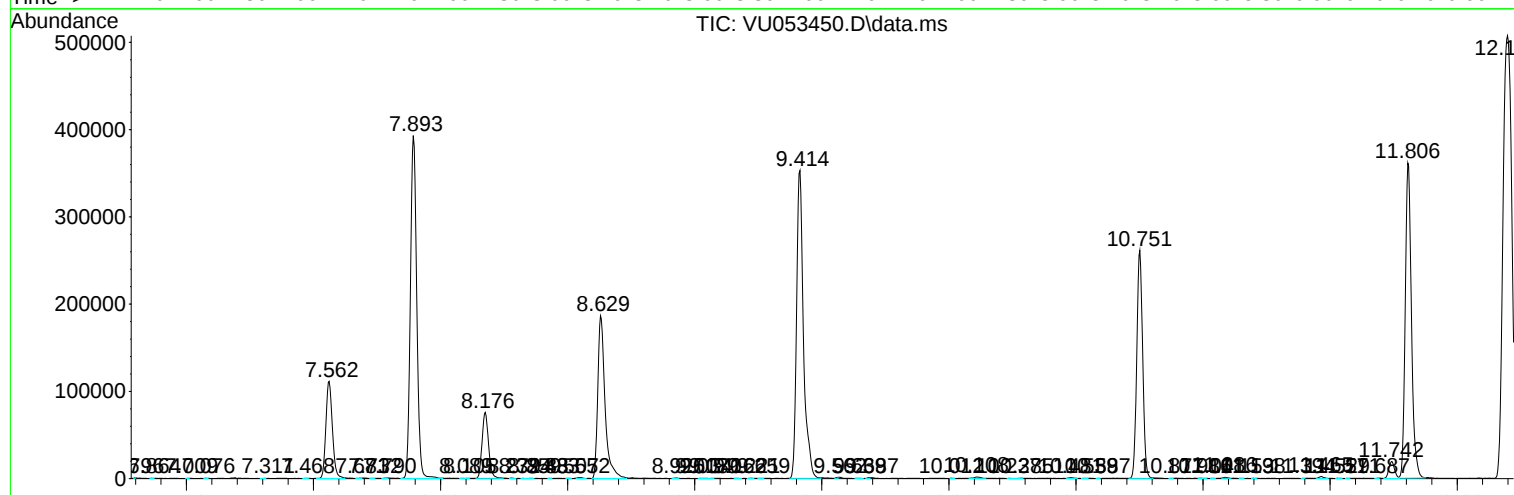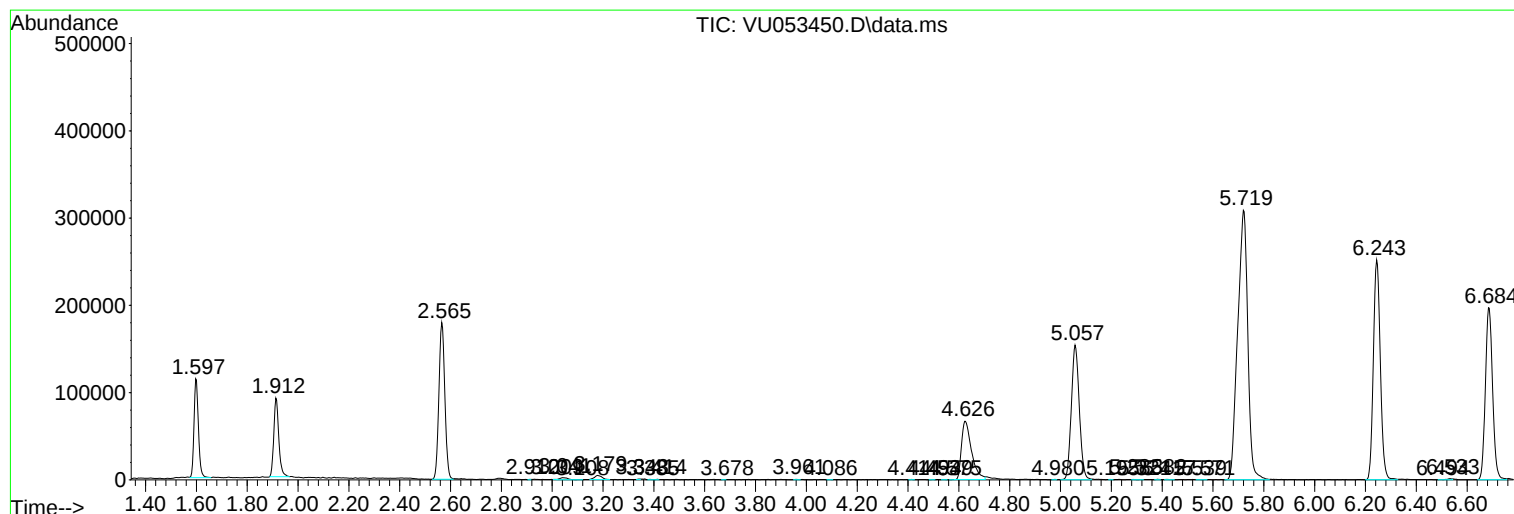

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032823\
Data File : VU053450.D
Acq On : 28 Mar 2023 22:09
Operator : JC/MD
Sample : 02085-01DL 4X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COMB0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032823\
Data File : VU053450.D
Acq On : 28 Mar 2023 22:09
Operator : JC/MD
Sample : 02085-01DL 4X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COMB0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------