

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032823\
 Data File : VU053451.D
 Acq On : 28 Mar 2023 22:32
 Operator : JC/MD
 Sample : 02037-11DL 1000X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E45F2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

Signal : TIC: VU053451.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	98	rVB	110881	131799	14.45%	1.907%
2	1.913	171	178	196	rVB	86293	121494	13.32%	1.758%
3	2.565	369	381	399	rBV	167919	274791	30.12%	3.976%
4	2.906	484	487	491	rVB2	426	307	0.03%	0.004%
5	3.041	519	529	541	rBV3	4820	8710	0.95%	0.126%
6	3.167	563	568	570	rBV2	247	233	0.03%	0.003%
7	3.253	592	595	601	rVB2	420	316	0.03%	0.005%
8	3.298	606	609	614	rBV2	307	307	0.03%	0.004%
9	3.359	617	628	640	rVB4	2642	5308	0.58%	0.077%
10	3.421	642	647	650	rBV2	276	264	0.03%	0.004%
11	3.588	695	699	705	rVB2	356	388	0.04%	0.006%
12	3.623	705	710	713	rBV2	313	260	0.03%	0.004%
13	3.642	713	716	719	rBV2	247	155	0.02%	0.002%
14	3.687	725	730	738	rVB2	578	654	0.07%	0.009%
15	4.025	831	835	837	rBV2	269	196	0.02%	0.003%
16	4.266	907	910	915	rVB2	235	235	0.03%	0.003%
17	4.359	936	939	945	rVB2	199	193	0.02%	0.003%
18	4.404	950	953	961	rVB2	212	212	0.02%	0.003%
19	4.478	972	976	981	rVB2	242	219	0.02%	0.003%
20	4.546	994	997	999	rBV	244	189	0.02%	0.003%
21	4.662	1010	1033	1068	rBV2	340238	912310	100.00%	13.201%
22	4.935	1115	1118	1122	rVB2	368	331	0.04%	0.005%
23	4.977	1128	1131	1134	rBV2	306	218	0.02%	0.003%
24	5.057	1139	1156	1175	rBV	148266	323299	35.44%	4.678%
25	5.183	1193	1195	1201	rBV2	229	172	0.02%	0.002%
26	5.276	1218	1224	1226	rBV2	317	305	0.03%	0.004%
27	5.385	1252	1258	1263	rVB	350	383	0.04%	0.006%
28	5.408	1263	1265	1269	rBV	204	165	0.02%	0.002%
29	5.443	1272	1276	1279	rBV2	229	182	0.02%	0.003%
30	5.559	1309	1312	1317	rVV2	232	202	0.02%	0.003%
31	5.581	1317	1319	1325	rVB2	236	189	0.02%	0.003%
32	5.719	1341	1362	1385	rBV2	294814	806990	88.46%	11.677%
33	5.948	1430	1433	1435	rBV	241	166	0.02%	0.002%
34	6.015	1450	1454	1458	rBV2	238	247	0.03%	0.004%
35	6.157	1491	1498	1501	rBV	235	288	0.03%	0.004%
36	6.195	1503	1510	1511	rBV2	237	261	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032823\
 Data File : VU053451.D
 Acq On : 28 Mar 2023 22:32
 Operator : JC/MD
 Sample : 02037-11DL 1000X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E45F2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

37	6.244	1512	1525	1551	rVV	245518	463641	50.82%	6.709%
38	6.424	1579	1581	1584	rVB	256	166	0.02%	0.002%
39	6.443	1584	1587	1589	rBV2	301	191	0.02%	0.003%
40	6.475	1594	1597	1602	rVB3	339	327	0.04%	0.005%
41	6.536	1603	1616	1626	rBV7	3535	6539	0.72%	0.095%
42	6.639	1644	1648	1649	rBV2	236	170	0.02%	0.002%
43	6.687	1649	1663	1683	rVV	188959	372665	40.85%	5.393%
44	6.803	1697	1699	1700	rVV	327	154	0.02%	0.002%
45	6.864	1713	1718	1720	rBV	269	208	0.02%	0.003%
46	6.964	1746	1749	1752	rBV2	216	149	0.02%	0.002%
47	7.250	1835	1838	1848	rVB2	228	225	0.02%	0.003%
48	7.369	1872	1875	1879	rBV2	273	227	0.02%	0.003%
49	7.514	1917	1920	1923	rBV	285	196	0.02%	0.003%
50	7.562	1923	1935	1961	rBV2	107450	186974	20.49%	2.706%
51	7.649	1961	1962	1965	rVB	299	162	0.02%	0.002%
52	7.771	1995	2000	2003	rBV	242	274	0.03%	0.004%
53	7.790	2003	2006	2012	rVB2	301	314	0.03%	0.005%
54	7.893	2024	2038	2067	rBV	378331	647065	70.93%	9.363%
55	8.118	2106	2108	2112	rVB	274	171	0.02%	0.002%
56	8.176	2113	2126	2143	rBV	74300	128096	14.04%	1.854%
57	8.321	2167	2171	2173	rBV	289	203	0.02%	0.003%
58	8.362	2180	2184	2189	rVB	171	176	0.02%	0.003%
59	8.549	2233	2242	2251	rBV2	7735	12080	1.32%	0.175%
60	8.629	2256	2267	2301	rBV2	174706	351688	38.55%	5.089%
61	8.835	2327	2331	2333	rBV	190	160	0.02%	0.002%
62	8.877	2342	2344	2349	rVB	346	231	0.03%	0.003%
63	8.906	2350	2353	2355	rBV	277	160	0.02%	0.002%
64	9.166	2428	2434	2438	rBV	351	356	0.04%	0.005%
65	9.411	2498	2510	2533	rBV	336402	567582	62.21%	8.213%
66	9.562	2552	2557	2559	rBV2	734	684	0.07%	0.010%
67	9.642	2577	2582	2588	rBV	405	431	0.05%	0.006%
68	9.697	2591	2599	2607	rVB4	769	1229	0.13%	0.018%
69	9.883	2650	2657	2660	rBV2	270	330	0.04%	0.005%
70	10.057	2706	2711	2716	rVB2	222	218	0.02%	0.003%
71	10.092	2717	2722	2723	rBV	457	305	0.03%	0.004%
72	10.436	2826	2829	2834	rBV2	267	273	0.03%	0.004%
73	10.478	2839	2842	2844	rBV	462	307	0.03%	0.004%
74	10.751	2911	2927	2943	rBV	251334	401683	44.03%	5.812%
75	10.915	2976	2978	2981	rBV2	271	179	0.02%	0.003%
76	10.951	2986	2989	2995	rVV	209	155	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032823\
 Data File : VU053451.D
 Acq On : 28 Mar 2023 22:32
 Operator : JC/MD
 Sample : 02037-11DL 1000X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E45F2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M

Title : VOC Analysis

77	11.092	3025	3033	3040	rBV3	627	1027	0.11%	0.015%
78	11.169	3054	3057	3060	rBV	323	205	0.02%	0.003%
79	11.214	3068	3071	3076	rVB	376	302	0.03%	0.004%
80	11.324	3098	3105	3109	rBV2	432	527	0.06%	0.008%
81	11.414	3130	3133	3135	rBV2	198	148	0.02%	0.002%
82	11.690	3217	3219	3225	rVB2	206	143	0.02%	0.002%
83	11.748	3231	3237	3243	rVB3	1160	1525	0.17%	0.022%
84	11.806	3243	3255	3272	rBV	346856	551787	60.48%	7.985%
85	12.066	3333	3336	3339	rBV	265	206	0.02%	0.003%
86	12.189	3362	3374	3396	rBV	350854	586860	64.33%	8.492%
87	12.311	3410	3412	3413	rBV2	331	162	0.02%	0.002%
88	12.613	3502	3506	3509	rBV	248	179	0.02%	0.003%
89	12.632	3509	3512	3516	rVV2	256	206	0.02%	0.003%
90	12.755	3547	3550	3551	rBV	319	184	0.02%	0.003%
91	12.877	3585	3588	3593	rBV2	431	392	0.04%	0.006%
92	13.311	3720	3723	3725	rBV	265	174	0.02%	0.003%
93	13.337	3728	3731	3734	rBV	317	171	0.02%	0.002%
94	13.365	3734	3740	3742	rBV2	298	325	0.04%	0.005%
95	13.726	3846	3852	3855	rBV2	413	449	0.05%	0.006%
96	13.841	3879	3888	3899	rBV3	8196	13341	1.46%	0.193%
97	13.967	3923	3927	3932	rVB2	471	516	0.06%	0.007%
98	14.095	3960	3967	3973	rBV5	2508	3939	0.43%	0.057%
99	14.330	4031	4040	4050	rVB5	5833	9457	1.04%	0.137%
100	14.555	4107	4110	4112	rBV	280	181	0.02%	0.003%




Sum of corrected areas: 6910688

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032823\
Data File : VU053451.D
Acq On : 28 Mar 2023 22:32
Operator : JC/MD
Sample : 02037-11DL 1000X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E45F2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

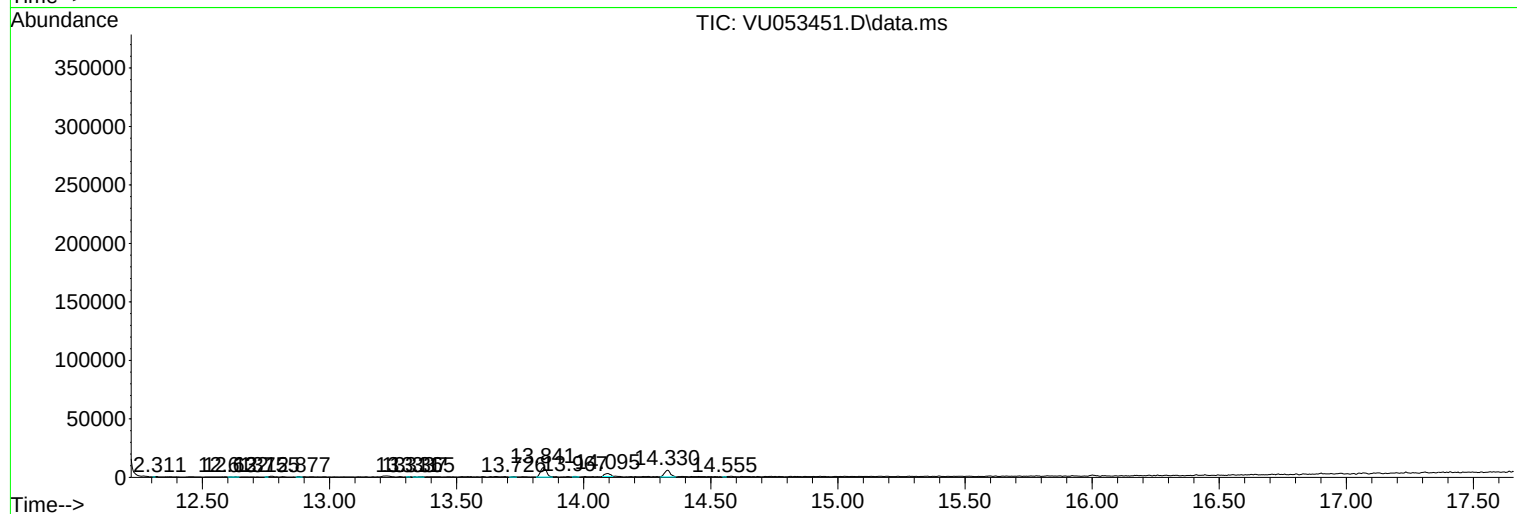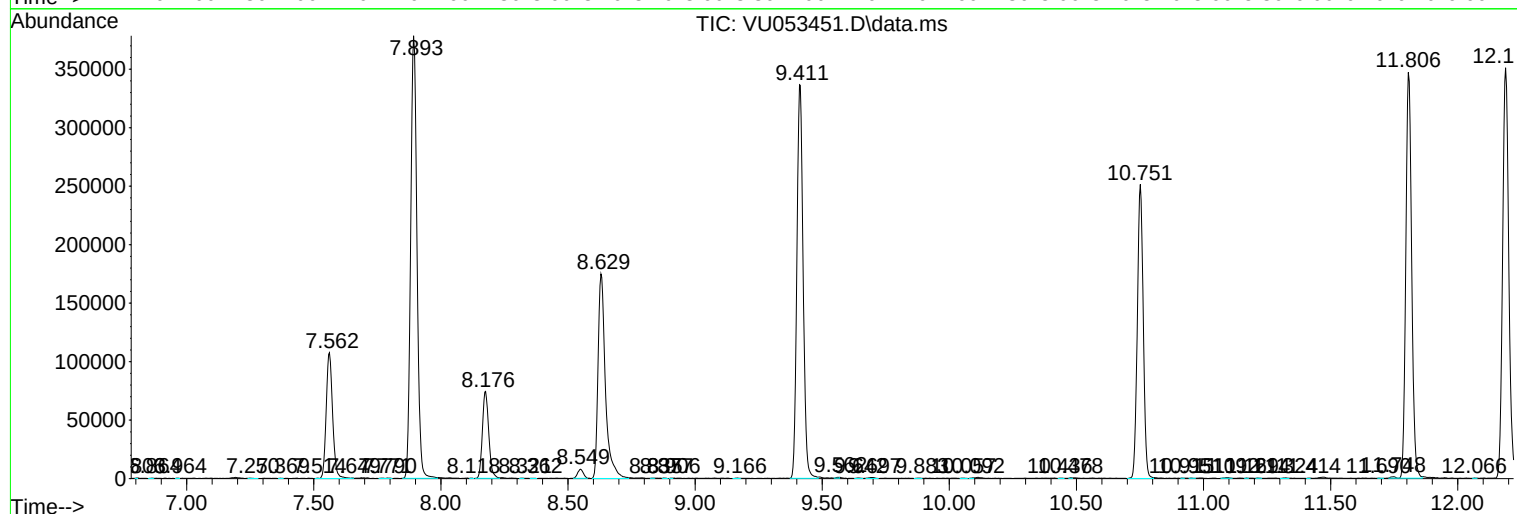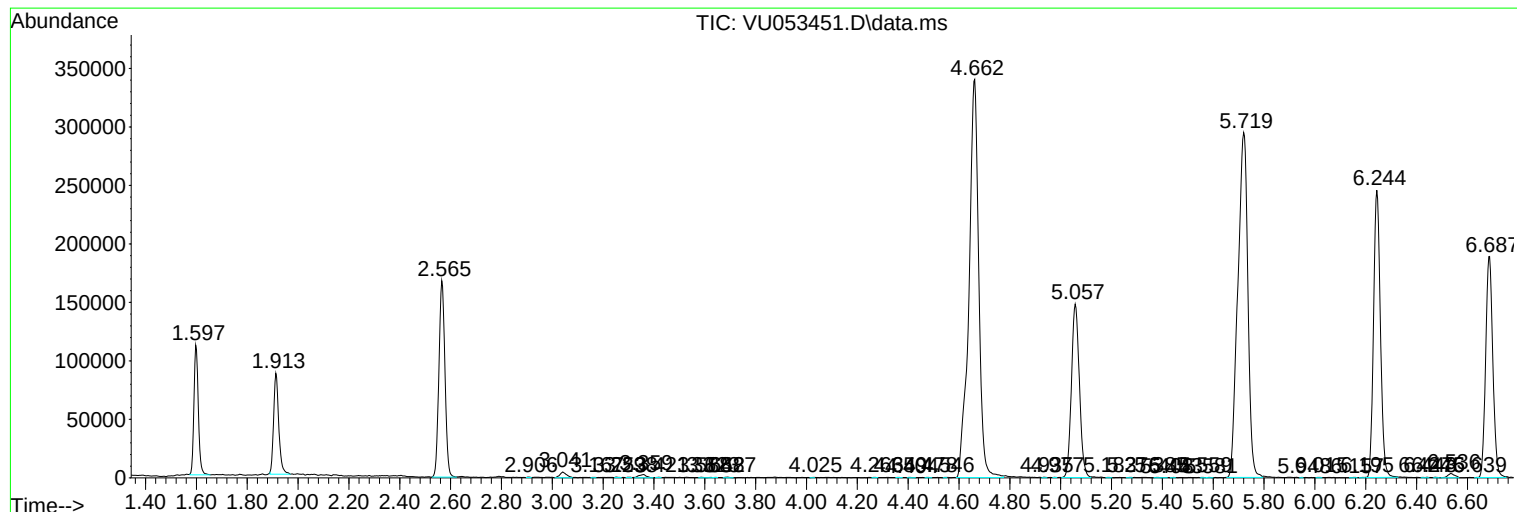

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032823\
Data File : VU053451.D
Acq On : 28 Mar 2023 22:32
Operator : JC/MD
Sample : 02037-11DL 1000X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E45F2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032823\
Data File : VU053451.D
Acq On : 28 Mar 2023 22:32
Operator : JC/MD
Sample : 02037-11DL 1000X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E45F2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------