

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032823\
 Data File : VU053453.D
 Acq On : 28 Mar 2023 23:19
 Operator : JC/MD
 Sample : 02037-02DL 250X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E45E5DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

Signal : TIC: VU053453.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	94	rVB	113877	138321	4.30%	1.486%
2	1.912	170	178	199	rBV	88681	123264	3.83%	1.324%
3	2.565	370	381	397	rVB	172133	280322	8.72%	3.011%
4	2.851	467	470	471	rBV	349	163	0.01%	0.002%
5	3.047	521	531	544	rVB4	5740	11270	0.35%	0.121%
6	3.157	562	565	566	rBV2	361	202	0.01%	0.002%
7	3.272	597	601	604	rBV	275	258	0.01%	0.003%
8	3.308	610	612	615	rBV	243	155	0.00%	0.002%
9	3.353	615	626	640	rVB2	8942	18064	0.56%	0.194%
10	3.430	647	650	654	rBV2	243	290	0.01%	0.003%
11	3.703	732	735	738	rVB2	313	148	0.00%	0.002%
12	3.813	766	769	773	rVB	242	149	0.00%	0.002%
13	3.854	778	782	783	rBV	1012	677	0.02%	0.007%
14	4.166	876	879	882	rBV	189	144	0.00%	0.002%
15	4.202	887	890	892	rBV2	242	171	0.01%	0.002%
16	4.359	936	939	941	rBV	197	162	0.01%	0.002%
17	4.555	996	1000	1006	rVB2	305	373	0.01%	0.004%
18	4.661	1010	1033	1065	rBV	1368460	3216094	100.00%	34.543%
19	5.057	1141	1156	1180	rVB	149361	328883	10.23%	3.532%
20	5.195	1197	1199	1203	rVB2	413	183	0.01%	0.002%
21	5.218	1203	1206	1209	rVB	327	203	0.01%	0.002%
22	5.292	1224	1229	1232	rBB2	209	170	0.01%	0.002%
23	5.311	1232	1235	1240	rBV2	357	353	0.01%	0.004%
24	5.372	1248	1254	1261	rBV	343	462	0.01%	0.005%
25	5.443	1274	1276	1280	rVB	329	180	0.01%	0.002%
26	5.491	1289	1291	1298	rVB	251	149	0.00%	0.002%
27	5.536	1299	1305	1308	rVB2	246	280	0.01%	0.003%
28	5.719	1342	1362	1384	rBV2	301334	817461	25.42%	8.780%
29	5.899	1415	1418	1423	rVB2	385	344	0.01%	0.004%
30	5.922	1423	1425	1427	rBV	314	165	0.01%	0.002%
31	5.935	1427	1429	1431	rBV2	312	157	0.00%	0.002%
32	6.025	1455	1457	1458	rBV2	335	146	0.00%	0.002%
33	6.140	1490	1493	1496	rBV2	245	223	0.01%	0.002%
34	6.243	1512	1525	1548	rVV	246889	470896	14.64%	5.058%
35	6.456	1588	1591	1595	rBV2	310	156	0.00%	0.002%
36	6.539	1607	1617	1628	rVB5	10652	19316	0.60%	0.207%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032823\
 Data File : VU053453.D
 Acq On : 28 Mar 2023 23:19
 Operator : JC/MD
 Sample : 02037-02DL 250X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E45E5DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

37	6.684	1648	1662	1681	rBV	190988	376179	11.70%	4.040%
38	6.793	1692	1696	1698	rBV3	355	243	0.01%	0.003%
39	7.279	1843	1847	1851	rBV2	272	231	0.01%	0.002%
40	7.452	1895	1901	1908	rBV	379	418	0.01%	0.004%
41	7.513	1916	1920	1922	rBV2	194	146	0.00%	0.002%
42	7.562	1922	1935	1955	rVV	105814	191010	5.94%	2.052%
43	7.729	1983	1987	1990	rBV2	224	219	0.01%	0.002%
44	7.832	2016	2019	2022	rVB2	249	178	0.01%	0.002%
45	7.893	2022	2038	2058	rBV	379712	650882	20.24%	6.991%
46	8.176	2114	2126	2141	rBV	74875	127247	3.96%	1.367%
47	8.349	2176	2180	2183	rBV	261	209	0.01%	0.002%
48	8.439	2205	2208	2209	rBV	285	159	0.00%	0.002%
49	8.497	2222	2226	2230	rBV	312	229	0.01%	0.002%
50	8.549	2230	2242	2255	rVB2	31839	52328	1.63%	0.562%
51	8.629	2255	2267	2297	rBV2	174441	347114	10.79%	3.728%
52	8.767	2308	2310	2312	rBV2	485	295	0.01%	0.003%
53	9.018	2383	2388	2391	rBV2	252	243	0.01%	0.003%
54	9.108	2413	2416	2419	rBV	243	208	0.01%	0.002%
55	9.198	2441	2444	2448	rVB2	271	215	0.01%	0.002%
56	9.311	2477	2479	2483	rVB2	289	189	0.01%	0.002%
57	9.336	2483	2487	2492	rBV	228	252	0.01%	0.003%
58	9.414	2496	2511	2538	rBV	344427	569977	17.72%	6.122%
59	9.565	2552	2558	2559	rBV2	697	555	0.02%	0.006%
60	9.594	2565	2567	2570	rBV	227	138	0.00%	0.001%
61	9.664	2586	2589	2591	rVV2	202	139	0.00%	0.001%
62	9.693	2592	2598	2605	rVB4	1631	2305	0.07%	0.025%
63	9.838	2638	2643	2644	rBV	220	167	0.01%	0.002%
64	10.060	2709	2712	2715	rBV	300	204	0.01%	0.002%
65	10.163	2741	2744	2746	rBV	262	166	0.01%	0.002%
66	10.214	2755	2760	2765	rVB2	244	281	0.01%	0.003%
67	10.327	2791	2795	2798	rBV2	247	241	0.01%	0.003%
68	10.443	2828	2831	2834	rVB	215	156	0.00%	0.002%
69	10.478	2839	2842	2844	rBV	330	256	0.01%	0.003%
70	10.594	2875	2878	2882	rBV	256	241	0.01%	0.003%
71	10.629	2886	2889	2893	rVB2	269	186	0.01%	0.002%
72	10.751	2913	2927	2948	rBV	256002	405064	12.59%	4.351%
73	10.912	2971	2977	2980	rBV2	379	350	0.01%	0.004%
74	10.931	2980	2983	2986	rVB2	241	171	0.01%	0.002%
75	10.970	2990	2995	2998	rBV	246	215	0.01%	0.002%
76	10.996	2998	3003	3006	rBV2	350	352	0.01%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032823\
 Data File : VU053453.D
 Acq On : 28 Mar 2023 23:19
 Operator : JC/MD
 Sample : 02037-02DL 250X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E45E5DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
 Title : VOC Analysis

77	11.057	3019	3022	3025	rBV2	296	206	0.01%	0.002%
78	11.082	3025	3030	3031	rBV2	422	336	0.01%	0.004%
79	11.147	3046	3050	3052	rBV	212	167	0.01%	0.002%
80	11.230	3070	3076	3086	rBV4	1633	2158	0.07%	0.023%
81	11.465	3144	3149	3151	rBV3	1017	1016	0.03%	0.011%
82	11.578	3181	3184	3186	rBV	242	163	0.01%	0.002%
83	11.745	3230	3236	3240	rBV3	751	712	0.02%	0.008%
84	11.806	3243	3255	3271	rBV	353162	557584	17.34%	5.989%
85	12.034	3322	3326	3328	rBV	212	165	0.01%	0.002%
86	12.047	3328	3330	3334	rVB	271	155	0.00%	0.002%
87	12.095	3340	3345	3350	rBV2	353	401	0.01%	0.004%
88	12.188	3361	3374	3394	rBV	360137	582088	18.10%	6.252%
89	12.465	3456	3460	3462	rBV	392	269	0.01%	0.003%
90	12.494	3466	3469	3473	rVB2	252	189	0.01%	0.002%
91	12.516	3473	3476	3482	rBV2	421	387	0.01%	0.004%
92	12.561	3487	3490	3492	rBV	323	199	0.01%	0.002%
93	12.770	3548	3555	3561	rBV2	368	619	0.02%	0.007%
94	13.024	3630	3634	3638	rBV2	423	362	0.01%	0.004%
95	13.304	3718	3721	3723	rBV	302	198	0.01%	0.002%
96	13.577	3804	3806	3809	rBV	230	156	0.00%	0.002%
97	13.844	3885	3889	3894	rVB5	1849	1746	0.05%	0.019%
98	13.973	3925	3929	3934	rVV2	510	509	0.02%	0.005%
99	14.327	4034	4039	4040	rBV3	1188	872	0.03%	0.009%
100	14.700	4151	4155	4159	rBV2	316	362	0.01%	0.004%




Sum of corrected areas: 9310331

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032823\
Data File : VU053453.D
Acq On : 28 Mar 2023 23:19
Operator : JC/MD
Sample : 02037-02DL 250X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E45E5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

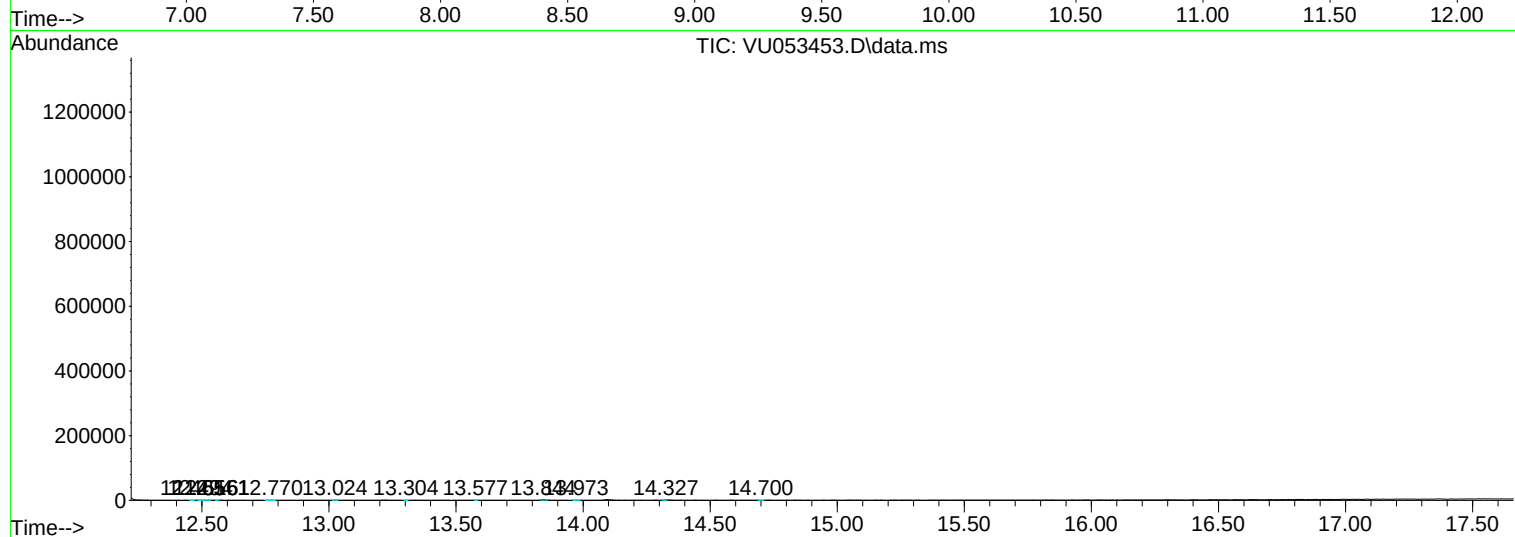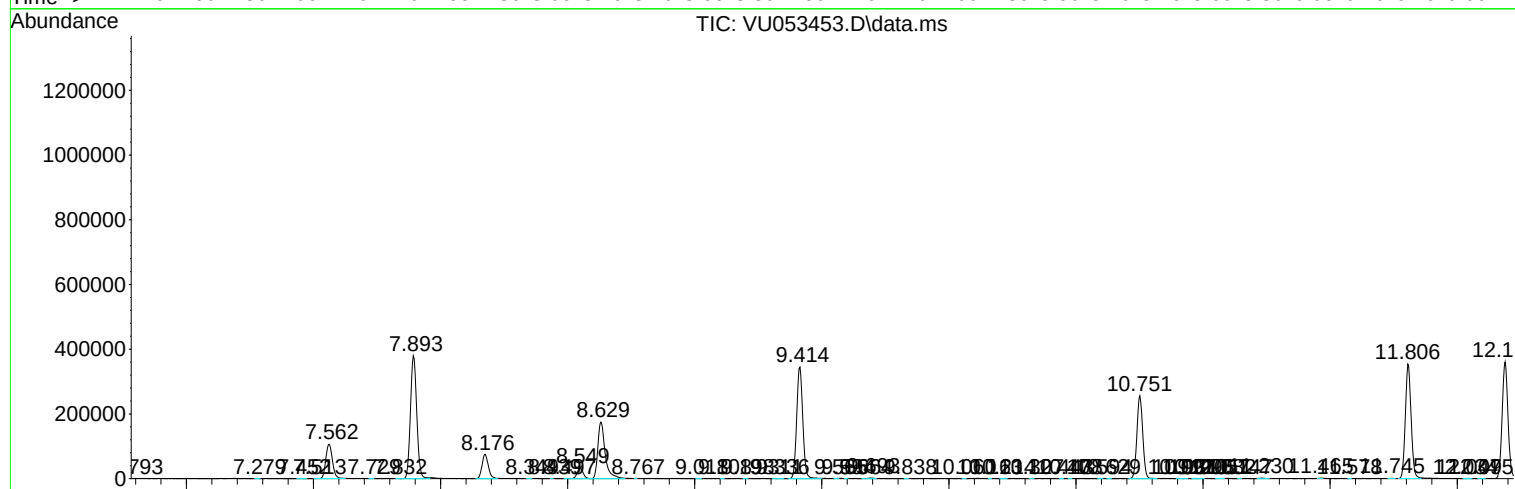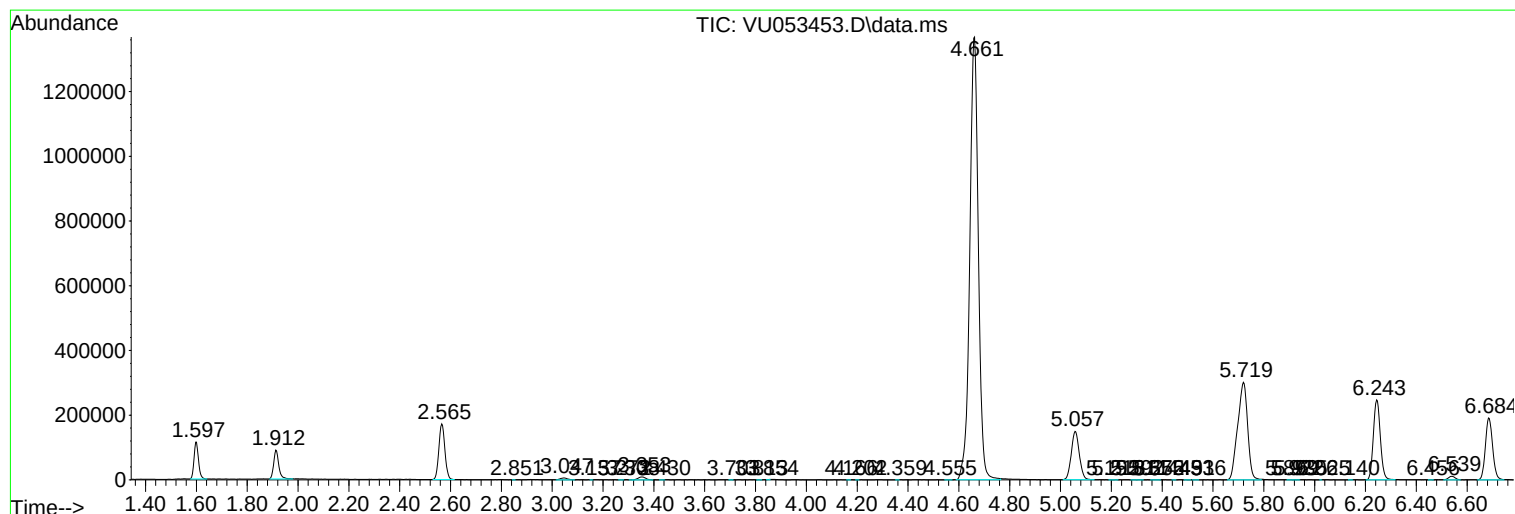

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032823\
Data File : VU053453.D
Acq On : 28 Mar 2023 23:19
Operator : JC/MD
Sample : 02037-02DL 250X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E45E5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032823\
Data File : VU053453.D
Acq On : 28 Mar 2023 23:19
Operator : JC/MD
Sample : 02037-02DL 250X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E45E5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------