


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032823\
Data File : VU053424.D
Acq On : 28 Mar 2023 10:05
Operator : JC/MD
Sample : BFB170
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB170

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM031523WMA.M
Title : VOC Analysis
Last Update : Wed Mar 29 02:16:14 2023

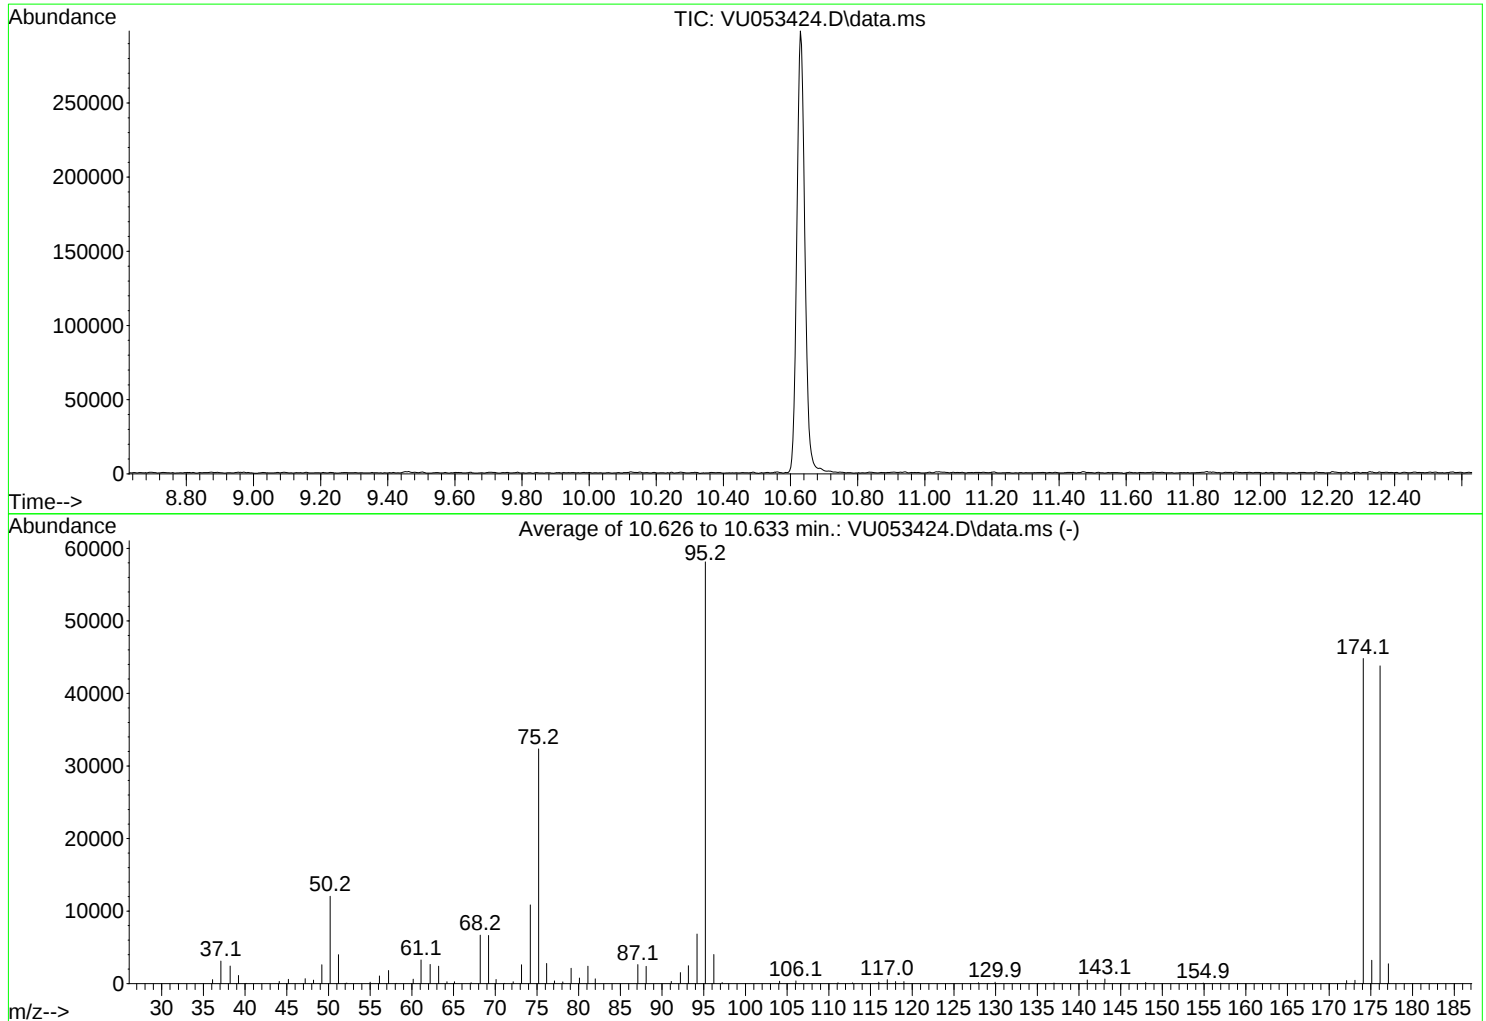

AutoFind: Scans 2888, 2889, 2890; Background Corrected with Scan 2876

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.7	12037	PASS
75	95	30	80	55.7	32363	PASS
95	95	100	100	100.0	58141	PASS
96	95	5	9	6.9	4014	PASS
173	174	0.00	2	1.0	457	PASS
174	95	50	120	77.1	44811	PASS
175	174	5	9	7.2	3230	PASS
176	174	95	101	97.7	43800	PASS
177	176	5	9	6.3	2745	PASS

Scan 2876 (10.588 min): VU053424.D\data.ms
BFB170

m/z	Abundance
40.20	193.0
44.10	719.0

Instrument :
MSVOA_U
ClientSampleId :
BFB170

m/z	Abundance
36.10	511.0
37.10	3248.0
38.20	2519.0
39.20	1132.0
40.00	226.0
44.10	976.0
45.20	581.0
47.20	748.0
48.20	379.0
49.20	2580.0
50.20	11870.0
51.20	3869.0
52.00	113.0
55.00	151.0
56.10	1067.0
57.20	1746.0
60.10	666.0
61.10	3254.0
62.20	2470.0
63.20	2427.0
64.20	235.0
65.10	273.0
67.10	152.0
68.20	6381.0
69.20	6247.0
70.10	513.0
72.10	214.0
73.20	2743.0
74.20	10377.0
75.20	31776.0
76.20	2720.0
77.10	445.0
78.10	285.0
79.10	2128.0
80.10	711.0
81.10	2340.0
82.00	617.0
87.10	2474.0
88.10	2195.0
91.10	286.0
92.20	1373.0
93.10	2436.0
94.20	6509.0
95.20	56352.0
96.20	3944.0
97.20	162.0
104.10	391.0
106.10	374.0
111.10	121.0
112.80	103.0
116.00	239.0
117.00	506.0
118.00	228.0
119.00	282.0
127.90	126.0
129.90	202.0
137.00	131.0
141.00	578.0
143.10	587.0
146.10	105.0
148.00	167.0
154.90	164.0
159.00	106.0
172.10	472.0
173.10	440.0
174.10	42128.0
175.10	3282.0
176.10	42632.0
177.10	2635.0

Instrument :
MSVOA_U
ClientSampleId :
BFB170

m/z	Abundance
36.10	555.0
37.10	3238.0
38.20	2448.0
39.20	1232.0
40.00	251.0
44.10	1068.0
45.20	634.0
47.20	728.0
48.20	538.0
49.20	2709.0
50.20	12461.0
51.20	4118.0
52.20	119.0
55.00	211.0
56.10	1124.0
57.20	1918.0
60.20	659.0
61.10	3360.0
62.20	2713.0
63.20	2450.0
64.20	280.0
65.10	262.0
67.10	158.0
68.20	6970.0
69.20	6771.0
70.10	596.0
71.10	102.0
72.10	278.0
73.20	2651.0
74.20	11268.0
75.20	33584.0
76.10	2899.0
77.10	384.0
78.10	245.0
79.10	2173.0
80.10	803.0
81.10	2516.0
82.00	667.0
87.10	2768.0
88.10	2448.0
91.10	315.0
92.20	1555.0
93.10	2475.0
94.20	6955.0
95.20	59912.0
96.20	4111.0
97.20	167.0
104.10	352.0
106.10	400.0
111.10	145.0
112.90	131.0
116.00	205.0
117.00	582.0
118.00	284.0
119.00	292.0
127.90	115.0
130.00	208.0
137.00	107.0
141.00	514.0
143.10	637.0
148.00	163.0
154.90	109.0
157.00	110.0
172.10	415.0
173.10	488.0
174.10	46120.0
175.10	3332.0
176.10	45128.0
177.10	2792.0

Instrument :
MSVOA_U
ClientSampleId :
BFB170

m/z	Abundance
36.10	587.0
37.10	2878.0
38.20	2291.0
39.20	1037.0
40.10	203.0
44.10	1056.0
45.20	577.0
47.20	555.0
48.20	537.0
49.20	2494.0
50.20	11779.0
51.20	3980.0
52.20	149.0
55.00	245.0
56.10	989.0
57.20	1781.0
58.10	101.0
60.20	500.0
61.10	3156.0
62.20	2731.0
63.20	2321.0
64.20	272.0
65.10	244.0
67.10	114.0
68.20	6672.0
69.20	6901.0
70.10	616.0
72.20	322.0
73.10	2429.0
74.20	10917.0
75.20	31728.0
76.10	2736.0
77.10	283.0
78.10	192.0
79.10	2073.0
80.10	781.0
81.10	2328.0
82.00	691.0
87.10	2622.0
88.10	2513.0
91.10	322.0
92.20	1644.0
93.20	2513.0
94.20	7019.0
95.20	58160.0
96.20	3986.0
97.20	147.0
104.10	285.0
106.00	353.0
111.10	102.0
112.90	113.0
116.00	157.0
117.00	589.0
118.00	321.0
119.00	290.0
128.00	149.0
129.10	111.0
130.00	200.0
135.10	127.0
141.00	431.0
143.10	679.0
145.10	112.0
148.00	136.0
157.00	104.0
172.10	400.0
173.10	443.0
174.10	46184.0
175.10	3076.0
176.10	43640.0
177.10	2808.0

Instrument :
MSVOA_U
ClientSampleId :
BFB170