


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032919\
 Data File : VU030530.D
 Acq On : 29 Mar 2019 08:26
 Operator : JC/SP
 Sample : BFB01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB01

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR032919WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Tue Apr 02 07:56:08 2019

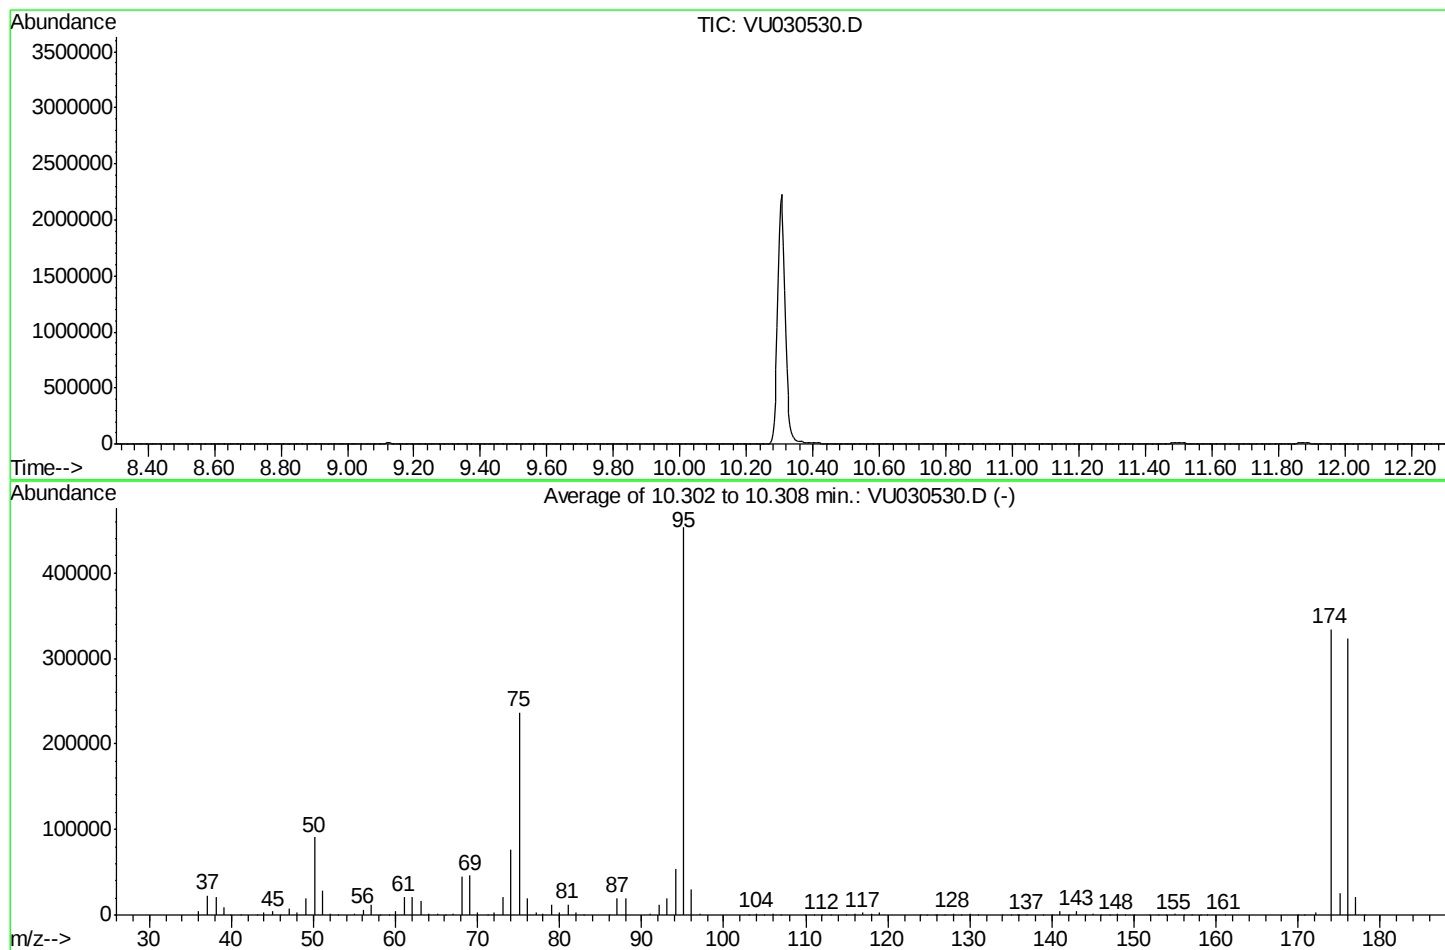

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2851

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.0	90874	PASS
75	95	30	80	52.2	236544	PASS
95	95	100	100	100.0	453290	PASS
96	95	5	9	6.7	30474	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	73.8	334464	PASS
175	174	5	9	7.8	26189	PASS
176	174	95	101	96.7	323349	PASS
177	176	5	9	6.6	21213	PASS

m/z	Abundance
36.00	3801.0
37.10	21800.0
38.10	19536.0
39.10	7908.0
40.00	500.0
41.10	202.0
43.10	129.0
44.10	3220.0
45.10	3365.0
46.00	413.0
47.10	6962.0
48.00	2768.0
49.10	18016.0
50.10	85592.0
51.10	26224.0
52.00	1294.0
53.00	246.0
55.00	1107.0
56.10	6339.0
57.10	12036.0
58.10	317.0
59.20	196.0
60.00	4267.0
61.10	20976.0
62.10	20288.0
63.10	15299.0
64.10	1594.0
65.20	1803.0
67.00	1114.0
68.10	42992.0
69.10	44296.0
70.00	3412.0
72.10	2270.0
73.10	19864.0
74.10	74384.0
75.10	225664.0
76.10	18928.0
77.10	2366.0
78.00	1638.0
79.00	11302.0
80.00	3654.0
81.00	11788.0
82.00	2520.0
82.90	276.0
86.00	629.0
87.00	18656.0
88.00	18568.0
91.00	1489.0
92.10	11869.0
93.10	18288.0
94.10	51512.0
95.10	436864.0
96.10	28648.0
97.10	864.0
103.00	222.0
104.00	1741.0
104.90	629.0
106.00	1505.0
106.90	366.0
109.90	210.0
110.90	180.0
112.00	215.0
113.00	318.0
114.90	482.0
115.90	1353.0
117.00	2625.0
118.00	1631.0
119.00	2366.0
123.90	225.0
126.00	145.0
126.80	110.0
128.00	1580.0
128.90	715.0
130.00	1395.0
131.00	557.0
134.00	154.0
135.00	644.0
136.00	141.0
136.90	665.0
138.90	152.0
141.00	4301.0
142.00	548.0
143.00	4436.0
144.10	328.0
145.00	769.0
146.00	615.0
147.00	270.0
147.90	1121.0
149.00	416.0
150.00	408.0
151.90	156.0

Instrument :
MSVOA_U
ClientSampleId :
BFB01

152.90	242.0
153.90	265.0
155.00	908.0
156.00	247.0
157.00	721.0
158.00	231.0
159.00	491.0
161.00	346.0
172.10	2856.0
174.00	328768.0
175.10	25736.0
176.00	319040.0
177.00	19976.0
178.00	461.0

Instrument :
MSVOA_U
ClientSampleId :
BFB01

m/z	Abundance
36.00	4318.0
37.10	23664.0
38.10	21544.0
39.10	8711.0
40.00	624.0
41.10	138.0
43.20	198.0
44.00	3273.0
45.10	4072.0
46.00	456.0
47.10	7398.0
47.90	2987.0
49.10	19576.0
50.10	94000.0
51.10	29240.0
52.00	1336.0
53.00	290.0
55.00	1263.0
56.10	6957.0
57.10	12870.0
58.10	414.0
60.00	4553.0
61.00	22624.0
62.10	22352.0
63.10	16864.0
64.00	2005.0
65.10	1998.0
66.20	214.0
67.10	1220.0
68.10	46216.0
69.10	47896.0
70.10	3902.0
72.00	2568.0
73.10	21696.0
74.10	79392.0
75.10	244288.0
76.10	20104.0
77.10	2734.0
77.90	1717.0
79.00	12733.0
80.00	3872.0
81.00	12892.0
82.00	2748.0
82.90	275.0
86.00	661.0
87.00	20224.0
88.00	19800.0
91.00	1709.0
92.00	12889.0
93.10	19528.0
94.10	54856.0
95.10	468544.0
96.10	31360.0
97.10	995.0
103.00	231.0
104.00	1862.0
105.00	676.0
106.00	1741.0
106.90	454.0
109.90	241.0
111.00	193.0
111.90	277.0
113.00	323.0
114.90	476.0
116.00	1439.0
117.00	2741.0
118.00	1626.0
119.00	2496.0
123.90	239.0
125.80	148.0
128.00	1663.0
129.00	789.0
130.00	1525.0
131.00	661.0
133.90	127.0
135.00	630.0
135.80	105.0
137.00	675.0
138.90	196.0
140.10	307.0
141.00	4581.0
142.00	558.0
143.00	4730.0
144.00	363.0
145.10	852.0
146.00	697.0
147.00	333.0
147.90	1170.0
149.00	411.0
150.00	404.0
151.80	163.0

Instrument :
MSVOA_U
ClientSampleId :
BFB01

152.90	250.0
153.90	311.0
154.90	979.0
156.10	273.0
157.00	812.0
158.10	219.0
159.00	536.0
161.00	428.0
170.80	223.0
172.10	3427.0
174.00	345536.0
175.10	27016.0
176.00	335360.0
177.00	21984.0
178.00	461.0

Instrument :
MSVOA_U
ClientSampleId :
BFB01

m/z	Abundance
36.00	4477.0
37.10	23312.0
38.10	21088.0
39.10	8860.0
39.90	683.0
43.20	218.0
44.00	2933.0
45.00	4218.0
46.00	475.0
47.10	7090.0
47.90	2991.0
49.10	19176.0
50.10	93032.0
51.10	29296.0
52.10	1312.0
53.00	289.0
55.00	1263.0
56.10	6830.0
57.10	12417.0
58.10	552.0
60.10	4465.0
61.00	21472.0
62.10	22416.0
63.10	16960.0
64.00	2224.0
65.10	2313.0
66.10	253.0
67.10	1208.0
68.10	45336.0
69.10	46832.0
70.10	3929.0
71.30	168.0
72.00	2609.0
73.10	21304.0
74.10	76688.0
75.10	239680.0
76.10	19960.0
77.10	2766.0
77.90	1791.0
79.00	12563.0
80.00	3711.0
81.00	12625.0
81.90	2861.0
82.90	243.0
86.00	619.0
87.00	19560.0
88.00	18608.0
91.00	1785.0
92.00	12621.0
93.10	18816.0
94.10	53472.0
95.10	454464.0
96.10	31416.0
97.10	999.0
103.00	215.0
104.00	1758.0
105.00	714.0
106.00	1712.0
106.90	465.0
109.90	261.0
111.00	232.0
111.90	265.0
113.10	309.0
115.00	484.0
116.00	1482.0
117.00	2642.0
117.90	1521.0
119.00	2477.0
124.00	228.0
124.80	121.0
125.80	101.0
127.00	102.0
128.00	1554.0
129.10	854.0
130.00	1563.0
130.90	650.0
133.90	121.0
135.00	561.0
135.80	124.0
137.00	645.0
138.90	226.0
140.00	326.0
141.00	4432.0
142.10	585.0
143.00	4718.0
144.00	379.0
145.00	917.0
146.00	696.0
147.00	295.0
147.90	1023.0
148.90	382.0

Instrument :
MSVOA_U
ClientSampleId :
BFB01

149.90	382.0
151.80	182.0
153.00	275.0
153.90	325.0
154.90	946.0
156.10	219.0
157.00	863.0
158.10	161.0
158.90	557.0
161.00	474.0
170.00	184.0
170.70	231.0
172.10	3526.0
174.00	329088.0
175.10	25816.0
176.00	315648.0
177.00	21680.0
178.10	536.0

Instrument :
MSVOA_U
ClientSampleId :
BFB01

m/z	Abundance
40.00	205.0
44.00	512.0

Instrument :
MSVOA_U
ClientSampleId :
BFB01