

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032921\
 Data File : VU042810.D
 Acq On : 29 Mar 2021 12:37
 Operator : SY/MD
 Sample : M1818-07
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AA8

Quant Time: Mar 30 01:13:33 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Mar 30 01:12:10 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.259	114	91340	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.426	117	90083	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.822	152	43932	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.604	65	23477	3.86	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	77.20%
7) Chloroethane-d5	1.919	69	20811	4.51	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	90.20%
11) 1,1-Dichloroethene-d2	2.575	63	43081	3.13	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	62.60%
20) 2-Butanone-d5	4.649	46	80016	40.02	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	80.04%
24) Chloroform-d	5.076	84	54305	4.51	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.20%
26) 1,2-Dichloroethane-d4	5.713	65	34673	4.68	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.60%
32) Benzene-d6	5.739	84	97214	4.40	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.00%
36) 1,2-Dichloropropane-d6	6.700	67	31945	4.48	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	89.60%
41) Toluene-d8	7.906	98	88789	4.12	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	82.40%
43) trans-1,3-Dichloroprop...	8.189	79	13783	4.14	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	82.80%
46) 2-Hexanone-d5	8.645	63	74314	46.63	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	93.26%
57) 1,1,2,2-Tetrachloroeth...	10.764	84	28367	4.47	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	89.40%
64) 1,2-Dichlorobenzene-d4	12.201	152	37326	4.69	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	93.80%
Target Compounds					Qvalue	
13) Acetone	2.665	43	5499	3.57	ug/L	77


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032921\
Data File : VU042810.D
Acq On : 29 Mar 2021 12:37
Operator : SY/MD
Sample : M1818-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AA8


Quant Time: Mar 30 01:13:33 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Mar 30 01:12:10 2021
Response via : Initial Calibration

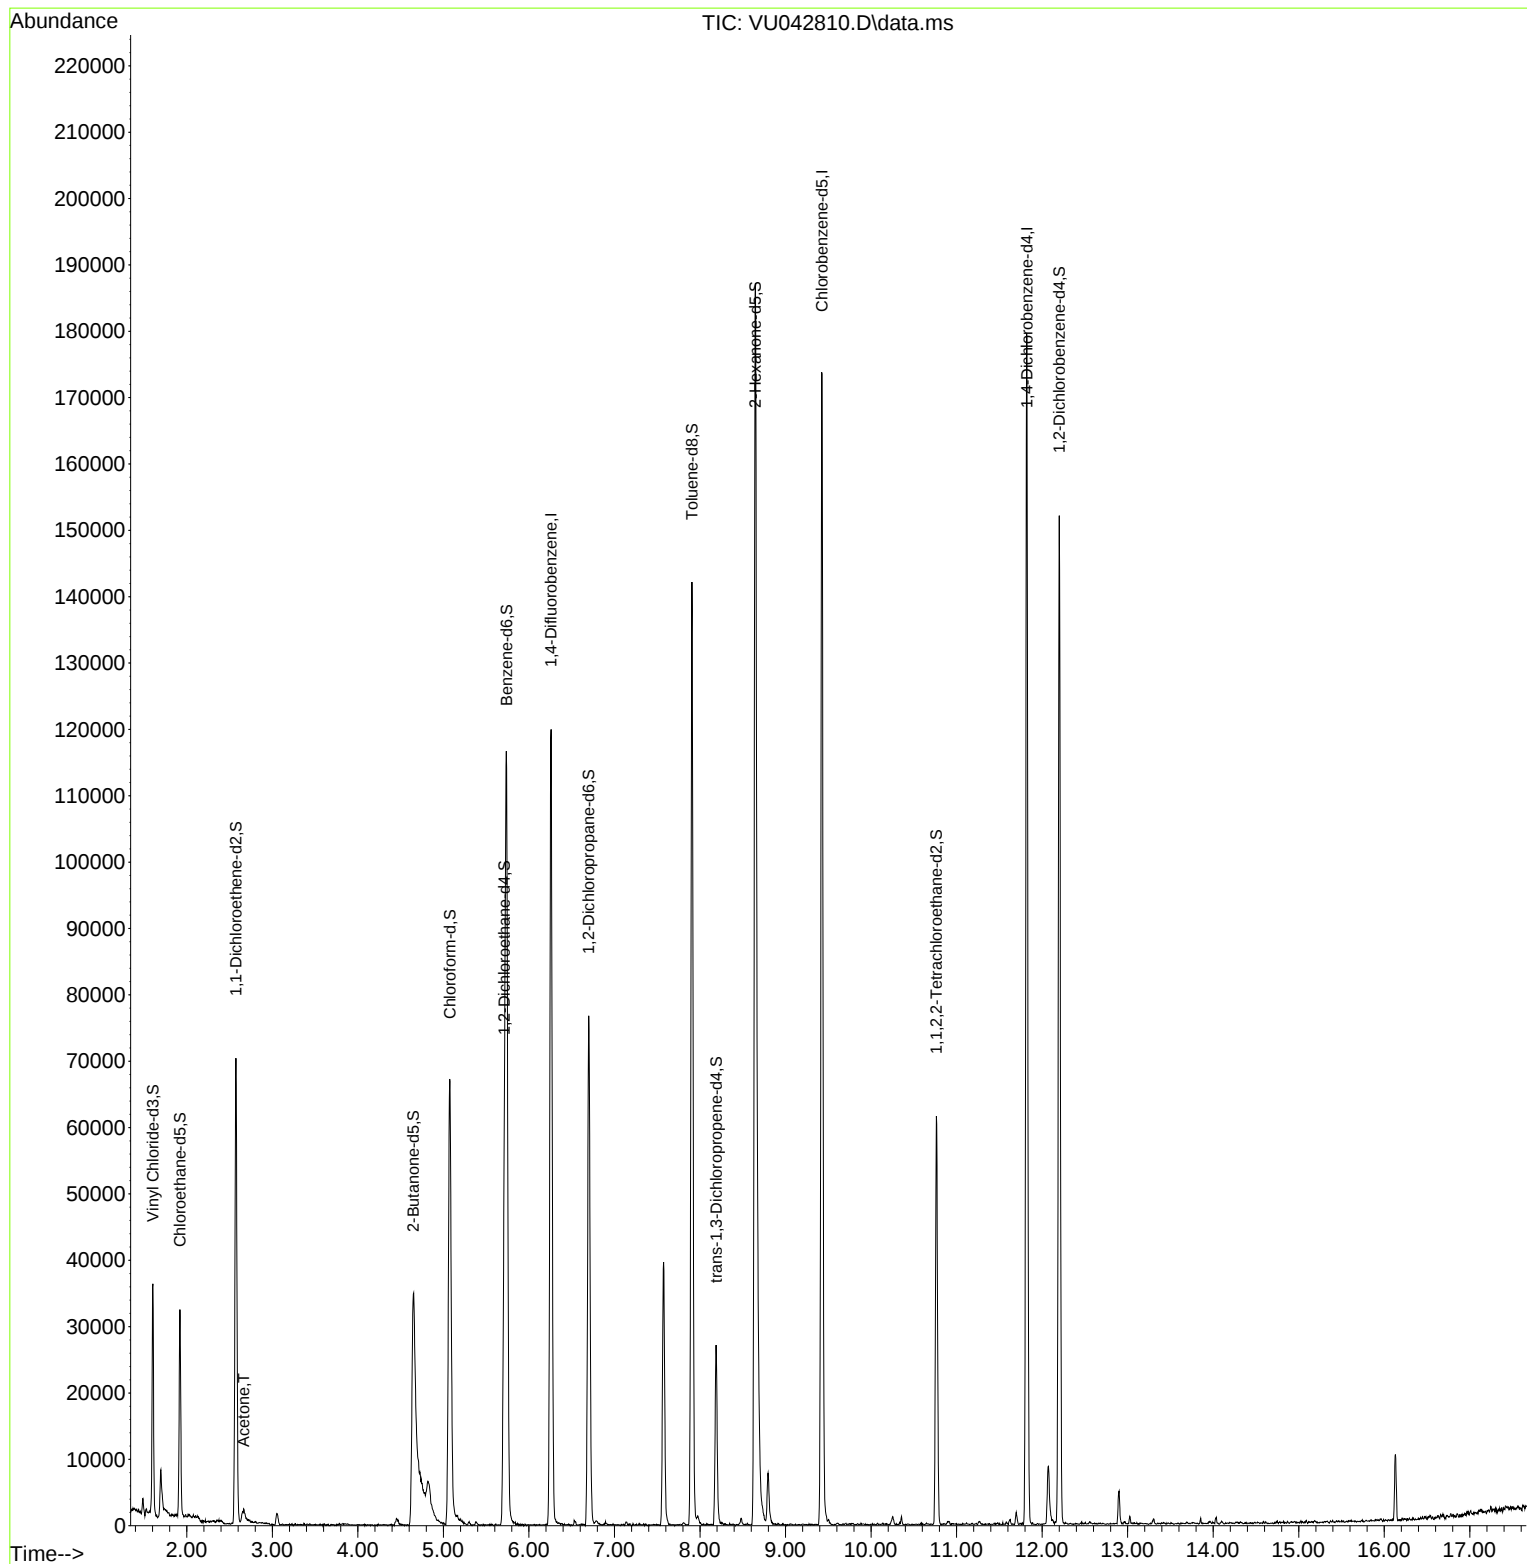

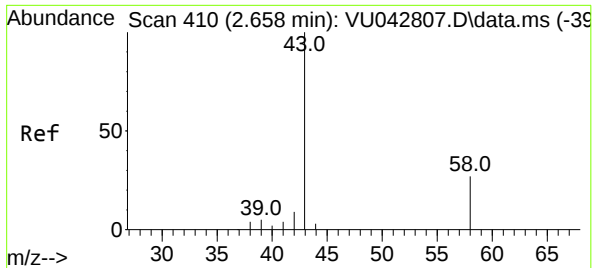

#13
 Acetone
 Concen: 3.57 ug/L
 RT: 2.665 min Scan# 412
 Delta R.T. 0.006 min
 Lab File: VU042810.D
 Acq: 29 Mar 2021 12:37

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AA8

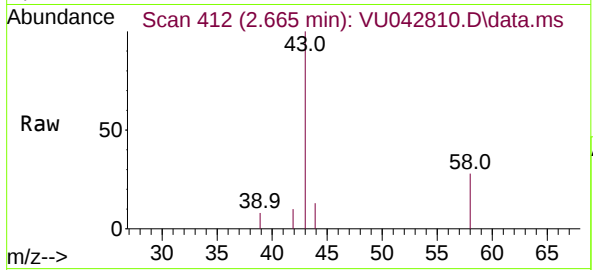

Tgt Ion: 43 Resp: 5499
 Ion Ratio Lower Upper
 43 100
 58 15.8 0.0 55.8

