
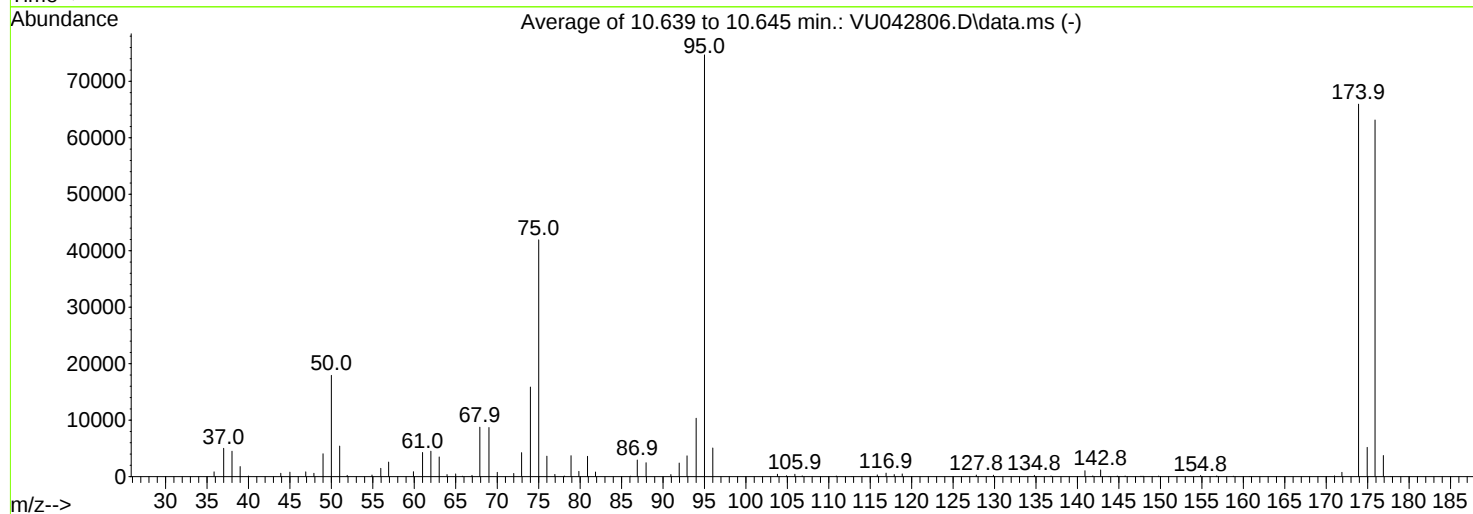


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032921\
 Data File : VU042806.D
 Acq On : 29 Mar 2021 08:46
 Operator : SY/MD
 Sample : BFB29
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB29

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Wed Mar 31 02:07:34 2021

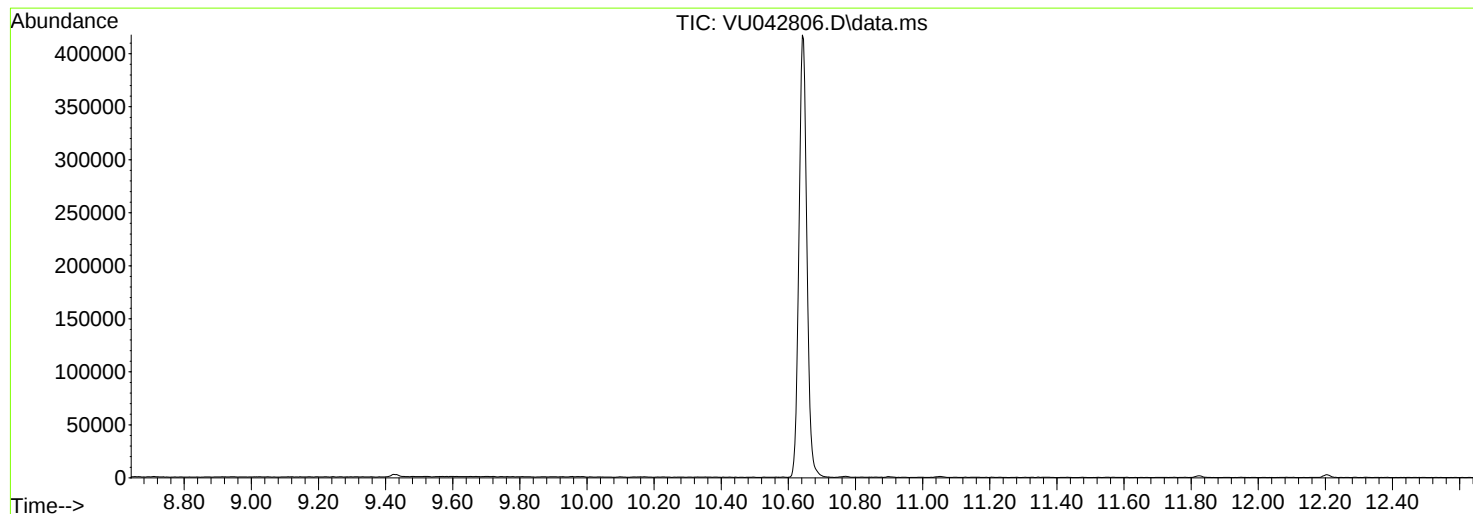

AutoFind: Scans 2892, 2893, 2894; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.0	17944	PASS
75	95	30	80	56.1	41933	PASS
95	95	100	100	100.0	74696	PASS
96	95	5	9	6.8	5069	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	88.3	65955	PASS
175	174	5	9	7.9	5195	PASS
176	174	95	101	95.8	63160	PASS
177	176	5	9	5.9	3741	PASS

m/z	Abundance
35.90	366.0
44.00	208.0

Instrument :
MSVOA_U
ClientSampleId :
BFB29

m/z	Abundance
35.90	1174.0
37.00	4892.0
38.00	4304.0
39.00	1656.0
40.00	124.0
43.90	715.0
45.00	804.0
46.90	811.0
47.90	651.0
49.00	3918.0
50.00	17024.0
51.00	5456.0
51.90	241.0
54.90	285.0
56.00	1414.0
56.90	2389.0
59.90	854.0
61.00	4270.0
62.00	4346.0
63.00	3470.0
63.90	367.0
65.00	501.0
66.90	168.0
67.90	8394.0
69.00	8194.0
70.00	744.0
72.00	535.0
73.00	4120.0
74.00	14829.0
75.00	39984.0
76.00	3458.0
76.90	397.0
78.90	3426.0
79.80	878.0
80.90	3353.0
81.80	819.0
86.10	108.0
86.90	2754.0
88.00	2297.0
91.00	389.0
91.90	2268.0
92.90	3504.0
94.00	9543.0
95.00	71672.0
96.00	4832.0
103.80	384.0
104.90	159.0
105.90	431.0
106.80	121.0
110.90	112.0
112.80	128.0
115.90	304.0
116.90	542.0
117.90	330.0
118.80	495.0
127.80	245.0
129.90	241.0
134.80	254.0
136.80	118.0
140.90	907.0
141.90	149.0
142.80	1139.0
144.80	128.0
145.80	108.0
147.70	143.0
149.80	102.0
154.90	192.0
156.80	129.0
171.00	151.0
171.90	735.0
173.90	61296.0
175.00	4831.0
175.90	58704.0
176.90	3510.0

Instrument :
MSVOA_U
ClientSampleId :
BFB29

m/z	Abundance
35.90	1262.0
37.00	5210.0
38.00	4647.0
39.00	1843.0
40.00	137.0
43.90	811.0
45.00	817.0
46.90	921.0
47.90	623.0
49.00	4209.0
50.00	18568.0
51.00	5581.0
51.90	216.0
54.90	299.0
56.00	1522.0
56.90	2676.0
59.90	879.0
61.00	4413.0
62.00	4630.0
63.00	3568.0
64.00	360.0
65.00	502.0
65.80	108.0
67.00	239.0
67.90	9030.0
69.00	8859.0
70.00	790.0
72.00	591.0
73.00	4456.0
74.00	16536.0
75.00	43232.0
76.00	3717.0
76.90	413.0
78.90	3810.0
79.90	943.0
80.90	3726.0
81.90	831.0
86.10	127.0
86.90	3037.0
87.90	2534.0
91.00	381.0
91.90	2477.0
92.90	3834.0
94.00	10644.0
95.00	77232.0
96.00	5222.0
103.80	423.0
104.90	163.0
105.90	440.0
106.80	153.0
110.90	108.0
115.90	315.0
116.90	612.0
117.90	376.0
118.90	503.0
127.80	313.0
129.80	261.0
134.80	243.0
136.80	113.0
140.90	1092.0
141.80	156.0
142.80	1260.0
143.80	118.0
144.80	132.0
145.80	106.0
147.60	126.0
147.90	121.0
149.80	135.0
154.80	200.0
156.80	157.0
158.80	124.0
171.00	158.0
171.90	797.0
173.90	67952.0
175.00	5364.0
175.90	65304.0
176.90	3813.0

Instrument :
MSVOA_U
ClientSampleId :
BFB29

m/z	Abundance
35.90	1262.0
37.00	4909.0
38.00	4581.0
39.00	1839.0
40.00	123.0
43.90	850.0
45.00	803.0
46.90	868.0
47.90	549.0
49.00	4032.0
50.00	18240.0
51.00	5231.0
51.90	226.0
54.90	305.0
55.90	1520.0
56.90	2695.0
59.90	913.0
61.00	4122.0
62.00	4565.0
63.00	3410.0
64.00	341.0
65.00	439.0
65.80	131.0
67.00	256.0
67.90	8846.0
69.00	9045.0
70.00	747.0
72.00	551.0
72.90	4195.0
74.00	16245.0
75.00	42584.0
76.00	3740.0
77.00	377.0
78.10	312.0
78.90	3890.0
79.90	985.0
80.90	3756.0
81.90	813.0
86.90	3051.0
87.90	2547.0
90.90	318.0
92.00	2513.0
92.90	3744.0
94.00	10814.0
95.00	75184.0
96.00	5154.0
103.80	458.0
104.90	172.0
105.90	409.0
106.80	148.0
110.90	100.0
115.80	305.0
116.90	681.0
117.90	373.0
118.90	486.0
127.80	332.0
129.80	288.0
134.80	202.0
136.80	131.0
140.90	1145.0
141.80	132.0
142.80	1144.0
144.80	122.0
145.70	155.0
147.90	142.0
149.80	154.0
154.80	175.0
156.80	156.0
158.80	114.0
160.80	111.0
171.00	137.0
171.90	811.0
173.90	68616.0
174.90	5391.0
175.90	65472.0
176.90	3901.0
177.80	103.0

Instrument :
MSVOA_U
ClientSampleId :
BFB29