

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032923\
 Data File : VU053470.D
 Acq On : 29 Mar 2023 17:42
 Operator : JC/MD
 Sample : VU0329WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0329WBL01

Quant Time: Mar 30 14:08:49 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U032923DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Thu Mar 30 13:33:10 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Fluorobenzene	6.111	96	44195	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.629	95	13880	0.870	ug/l	0.00
Spiked Amount 1.000			Recovery	=	87.000%	
68) 1,2-Dichlorobenzene-d4	12.188	152	13579	0.848	ug/l	0.00
Spiked Amount 1.000			Recovery	=	85.000%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032923\
Data File : VU053470.D
Acq On : 29 Mar 2023 17:42
Operator : JC/MD
Sample : VU0329WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0329WBL01

Quant Time: Mar 30 14:08:49 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U032923DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Thu Mar 30 13:33:10 2023
Response via : Initial Calibration




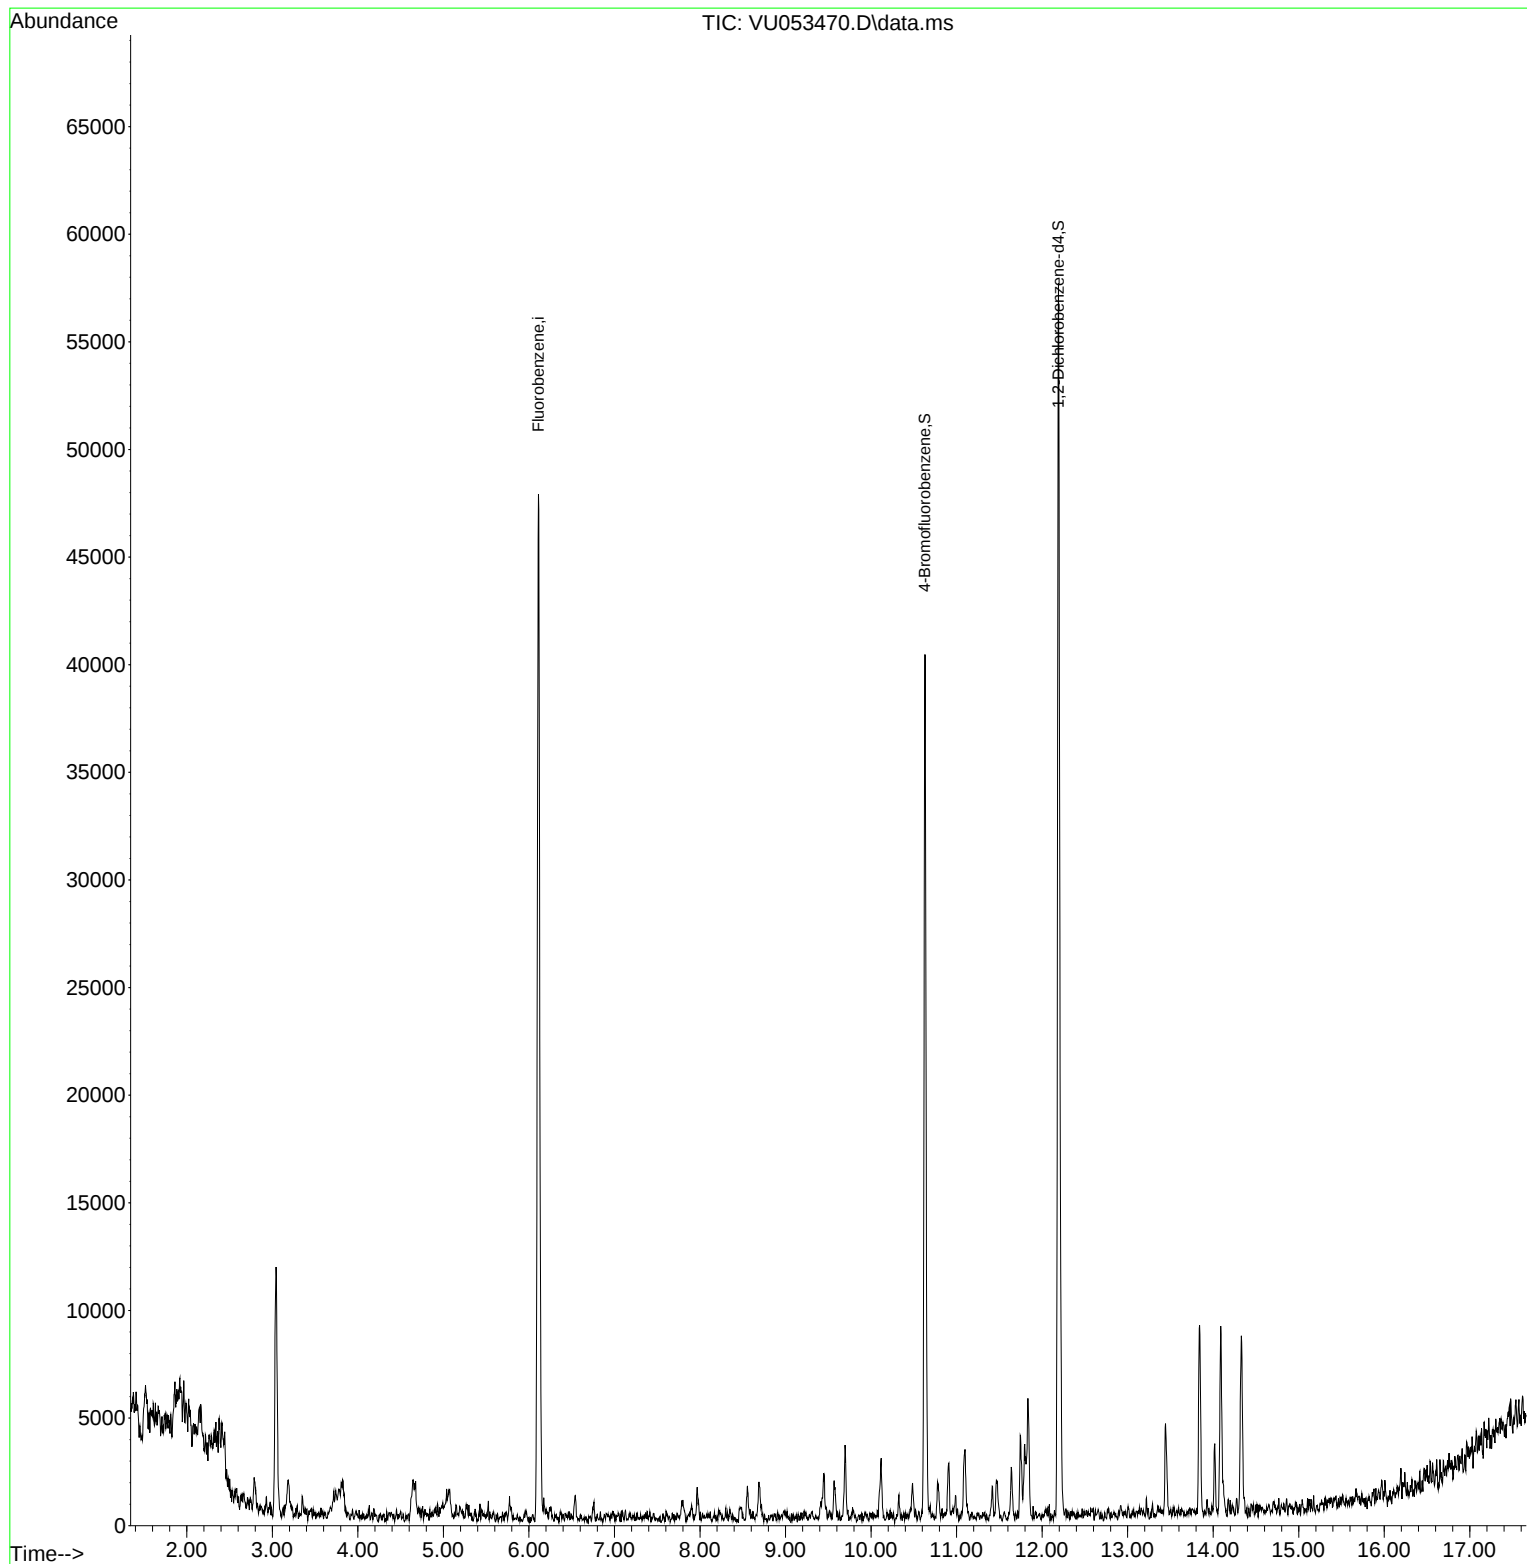


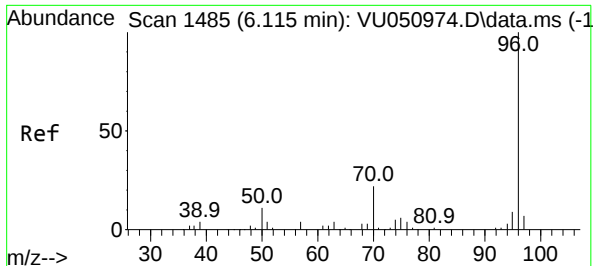

#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.111 min Scan# 1485
Delta R.T. -0.004 min
Lab File: VU053470.D
Acq: 29 Mar 2023 17:42




Instrument :
MSVOA_U
ClientSampleId :
VU0329WBL01


Tgt Ion: 96	Resp: 44195
Ion Ratio	Lower Upper
96 100	
70 21.6	16.5 24.7
95 9.0	7.4 11.0
97 6.7	0.0 0.0

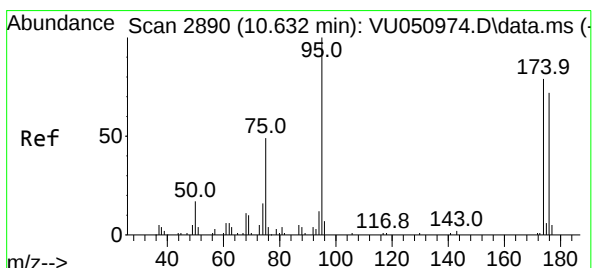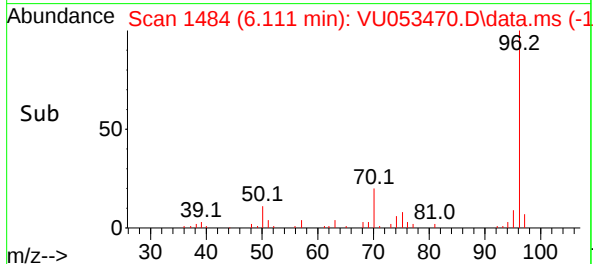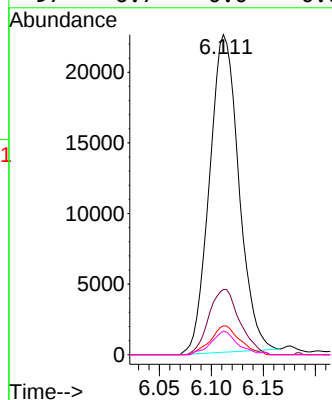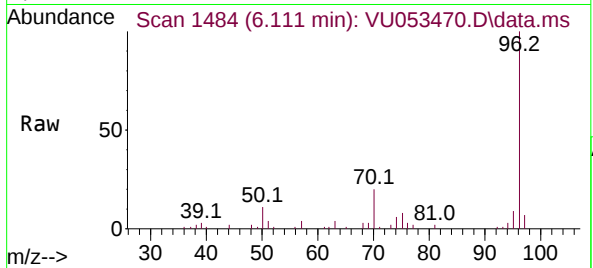

#57
4-Bromofluorobenzene
Concen: 0.870 ug/l
RT: 10.629 min Scan# 2889
Delta R.T. -0.003 min
Lab File: VU053470.D
Acq: 29 Mar 2023 17:42


Tgt Ion: 95	Resp: 13880
Ion Ratio	Lower Upper
95 100	
174 72.9	63.3 94.9
176 69.3	59.3 88.9

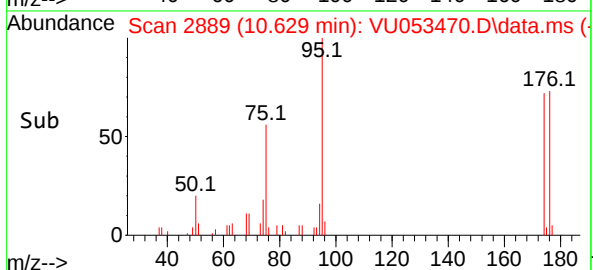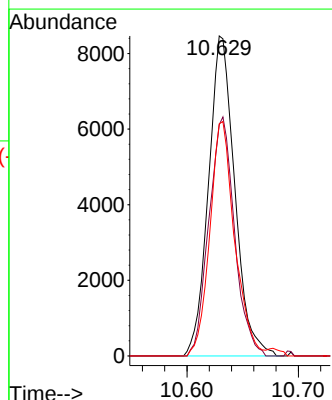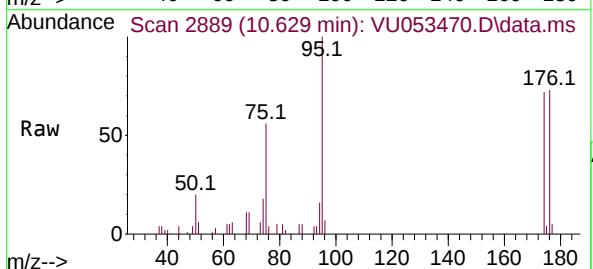

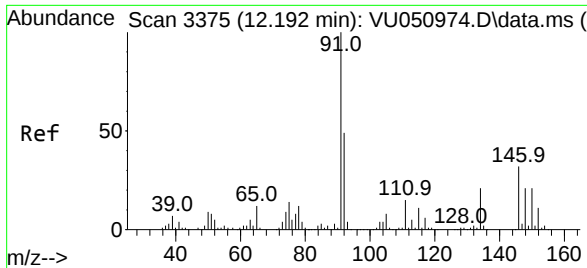

#68
 1,2-Dichlorobenzene-d4
 Concen: 0.848 ug/l
 RT: 12.188 min Scan# 31
 Delta R.T. -0.003 min
 Lab File: VU053470.D
 Acq: 29 Mar 2023 17:42

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0329WBL01

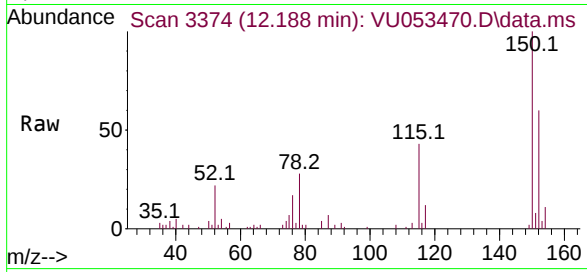

Tgt Ion:	152	Resp:	13579
Ion	Ratio	Lower	Upper
152	100		
115	69.5	0.0	308.8
150	170.2	0.0	635.0

