


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032923\
Data File : VU053462.D
Acq On : 29 Mar 2023 09:33
Operator : JC/MD
Sample : BFB
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U032923DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER
Last Update : Thu Mar 30 13:33:10 2023

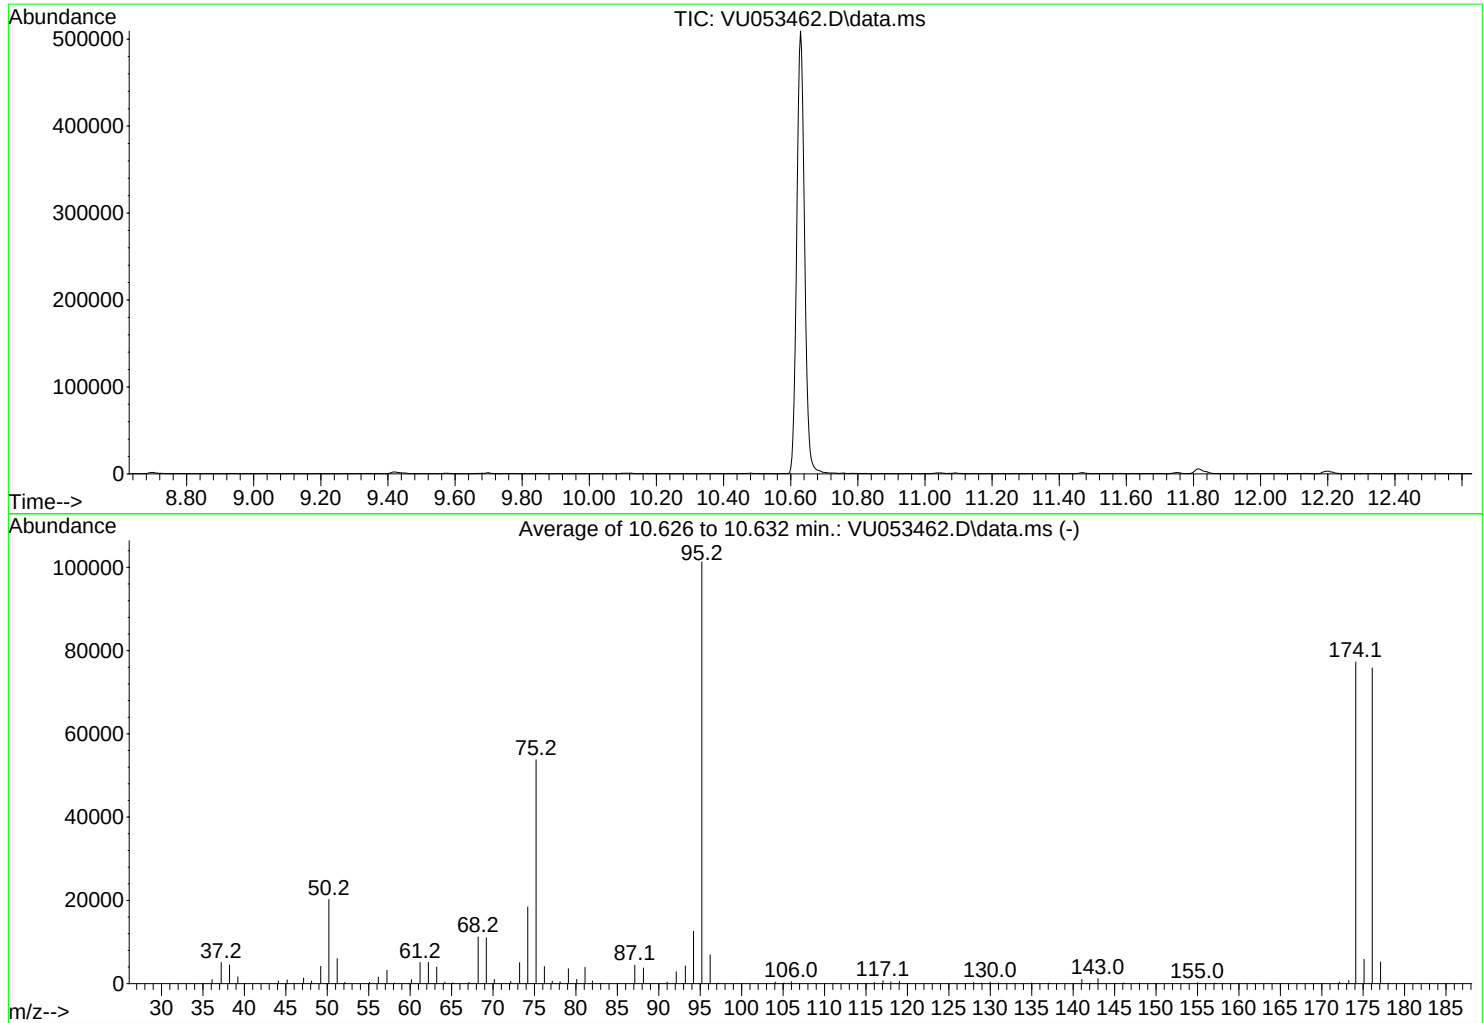

AutoFind: Scans 2888, 2889, 2890; Background Corrected with Scan 2875

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.9	20211	PASS
75	95	30	60	53.1	53763	PASS
95	95	100	100	100.0	101331	PASS
96	95	5	9	6.8	6924	PASS
173	174	0.00	2	1.0	745	PASS
174	95	50	100	76.2	77256	PASS
175	174	5	9	7.6	5870	PASS
176	174	95	101	98.2	75853	PASS
177	176	5	9	6.8	5172	PASS