

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032924\
 Data File : VU058264.D
 Acq On : 29 Mar 2024 13:09
 Operator : MD/SY
 Sample : P1902-13
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DCOC2

Quant Time: Mar 29 23:41:49 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032124WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Mar 29 23:40:26 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	69887	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	65934	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	28460	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.596	65	30382	5.144	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	102.800%	
7) Chloroethane-d5	1.907	69	27001	5.601	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	112.000%	
11) 1,1-Dichloroethene-d2	2.560	65	12652	5.160	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	103.200%	
20) 2-Butanone-d5	4.624	46	52630	50.161	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	100.320%	
24) Chloroform-d	5.052	84	52663	4.988	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	99.800%	
26) 1,2-Dichloroethane-d4	5.692	65	25417	5.149	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	103.000%	
32) Benzene-d6	5.718	84	108414	5.062	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	101.200%	
36) 1,2-Dichloropropane-d6	6.682	67	33223	5.264	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	105.200%	
41) Toluene-d8	7.891	98	93536	4.930	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	98.600%	
43) trans-1,3-Dichloroprop...	8.177	79	9612	4.753	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	95.000%	
46) 2-Hexanone-d5	8.627	63	39022	47.646	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	95.300%	
56) 1,1,2,2-Tetrachloroeth...	10.749	84	20836	5.067	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	101.400%	
66) 1,2-Dichlorobenzene-d4	12.187	152	28722	5.419	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	108.400%	
Target Compounds						Qvalue
22) cis-1,2-Dichloroethene	4.663	96	1692	0.374	ug/L	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032924\
Data File : VU058264.D
Acq On : 29 Mar 2024 13:09
Operator : MD/SY
Sample : P1902-13
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCOC2

Quant Time: Mar 29 23:41:49 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032124WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Mar 29 23:40:26 2024
Response via : Initial Calibration

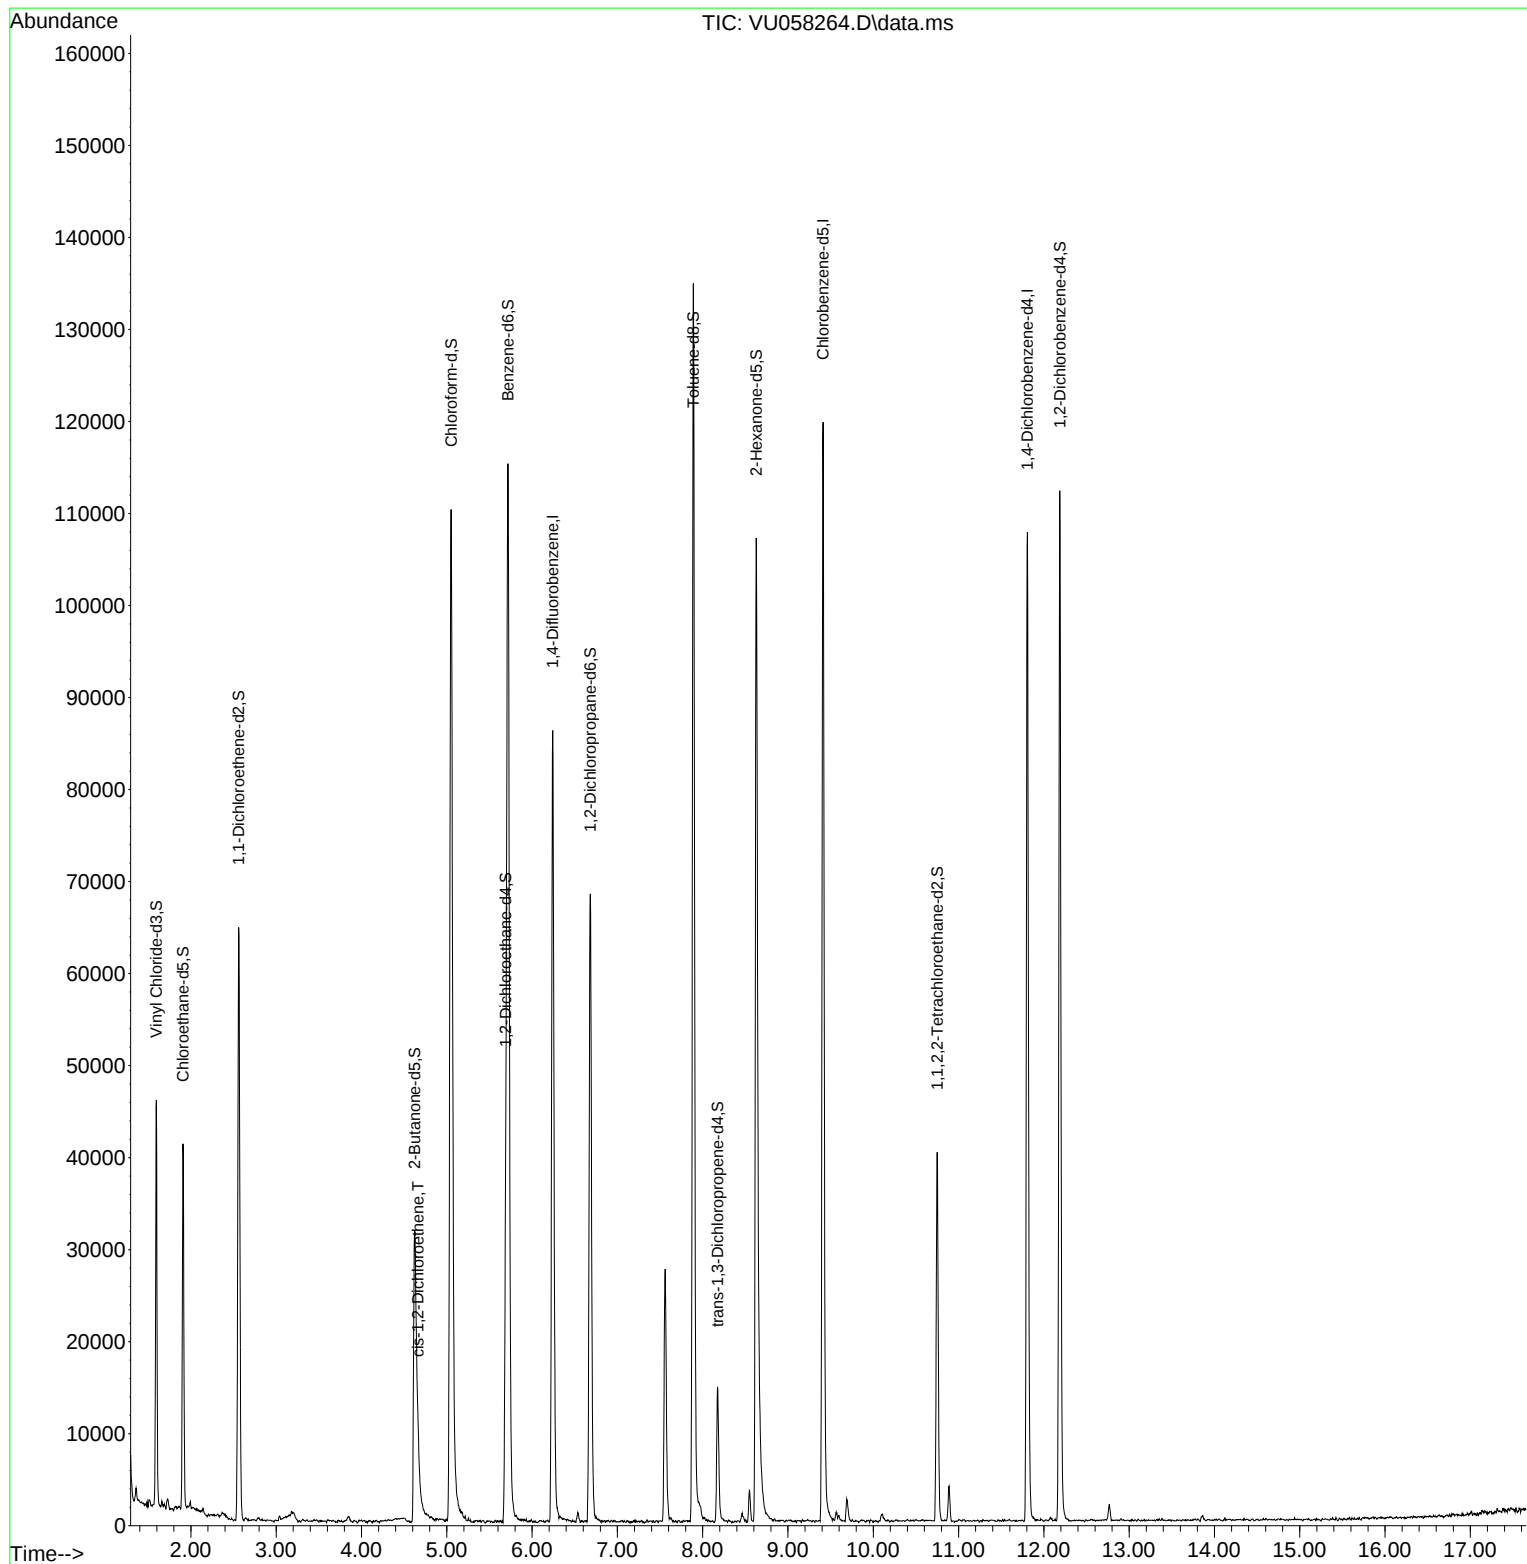

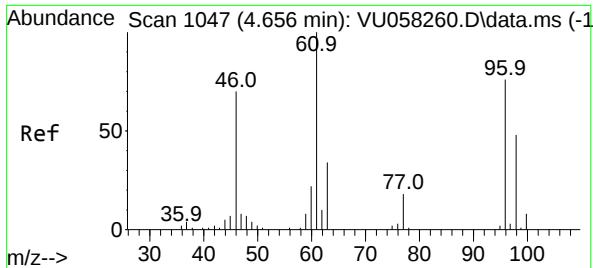

#22
 cis-1,2-Dichloroethene
 Concen: 0.374 ug/L
 RT: 4.663 min Scan# 10
 Delta R.T. 0.007 min
 Lab File: VU058264.D
 Acq: 29 Mar 2024 13:09

Instrument :
 MSVOA_U
 ClientSampleId :
 DCOC2

Tgt Ion: 96	Resp:	1692
Ion	Ratio	Lower Upper
96	100	
61	154.9	92.8 172.4
98	63.4	43.2 80.2

