

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032924\
 Data File : VU058273.D
 Acq On : 29 Mar 2024 16:39
 Operator : MD/SY
 Sample : P1902-11DL 100X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DCOC0DL

Quant Time: Mar 29 23:43:54 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032124WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Mar 29 23:40:26 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	67559	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	63512	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	28740	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.592	65	17990	3.151	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	63.000%	
7) Chloroethane-d5	1.907	69	19647	4.216	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	84.400%	
11) 1,1-Dichloroethene-d2	2.560	65	7947	3.353	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	67.000%	
20) 2-Butanone-d5	4.624	46	55548	54.767	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	109.540%	
24) Chloroform-d	5.052	84	43538	4.266	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	85.400%	
26) 1,2-Dichloroethane-d4	5.692	65	22347	4.683	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	93.600%	
32) Benzene-d6	5.718	84	83301	4.038	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	80.800%	
36) 1,2-Dichloropropane-d6	6.682	67	27802	4.573	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	91.400%	
41) Toluene-d8	7.891	98	66645	3.647	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	73.000%	
43) trans-1,3-Dichloroprop...	8.177	79	7936	4.074	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	81.400%	
46) 2-Hexanone-d5	8.627	63	40945	51.900	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	103.800%	
56) 1,1,2,2-Tetrachloroeth...	10.749	84	19505	4.925	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	98.400%	
66) 1,2-Dichlorobenzene-d4	12.190	152	24607	4.598	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	92.000%	
Target Compounds						Qvalue
22) cis-1,2-Dichloroethene	4.653	96	3210	0.734	ug/L	97
34) Trichloroethene	6.534	95	17718	4.077	ug/L	97
47) Tetrachloroethene	8.547	164	15339	5.270	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032924\
Data File : VU058273.D
Acq On : 29 Mar 2024 16:39
Operator : MD/SY
Sample : P1902-11DL 100X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCOC0DL

Quant Time: Mar 29 23:43:54 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032124WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Mar 29 23:40:26 2024
Response via : Initial Calibration




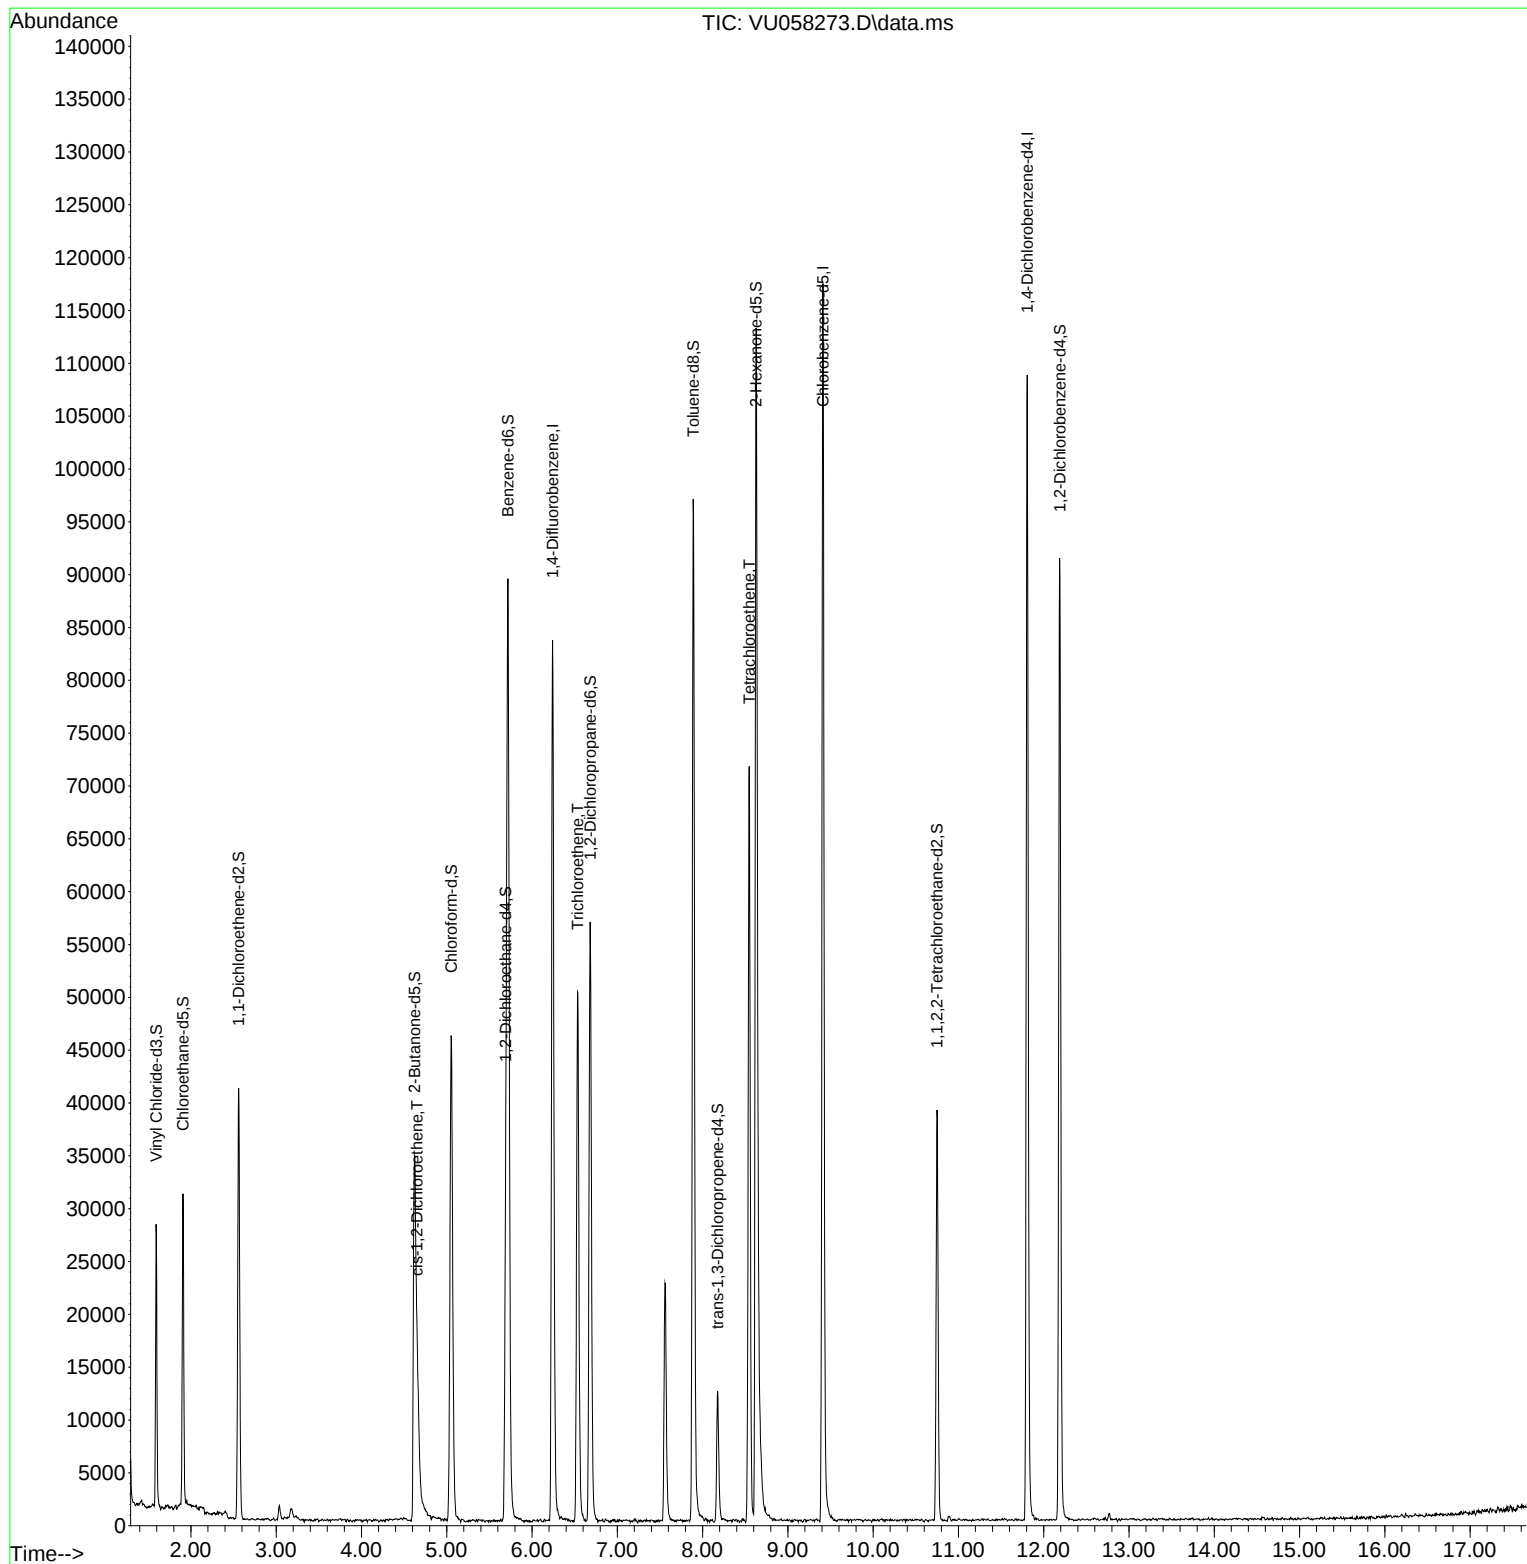


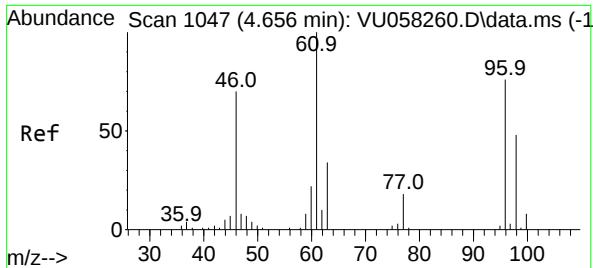

#22
 cis-1,2-Dichloroethene
 Concen: 0.734 ug/L
 RT: 4.653 min Scan# 1046
 Delta R.T. -0.003 min
 Lab File: VU058273.D
 Acq: 29 Mar 2024 16:39




Instrument :
 MSVOA_U
 ClientSampleId :
 DCOC0DL


Tgt Ion: 96 Resp: 3210
 Ion Ratio Lower Upper
 96 100
 61 128.2 92.8 172.4
 98 63.7 43.2 80.2

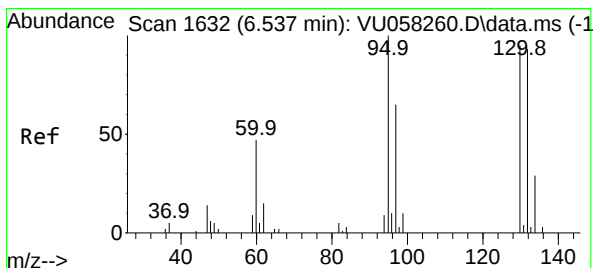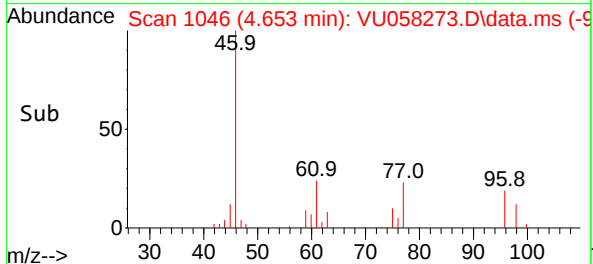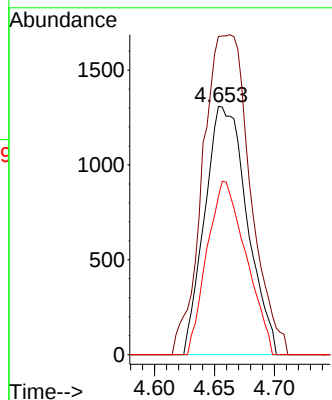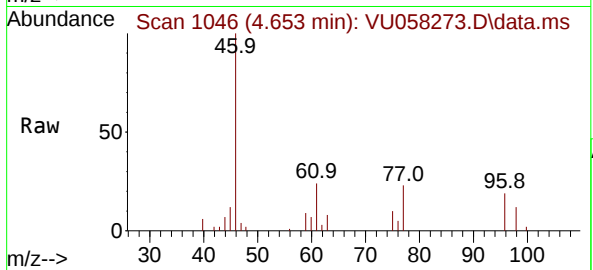

#34
 Trichloroethene
 Concen: 4.077 ug/L
 RT: 6.534 min Scan# 1631
 Delta R.T. -0.003 min
 Lab File: VU058273.D
 Acq: 29 Mar 2024 16:39


Tgt Ion: 95 Resp: 17718
 Ion Ratio Lower Upper
 95 100
 97 63.1 47.7 88.7
 132 93.3 63.6 118.2
 130 94.9 65.1 120.9

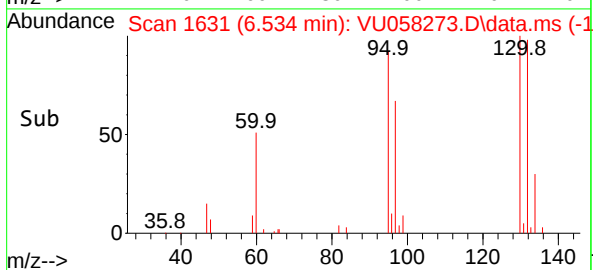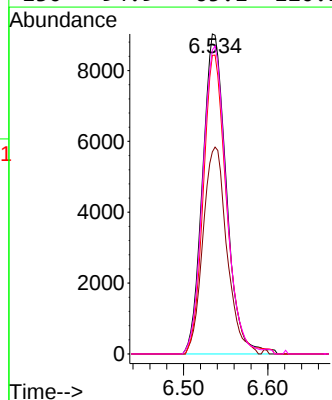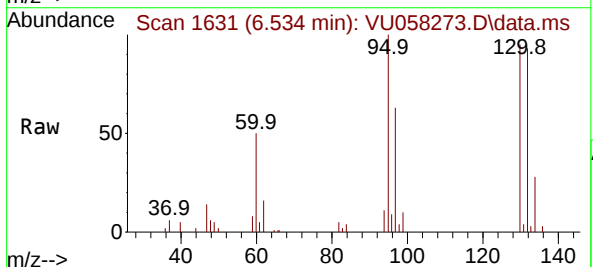

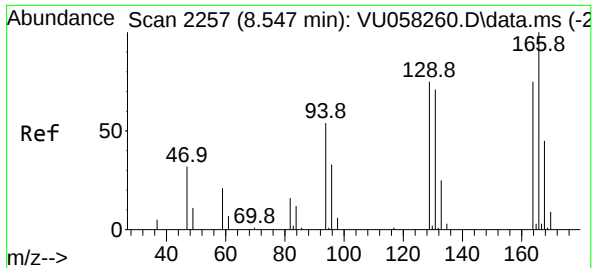

#47
 Tetrachloroethene
 Concen: 5.270 ug/L
 RT: 8.547 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: VU058273.D
 Acq: 29 Mar 2024 16:39

Instrument :
 MSVOA_U
 ClientSampleId :
 DCOC0DL

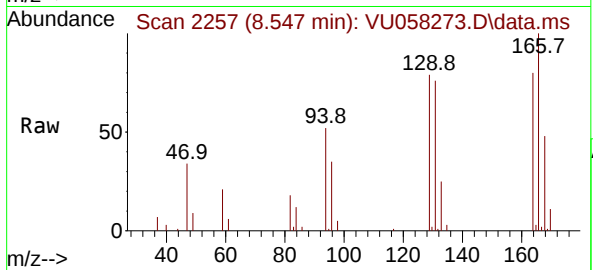

Tgt Ion:	164	Resp:	15339
Ion	Ratio	Lower	Upper
164	100		
129	99.6	71.3	132.3
131	95.5	70.8	131.4
166	125.4	90.9	168.9

