


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU032924\
Data File : VU058259.D
Acq On : 29 Mar 2024 09:16
Operator : MD/SY
Sample : BFB132
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB132

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032124WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Wed Apr 03 01:56:26 2024

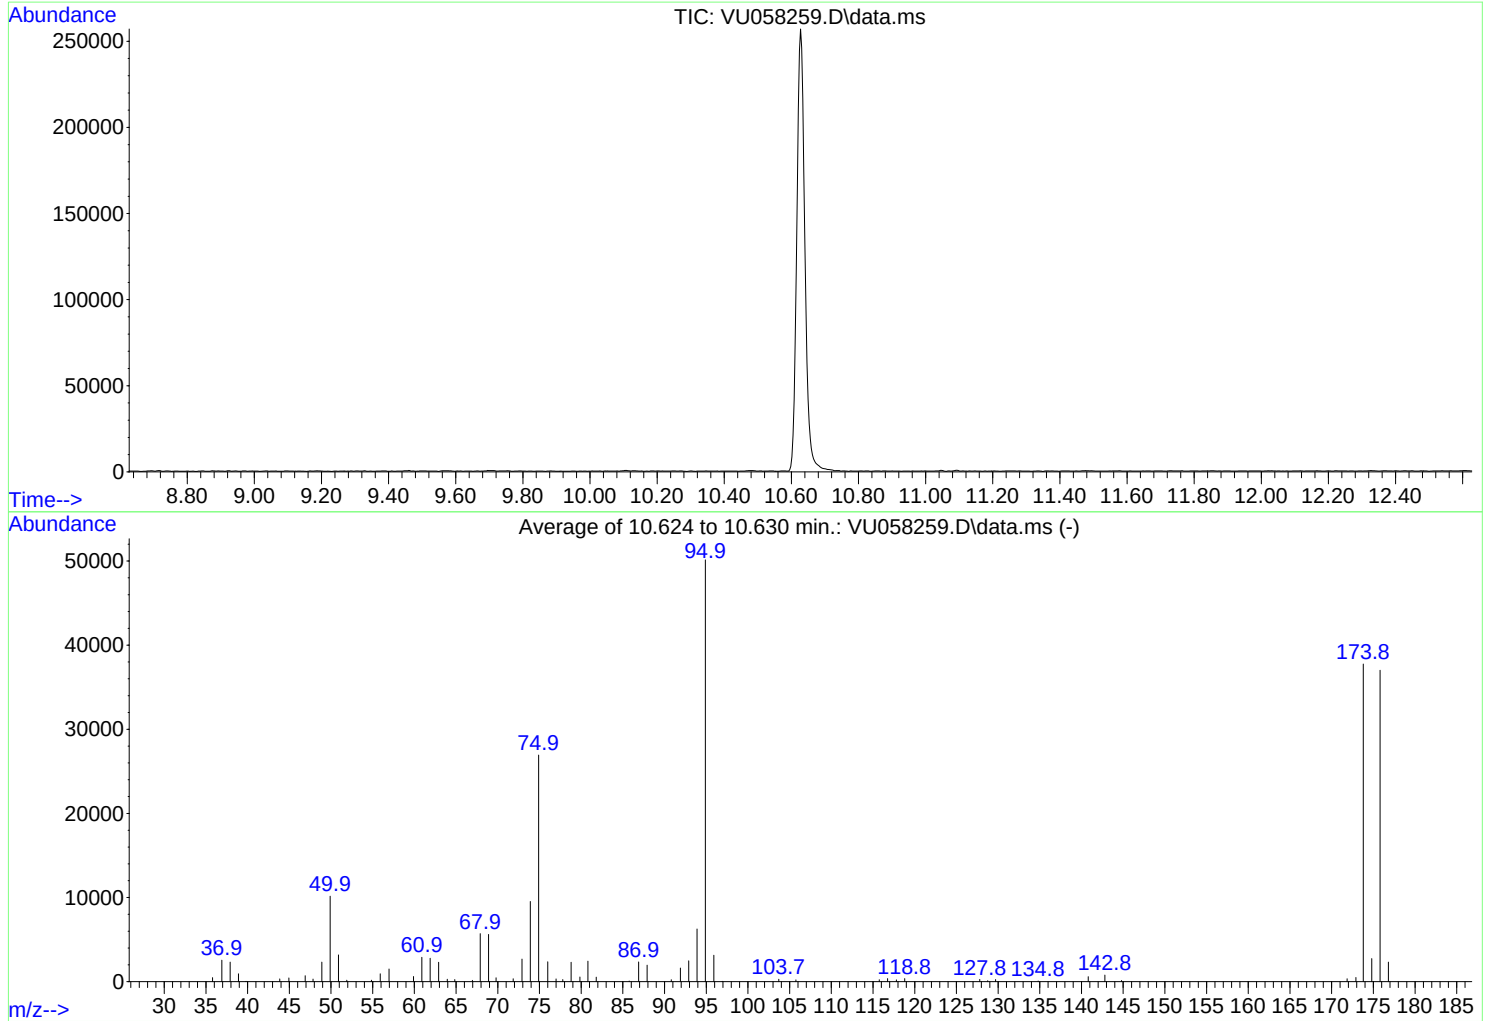

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.3	10161	PASS
75	95	30	80	53.7	26931	PASS
95	95	100	100	100.0	50144	PASS
96	95	5	9	6.3	3149	PASS
173	174	0.00	2	1.3	498	PASS
174	95	50	120	75.3	37752	PASS
175	174	5	9	7.3	2748	PASS
176	174	95	101	98.0	37008	PASS
177	176	5	9	6.3	2327	PASS

Scan 2890 (10.582 min): VU058259.D\data.ms
BFB132

m/z	Abundance
39.80	393.0
43.80	131.0

Instrument :
MSVOA_U
ClientSampleId :
BFB132

m/z	Abundance
35.80	523.0
36.90	2574.0
37.90	2292.0
38.90	1024.0
39.80	463.0
43.90	448.0
44.90	411.0
46.90	669.0
47.90	319.0
48.90	2362.0
49.90	10085.0
50.90	3062.0
51.90	168.0
54.90	171.0
55.90	943.0
57.00	1529.0
59.90	633.0
60.90	2962.0
61.90	2789.0
62.90	2322.0
64.00	264.0
64.90	292.0
66.90	149.0
67.90	5666.0
68.90	5582.0
69.80	442.0
71.90	308.0
72.90	2578.0
73.90	9508.0
74.90	26608.0
76.00	2265.0
77.00	277.0
77.80	229.0
78.80	2258.0
79.80	555.0
80.80	2405.0
81.80	553.0
85.80	111.0
86.90	2241.0
87.90	1900.0
90.80	218.0
91.90	1484.0
92.90	2455.0
93.90	6150.0
94.90	49192.0
95.90	3218.0
96.90	133.0
103.70	288.0
105.70	197.0
115.80	237.0
116.80	348.0
117.80	219.0
118.80	359.0
127.80	250.0
128.80	108.0
129.70	227.0
134.80	111.0
140.80	575.0
142.80	747.0
144.80	121.0
171.90	371.0
172.90	455.0
173.80	36248.0
174.80	2716.0
175.80	35584.0
176.80	2289.0

Instrument :
MSVOA_U
ClientSampleId :
BFB132

m/z	Abundance
35.80	492.0
36.90	2620.0
37.90	2371.0
38.90	945.0
39.80	458.0
43.90	465.0
44.90	439.0
46.90	741.0
47.80	293.0
48.90	2387.0
49.90	10476.0
50.90	3270.0
51.90	174.0
54.80	187.0
55.90	959.0
56.90	1519.0
59.90	651.0
60.90	2984.0
61.90	2902.0
62.90	2385.0
63.90	308.0
64.90	257.0
66.90	145.0
67.90	5906.0
68.90	5752.0
69.80	461.0
71.90	355.0
72.90	2793.0
73.90	9866.0
74.90	27792.0
76.00	2448.0
77.00	334.0
77.80	264.0
78.80	2386.0
79.90	562.0
80.80	2487.0
81.80	552.0
85.70	117.0
86.90	2413.0
87.90	2022.0
90.80	247.0
91.90	1656.0
92.90	2573.0
93.90	6436.0
94.90	51792.0
95.90	3246.0
103.70	314.0
105.80	217.0
115.80	248.0
116.70	369.0
117.80	209.0
118.80	377.0
127.80	268.0
128.80	127.0
129.70	260.0
134.80	108.0
140.80	602.0
142.80	805.0
144.80	136.0
171.90	369.0
172.90	516.0
173.80	38816.0
174.80	2820.0
175.80	38240.0
176.80	2387.0

Instrument :
MSVOA_U
ClientSampleId :
BFB132

m/z	Abundance
35.80	420.0
36.90	2484.0
37.90	2300.0
38.90	814.0
39.80	399.0
43.90	454.0
45.00	459.0
46.90	712.0
47.80	297.0
48.90	2222.0
49.90	9922.0
50.90	3184.0
51.90	161.0
54.80	181.0
55.90	902.0
56.90	1434.0
59.90	565.0
60.90	2749.0
61.90	2631.0
62.90	2176.0
63.90	306.0
64.80	219.0
67.00	148.0
67.90	5565.0
68.90	5484.0
69.80	449.0
71.80	383.0
72.90	2667.0
73.90	9229.0
74.90	26392.0
76.00	2346.0
77.00	376.0
77.80	237.0
78.80	2253.0
79.90	556.0
80.80	2385.0
81.80	499.0
86.90	2359.0
87.90	1934.0
90.80	232.0
91.90	1685.0
92.90	2387.0
93.90	6189.0
94.90	49448.0
95.90	2982.0
103.70	277.0
105.80	235.0
115.70	228.0
116.70	377.0
117.80	193.0
118.80	376.0
127.80	256.0
128.70	116.0
129.70	254.0
140.80	569.0
142.80	795.0
144.80	157.0
171.80	308.0
172.90	522.0
173.80	38192.0
174.80	2708.0
175.80	37200.0
176.80	2306.0

Instrument :
MSVOA_U
ClientSampleId :
BFB132