
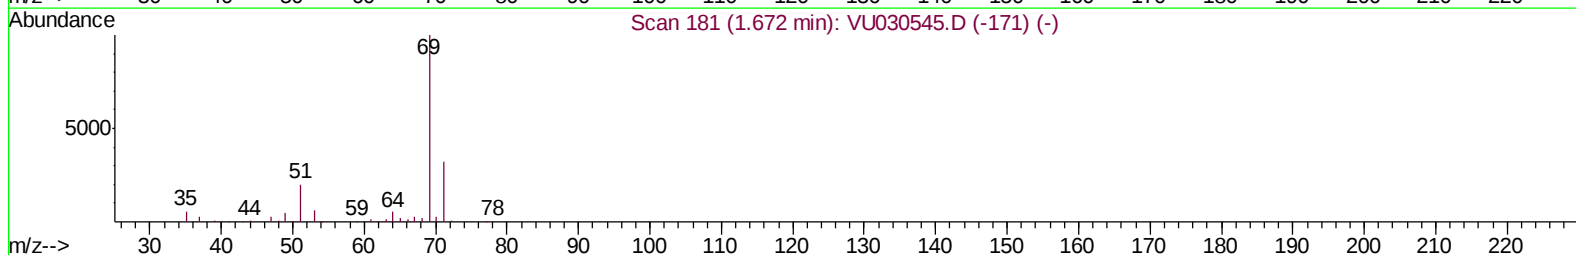
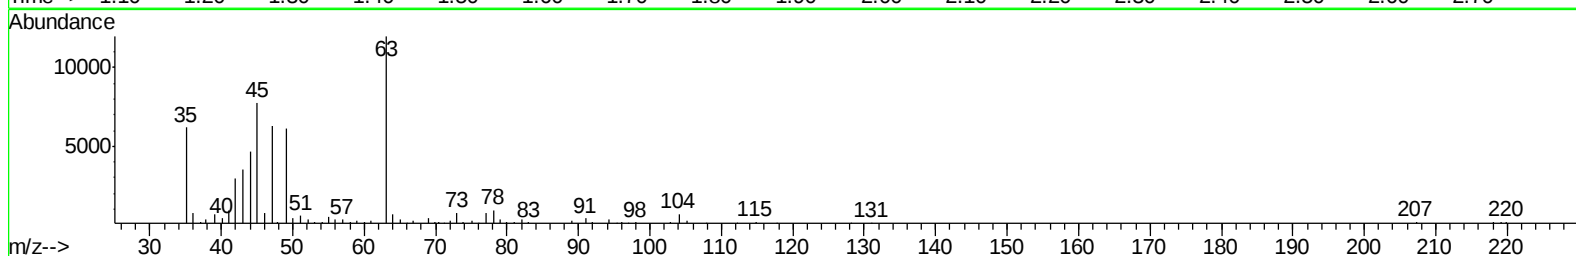


Data File : VU030560.D
Acq On : 29 Mar 2019 22:30
Operator : JC/SP
Sample : K2101-16ME
Misc : 4.47g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 17 Sample Multiplier: 1

Quant Time: Mar 30 02:17:27 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 30 02:12:04 2019
Response via : Initial Calibration

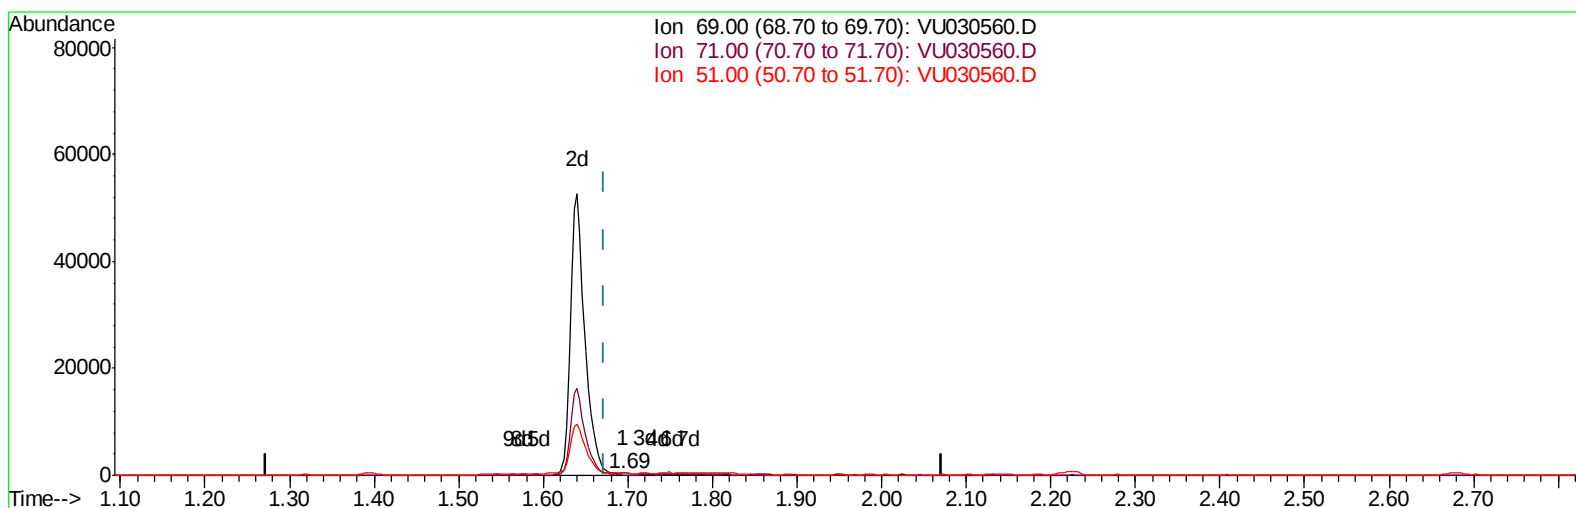

TIC: VU030560.D

(7) Chloroethane-d5 (S)

1.695min (+0.023) 0.08ug/L

response 199

Ion	Exp%	Act%
69.00	100	100
71.00	31.70	0.00#
51.00	28.60	0.00#
0.00	0.00	0.00