
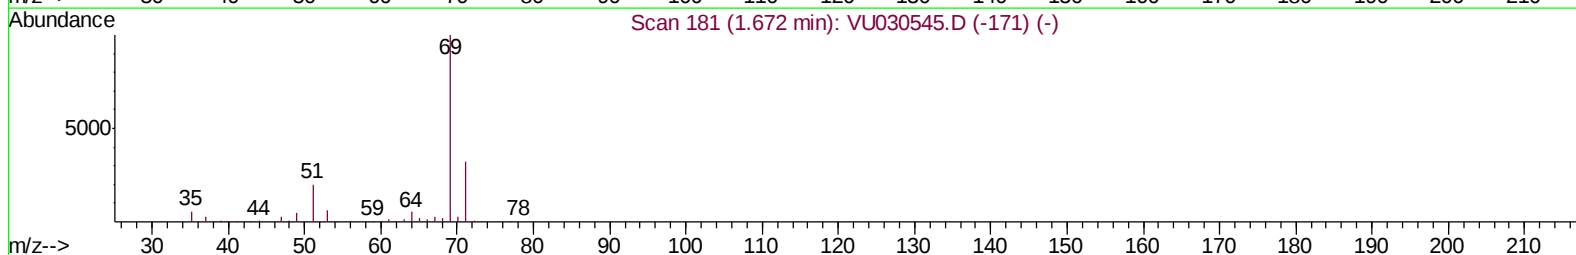
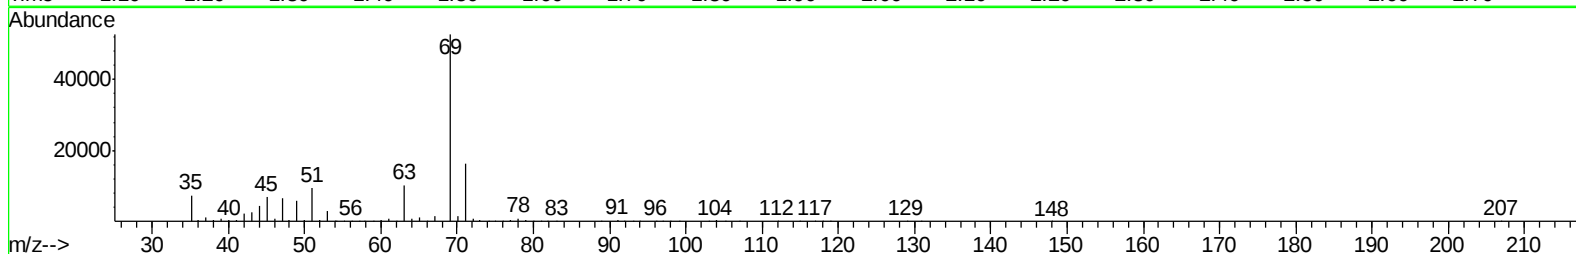


Data File : VU030560.D
Acq On : 29 Mar 2019 22:30
Operator : JC/SP
Sample : K2101-16ME
Misc : 4.47g/5mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 17 Sample Multiplier: 1

Quant Time: Mar 30 02:17:27 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 30 02:12:04 2019
Response via : Initial Calibration

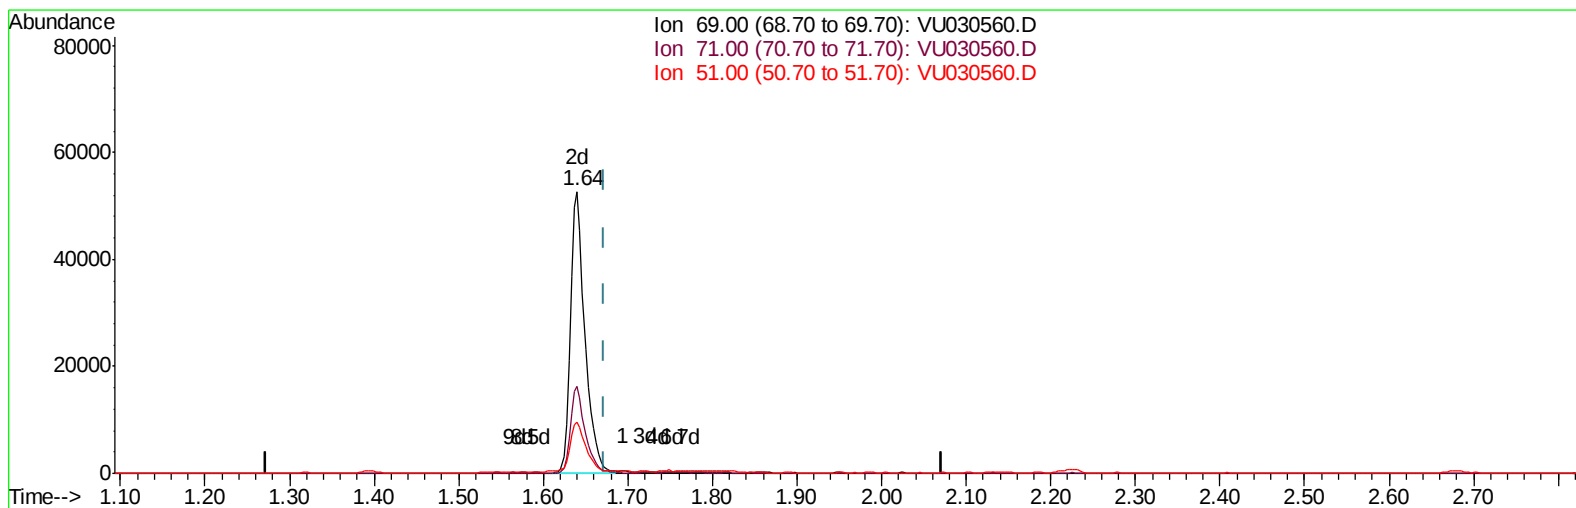

TIC: VU030560.D

(7) Chloroethane-d5 (S)
1.640min (-0.032) 23.89ug/L m
response 63016
Ion Exp% Act%
69.00 100 100
71.00 31.70 0.00#
51.00 28.60 0.00#
0.00 0.00 0.00