

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU033019\
Quantitation Report (QT Reviewed)


Data File : VU030562.D
Acq On : 29 Mar 2019 23:41
Operator : JC/SP
Sample : K2166-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF1A8

Manual Integrations
APPROVED

MMDadoda
3/30/2019 9:59:14 AM

Quant Time: Mar 30 03:44:54 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 30 02:12:04 2019
Response via : Initial Calibration

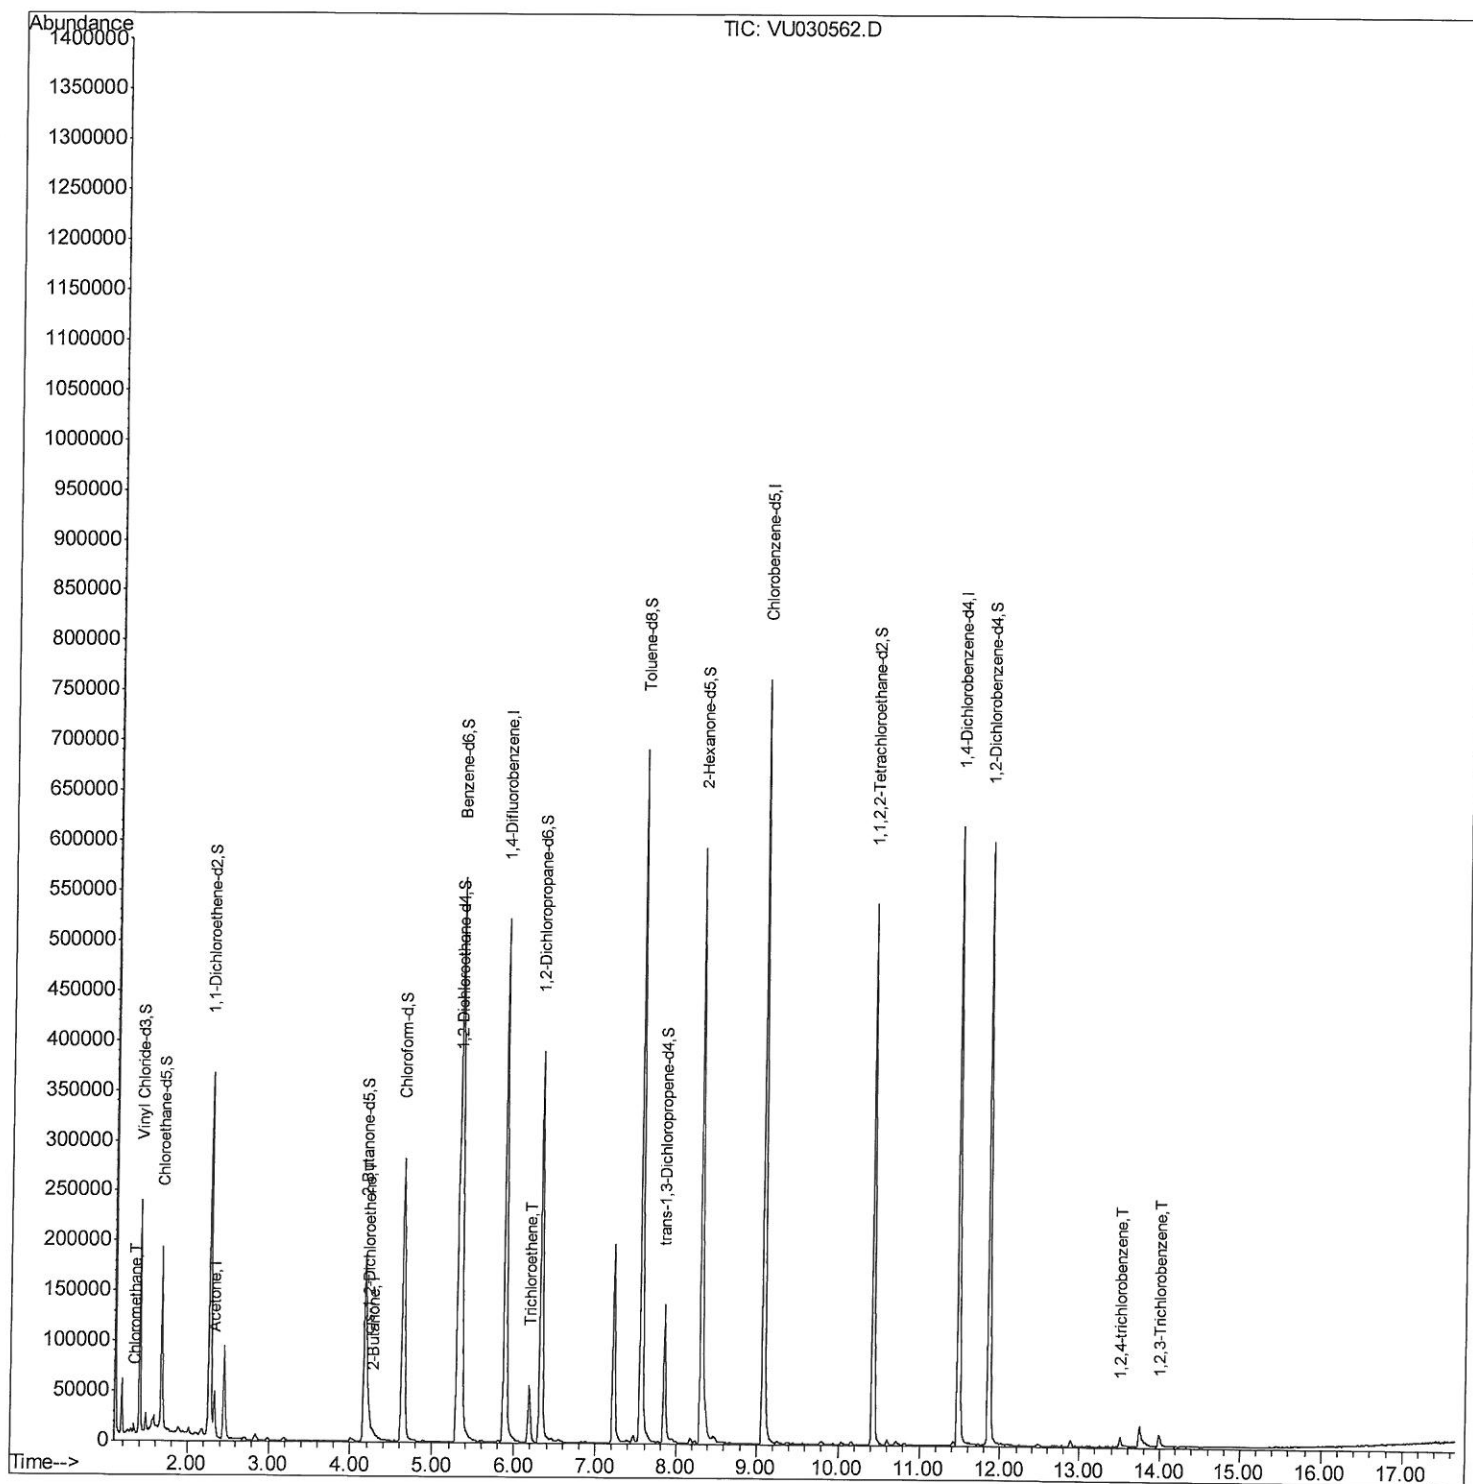

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU033019\
Quantitation Report (Qedit)




Data File : VU030562.D
Acq On : 29 Mar 2019 23:41
Operator : JC/SP
Sample : K2166-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF1A8

Manual Integrations
APPROVED

MMDadoda
3/30/2019 9:59:14 AM

Quant Time: Mar 30 02:17:50 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 30 02:12:04 2019
Response via : Initial Calibration

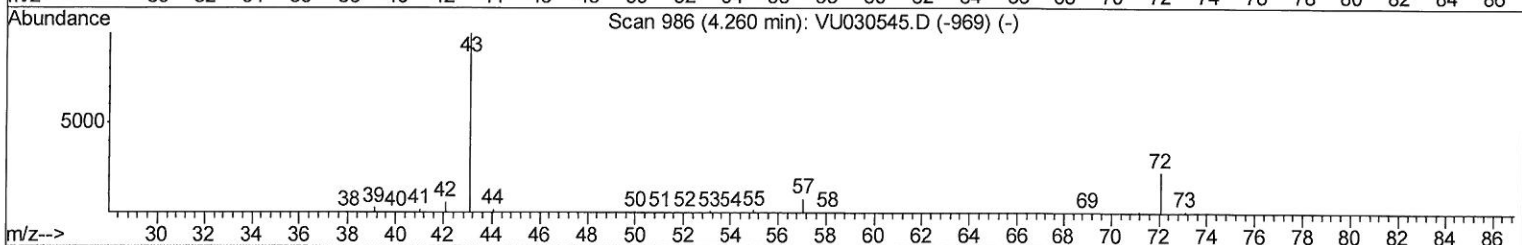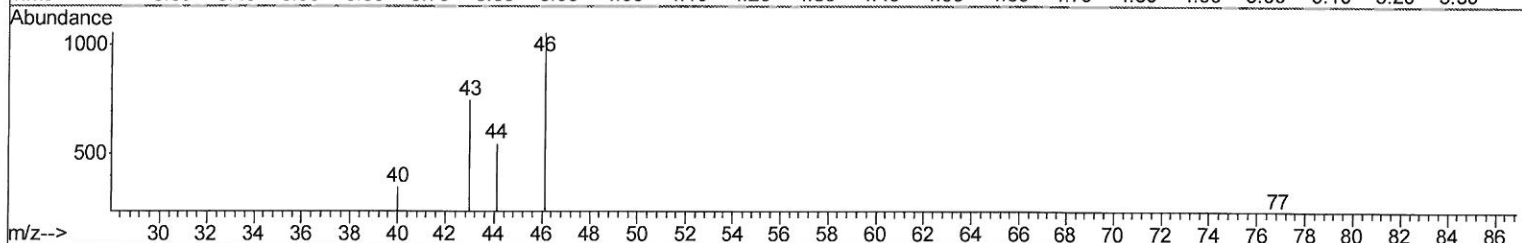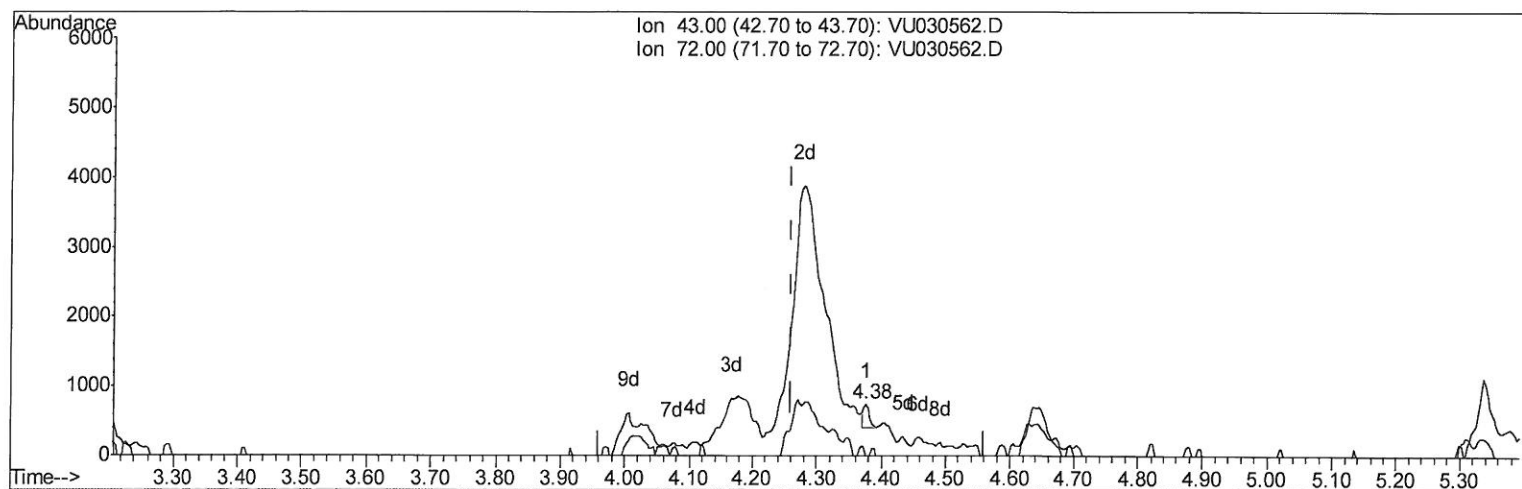

TIC: VU030562.D

(22) 2-Butanone (T)

4.376min (+0.116) 0.06ug/L

response 219

Ion	Exp%	Act%
43.00	100	100
72.00	24.10	32.42
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU033019\
Quantitation Report (Qedit)




Data File : VU030562.D
Acq On : 29 Mar 2019 23:41
Operator : JC/SP
Sample : K2166-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF1A8

Manual Integrations
APPROVED

MMDadoda
3/30/2019 9:59:14 AM

Quant Time: Mar 30 02:17:50 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 30 02:12:04 2019
Response via : Initial Calibration

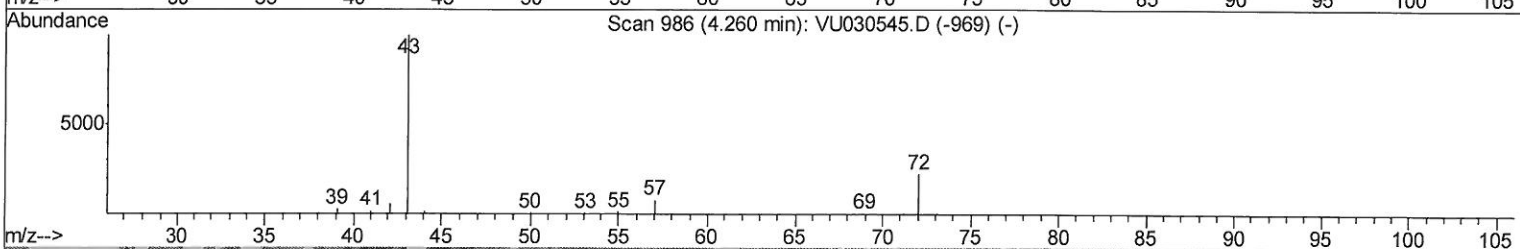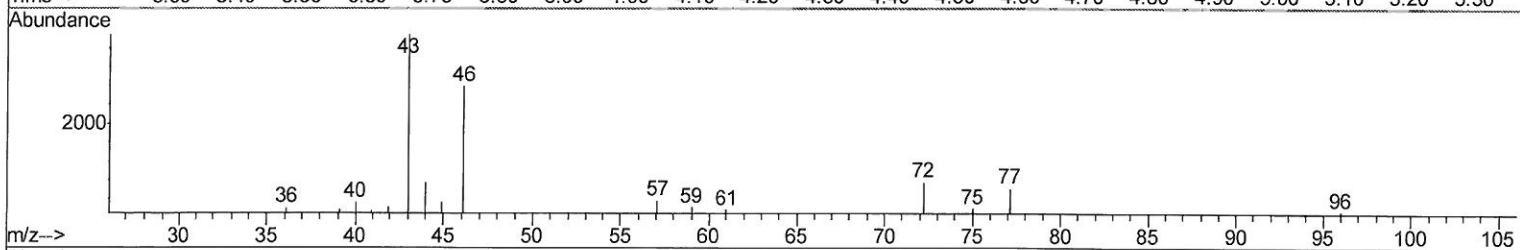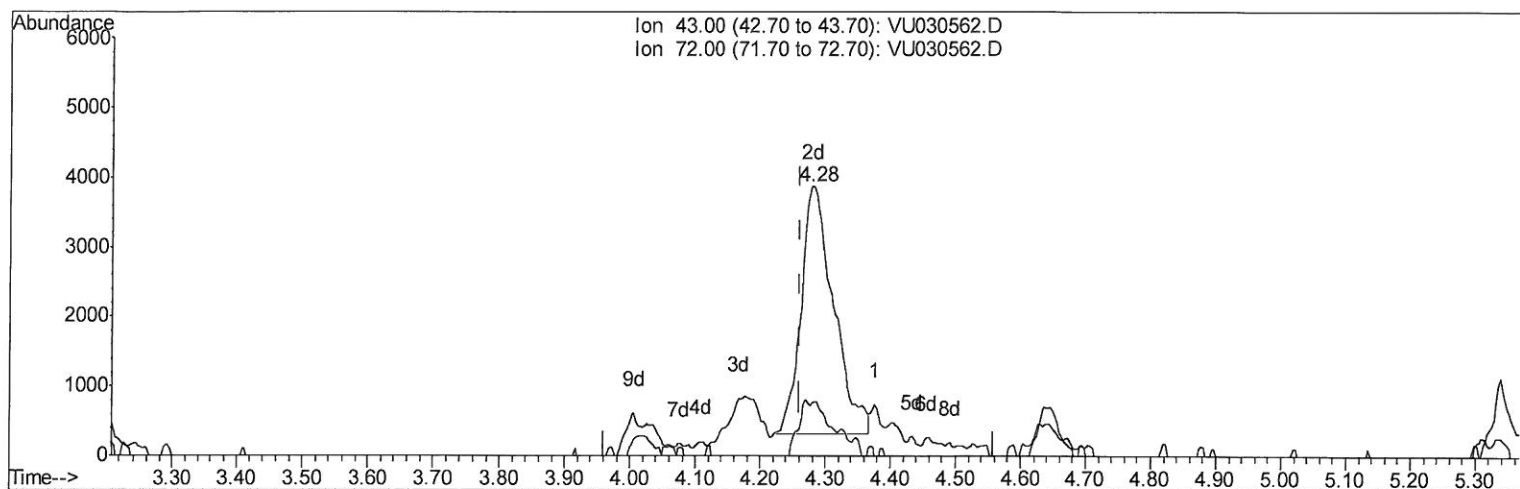

TIC: VU030562.D

(22) 2-Butanone (T)

4.280min (+0.019) 3.11ug/L m

response 12253

Ion Exp% Act%

43.00 100 100

72.00 24.10 0.58#

0.00 0.00 0.00

0.00 0.00 0.00

> MD
4/9/19

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU033019\
Quantitation Report (Qedit)




Data File : VU030562.D
Acq On : 29 Mar 2019 23:41
Operator : JC/SP
Sample : K2166-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF1A8

Manual Integrations
APPROVED

MMDadoda
3/30/2019 9:59:14 AM

Quant Time: Mar 30 02:17:50 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 30 02:12:04 2019
Response via : Initial Calibration

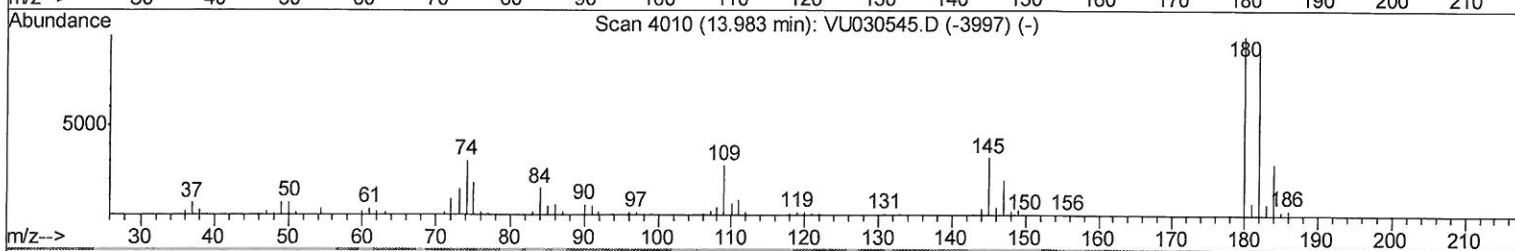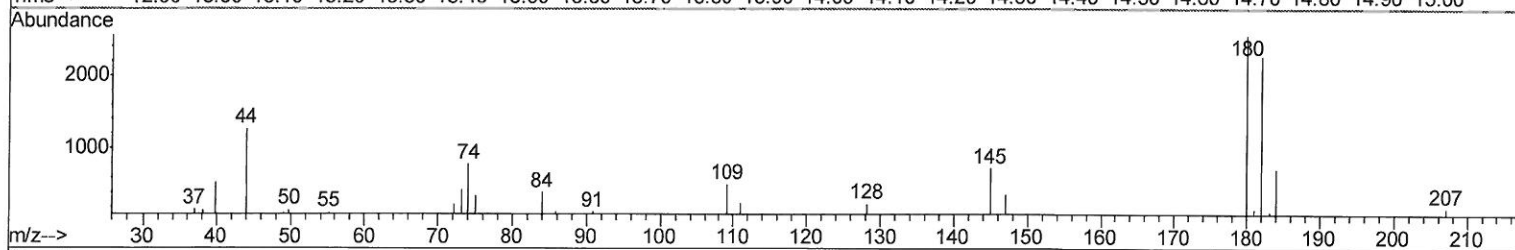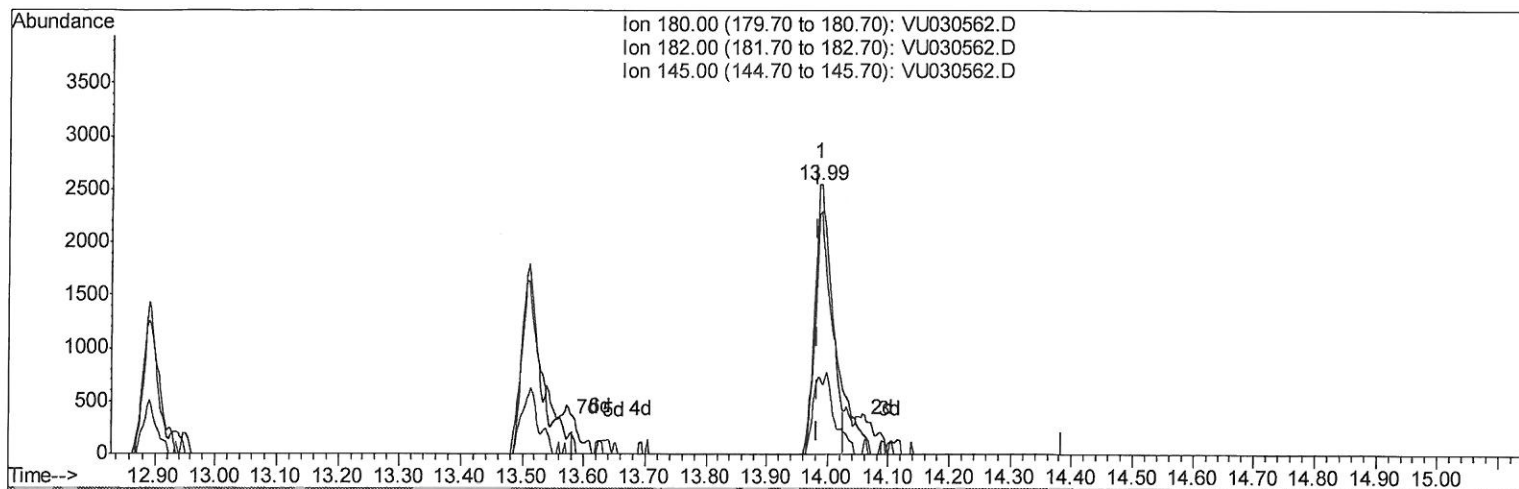

TIC: VU030562.D

(70) 1,2,3-Trichlorobenzene (T)

13.987min (+0.003) 1.40ug/L

response 4929

Ion	Exp%	Act%
180.00	100	100
182.00	96.80	101.22
145.00	32.40	17.67#
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU033019\
Quantitation Report (Qedit)




Data File : VU030562.D
Acq On : 29 Mar 2019 23:41
Operator : JC/SP
Sample : K2166-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF1A8

Manual Integrations
APPROVED

MMDadoda
3/30/2019 9:59:14 AM

Quant Time: Mar 30 02:17:50 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 30 02:12:04 2019
Response via : Initial Calibration

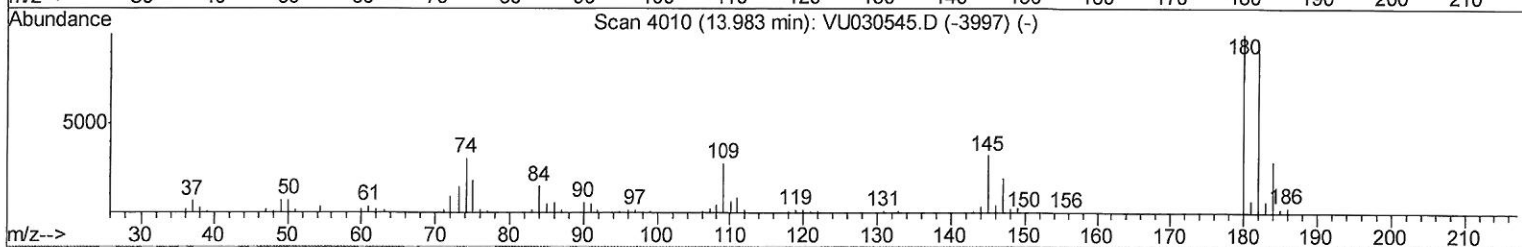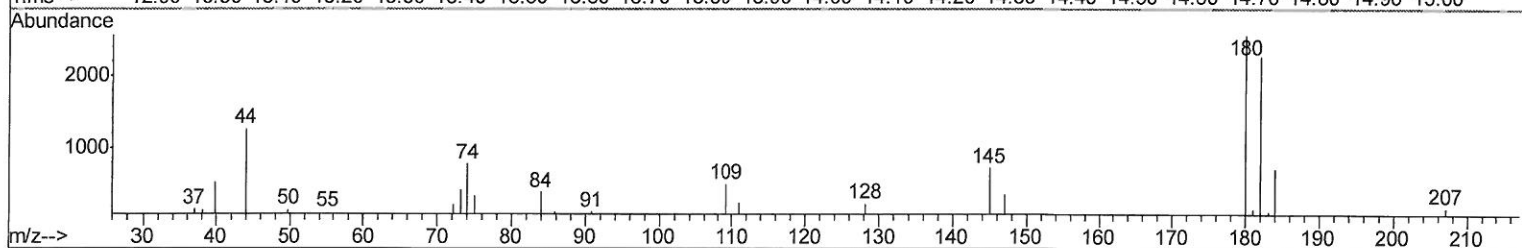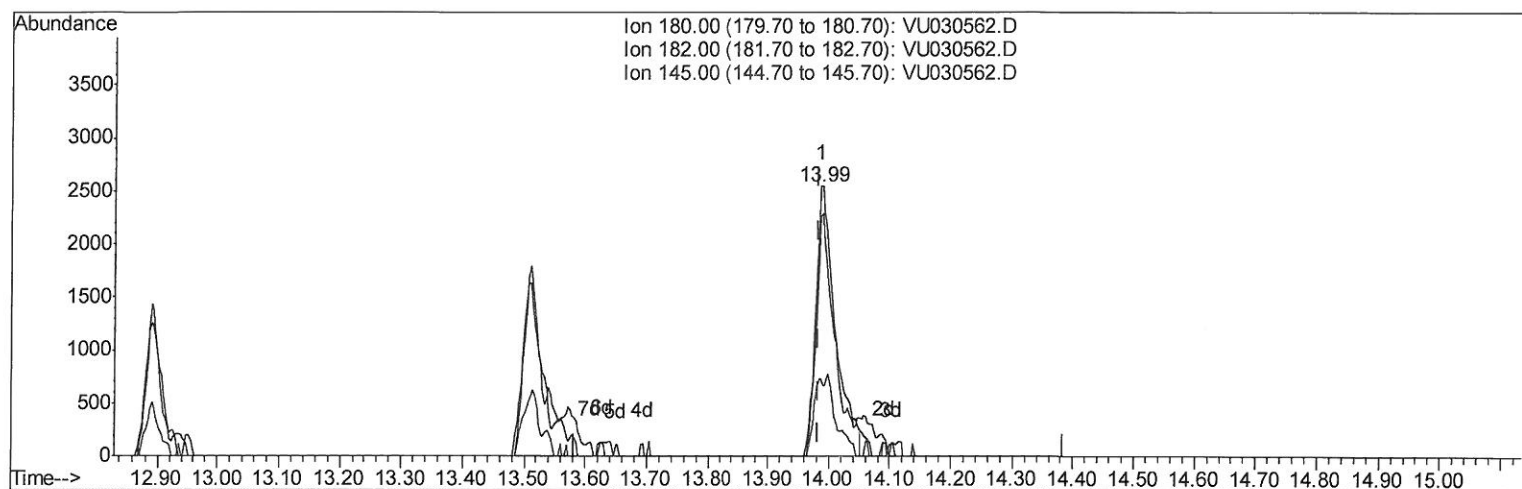

TIC: VU030562.D

(70) 1,2,3-Trichlorobenzene (T)

13.987min (+0.003) 1.55ug/L m

response 5467

Ion Exp% Act%

180.00 100 100

182.00 96.80 91.26

145.00 32.40 15.93#

0.00 0.00 0.00

70
419119

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU033019\
Quantitation Report (QT Reviewed)

Data File : VU030562.D
Acq On : 29 Mar 2019 23:41
Operator : JC/SP
Sample : K2166-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF1A8

Manual Integrations
APPROVED

MMDadoda
3/30/2019 9:59:14 AM

Quant Time: Mar 30 03:44:54 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Mar 30 02:12:04 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Difluorobenzene	5.88	114	425505	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	409701	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	156738	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	142280	41.55	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	83.10%
7) Chloroethane-d5	1.67	69	125961	46.41	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	92.82%
11) 1,1-Dichloroethene-d2	2.27	63	211548	32.57	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	65.14%
21) 2-Butanone-d5	4.17	46	324505	100.81	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	100.81%
24) Chloroform-d	4.64	84	280759	47.59	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.18%
26) 1,2-Dichloroethane-d4	5.31	65	193448	50.11	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	100.22%
32) Benzene-d6	5.34	84	548073	46.65	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.30%
36) 1,2-Dichloropropane-d6	6.33	67	204755	50.94	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	101.88%
41) Toluene-d8	7.56	98	458418	43.44	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	86.88%
43) trans-1,3-Dichloropropene-	7.85	79	83074	43.95	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	87.90%
47) 2-Hexanone-d5	8.31	63	203224	93.29	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	93.29%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	281512	48.94	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	97.88%
64) 1,2-Dichlorobenzene-d4	11.86	152	157288	50.08	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	100.16%

Target Compounds

					Qvalue
3) Chloromethane	1.33	50	6940	1.322	ug/L 98
13) Acetone	2.32	43	44786	13.757	ug/L 97
20) cis-1,2-Dichloroethene	4.22	96	6930	1.935	ug/L 87
22) 2-Butanone	4.28	43	12253m	3.114	ug/L
34) Trichloroethene	6.19	95	21488	6.267	ug/L 92
68) 1,2,4-trichlorobenzene	13.51	180	3416	1.025	ug/L 90
70) 1,2,3-Trichlorobenzene	13.99	180	5467m	1.553	ug/L

MD
4/9/19

(#) = qualifier out of range (m) = manual integration (+) = signals summed