

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU033019\
 Data File : VU030555.D
 Acq On : 29 Mar 2019 20:31
 Operator : JC/SP
 Sample : K2166-19 50X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF2L6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.183	24	29	36	rBV	18130	16872	0.97%	0.127%
2	1.399	89	96	109	rBV	231174	236282	13.58%	1.774%
3	1.672	174	181	199	rVB	190047	246282	14.15%	1.849%
4	2.270	355	367	380	rBV	358328	552590	31.76%	4.150%
5	2.456	417	425	426	rBV5	1923	2562	0.15%	0.019%
6	2.498	436	438	442	rVB2	899	561	0.03%	0.004%
7	2.521	442	445	446	rBV	514	311	0.02%	0.002%
8	2.701	492	501	511	rVB4	2658	4339	0.25%	0.033%
9	2.794	526	530	533	rBV	717	572	0.03%	0.004%
10	2.987	588	590	595	rVB3	701	416	0.02%	0.003%
11	3.019	595	600	602	rBV2	320	267	0.02%	0.002%
12	3.083	617	620	622	rBV3	364	273	0.02%	0.002%
13	3.164	641	645	651	rVB2	387	395	0.02%	0.003%
14	3.289	680	684	688	rBV2	435	311	0.02%	0.002%
15	3.341	694	700	703	rBV3	534	496	0.03%	0.004%
16	3.376	709	711	713	rBV	443	279	0.02%	0.002%
17	3.572	767	772	776	rBV2	235	303	0.02%	0.002%
18	3.710	811	815	820	rBV	297	332	0.02%	0.002%
19	3.849	855	858	864	rVB	490	399	0.02%	0.003%
20	3.955	887	891	893	rBV2	427	343	0.02%	0.003%
21	4.177	947	960	990	rBV	201302	535273	30.76%	4.020%
22	4.579	1081	1085	1089	rBV4	495	506	0.03%	0.004%
23	4.646	1089	1106	1132	rBV	282834	681741	39.18%	5.120%
24	4.823	1159	1161	1165	rBV4	551	339	0.02%	0.003%
25	4.971	1203	1207	1208	rVV2	594	367	0.02%	0.003%
26	4.980	1208	1210	1216	rVB4	470	440	0.03%	0.003%
27	5.045	1226	1230	1233	rBV2	489	359	0.02%	0.003%
28	5.080	1235	1241	1244	rVV3	517	435	0.02%	0.003%
29	5.099	1244	1247	1250	rVB	435	272	0.02%	0.002%
30	5.148	1256	1262	1267	rBV2	399	429	0.02%	0.003%
31	5.193	1272	1276	1280	rVB2	317	277	0.02%	0.002%
32	5.337	1293	1321	1369	rBV2	574222	1740143	100.00%	13.068%
33	5.701	1431	1434	1437	rVB2	362	260	0.01%	0.002%
34	5.768	1451	1455	1456	rBV2	496	356	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU033019\
 Data File : VU030555.D
 Acq On : 29 Mar 2019 20:31
 Operator : JC/SP
 Sample : K2166-19 50X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF2L6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

35	5.826	1471	1473	1477	rVB	457	264	0.02%	0.002%
36	5.884	1477	1491	1515	rBV	539852	1070812	61.54%	8.041%
37	6.186	1577	1585	1588	rVV7	1090	1274	0.07%	0.010%
38	6.205	1588	1591	1595	rVB3	594	366	0.02%	0.003%
39	6.267	1607	1610	1614	rVB2	399	267	0.02%	0.002%
40	6.328	1614	1629	1658	rBV	401402	821579	47.21%	6.170%
41	6.553	1695	1699	1701	rBV3	531	366	0.02%	0.003%
42	6.620	1716	1720	1726	rBV4	740	854	0.05%	0.006%
43	6.874	1796	1799	1801	rBV3	894	700	0.04%	0.005%
44	6.942	1816	1820	1824	rVB3	434	426	0.02%	0.003%
45	7.022	1838	1845	1848	rBV3	432	537	0.03%	0.004%
46	7.144	1879	1883	1888	rVB2	315	327	0.02%	0.002%
47	7.225	1896	1908	1932	rBV	205592	378997	21.78%	2.846%
48	7.414	1963	1967	1970	rBV5	758	846	0.05%	0.006%
49	7.485	1987	1989	1992	rVB2	496	305	0.02%	0.002%
50	7.562	2000	2013	2047	rBV	703108	1247712	71.70%	9.370%
51	7.807	2087	2089	2091	rBV2	436	263	0.02%	0.002%
52	7.848	2091	2102	2127	rVV	143267	258227	14.84%	1.939%
53	8.035	2157	2160	2163	rBV4	506	276	0.02%	0.002%
54	8.054	2163	2166	2168	rVV4	560	263	0.02%	0.002%
55	8.115	2181	2185	2187	rBV3	414	265	0.02%	0.002%
56	8.154	2193	2197	2200	rBV2	404	368	0.02%	0.003%
57	8.176	2200	2204	2209	rVB3	862	707	0.04%	0.005%
58	8.225	2209	2219	2234	rBV2	33553	58340	3.35%	0.438%
59	8.308	2234	2245	2287	rBV	638291	1195274	68.69%	8.976%
60	8.710	2367	2370	2373	rVB3	563	298	0.02%	0.002%
61	8.784	2390	2393	2397	rBV3	461	448	0.03%	0.003%
62	8.858	2414	2416	2422	rVB3	420	293	0.02%	0.002%
63	8.890	2422	2426	2429	rBV	487	389	0.02%	0.003%
64	8.938	2438	2441	2446	rVB2	530	503	0.03%	0.004%
65	8.974	2446	2452	2462	rBV3	879	1497	0.09%	0.011%
66	9.025	2462	2468	2470	rBV3	348	388	0.02%	0.003%
67	9.086	2473	2487	2511	rBV	775328	1307960	75.16%	9.822%
68	9.405	2584	2586	2591	rVB2	454	345	0.02%	0.003%
69	9.430	2591	2594	2597	rBV	523	366	0.02%	0.003%
70	9.472	2603	2607	2608	rBV	430	281	0.02%	0.002%
71	9.623	2651	2654	2657	rBV	394	285	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU033019\
 Data File : VU030555.D
 Acq On : 29 Mar 2019 20:31
 Operator : JC/SP
 Sample : K2166-19 50X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BF2L6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis

72	9.961	2755	2759	2762	rVB2	539	377	0.02%	0.003%
73	10.112	2803	2806	2812	rVB2	420	396	0.02%	0.003%
74	10.241	2844	2846	2850	rVB2	675	400	0.02%	0.003%
75	10.266	2850	2854	2862	rBB3	266	296	0.02%	0.002%
76	10.427	2887	2904	2929	rBV	558855	908203	52.19%	6.820%
77	10.598	2954	2957	2962	rVV4	428	367	0.02%	0.003%
78	10.707	2985	2991	2994	rVB2	292	297	0.02%	0.002%
79	10.945	3059	3065	3066	rBV	322	328	0.02%	0.002%
80	10.990	3075	3079	3083	rBV2	408	367	0.02%	0.003%
81	11.041	3092	3095	3098	rVB2	457	272	0.02%	0.002%
82	11.061	3098	3101	3104	rVB2	783	445	0.03%	0.003%
83	11.090	3108	3110	3114	rVB	512	270	0.02%	0.002%
84	11.192	3138	3142	3145	rBV3	285	295	0.02%	0.002%
85	11.289	3169	3172	3177	rVB	482	395	0.02%	0.003%
86	11.347	3186	3190	3191	rBV	536	347	0.02%	0.003%
87	11.379	3195	3200	3203	rBV2	366	394	0.02%	0.003%
88	11.482	3219	3232	3259	rBV	611963	1007365	57.89%	7.565%
89	11.742	3309	3313	3317	rBV4	875	870	0.05%	0.007%
90	11.858	3335	3349	3381	rBV	590922	1012281	58.17%	7.602%
91	12.411	3517	3521	3524	rBV3	571	412	0.02%	0.003%
92	12.466	3535	3538	3540	rBV	642	469	0.03%	0.004%
93	12.543	3559	3562	3565	rBV	457	295	0.02%	0.002%
94	12.675	3601	3603	3606	rVB2	458	271	0.02%	0.002%
95	12.726	3616	3619	3623	rBB3	553	364	0.02%	0.003%
96	13.199	3764	3766	3770	rBV2	432	332	0.02%	0.002%
97	13.270	3783	3788	3791	rBV3	611	570	0.03%	0.004%
98	13.298	3795	3797	3800	rVB2	557	295	0.02%	0.002%
99	13.334	3805	3808	3814	rBV3	607	703	0.04%	0.005%
100	13.684	3914	3917	3921	rBV	678	489	0.03%	0.004%


Sum of corrected areas: 13316215

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU033019\
Data File : VU030555.D
Acq On : 29 Mar 2019 20:31
Operator : JC/SP
Sample : K2166-19 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BF2L6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

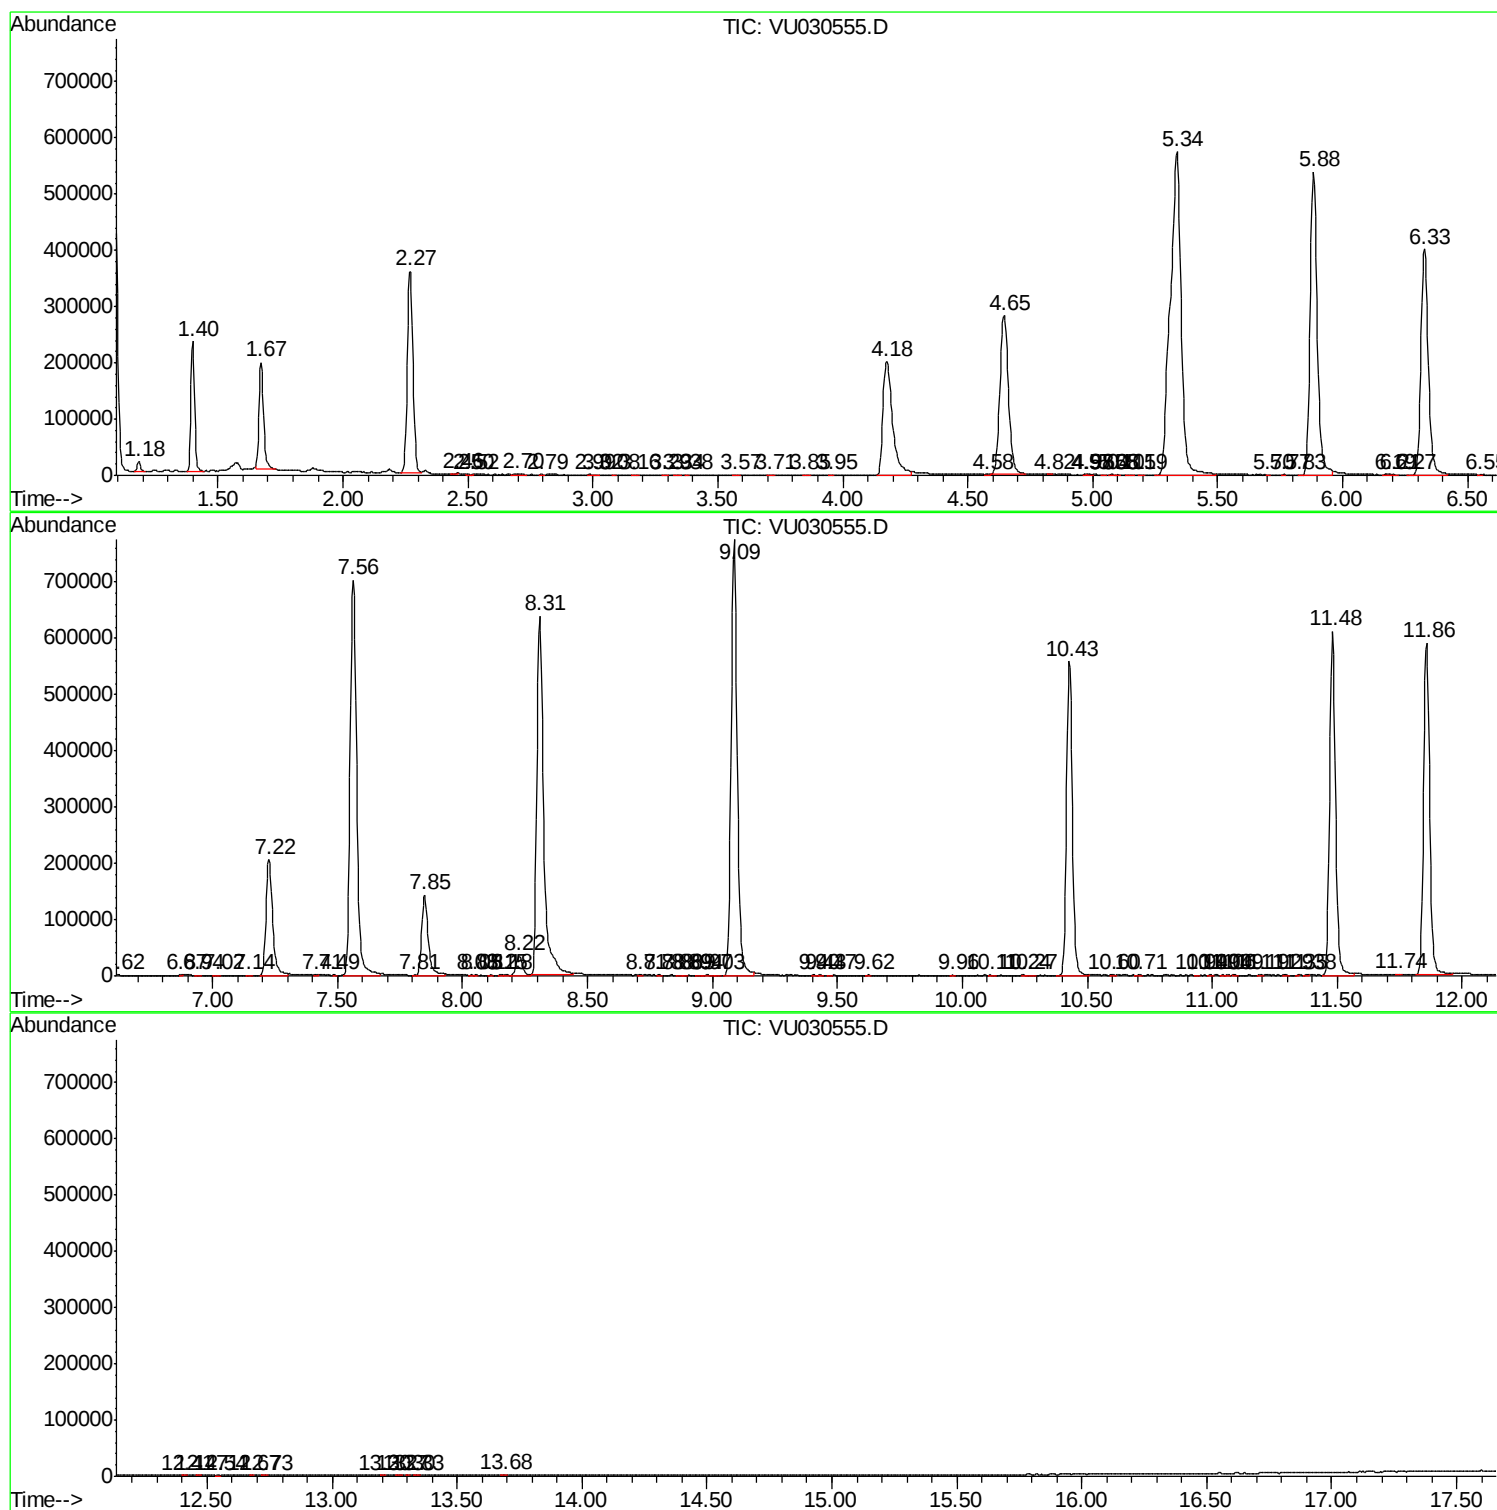

DbaaaPathh::ZZ\VV0ASRVNREBBBMM\MSVOA\UNDA\AA\VV0030099\
 DbaaaFile::VV0000555DD
 Aaqq00n::209Mar2009 200331
 Opeaaor::J008BP
 Saaapbe::K02666199500X
 Mmsc::5500m\MSVOA\UNDA\AA\VV0030099\
 AASSVaal::122 SaaapbeMMuipbeer:11

Instrument :
 MSVOA_U
 ClientSampleId :
 BF2L6

QqaabtMebbdd::ZZ\VV0ASRVNREBBBMM\MSVOA\UNDA\AA\VV0030099\
 QqaabtFile::VV0CAAA\ysiss

TICCLibbaay::CC\DATA\BASSEN\SI11LL
 TICInteggaionPaaameess:LS6CNTPP

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc

No Library Search Compounds Detected
