


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU033019\
 Data File : VU030544.D
 Acq On : 29 Mar 2019 16:01
 Operator : JC/SP
 Sample : BFB47
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB47

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM032319WMA.M
 Title : VOC Analysis
 Last Update : Tue Apr 02 08:36:56 2019

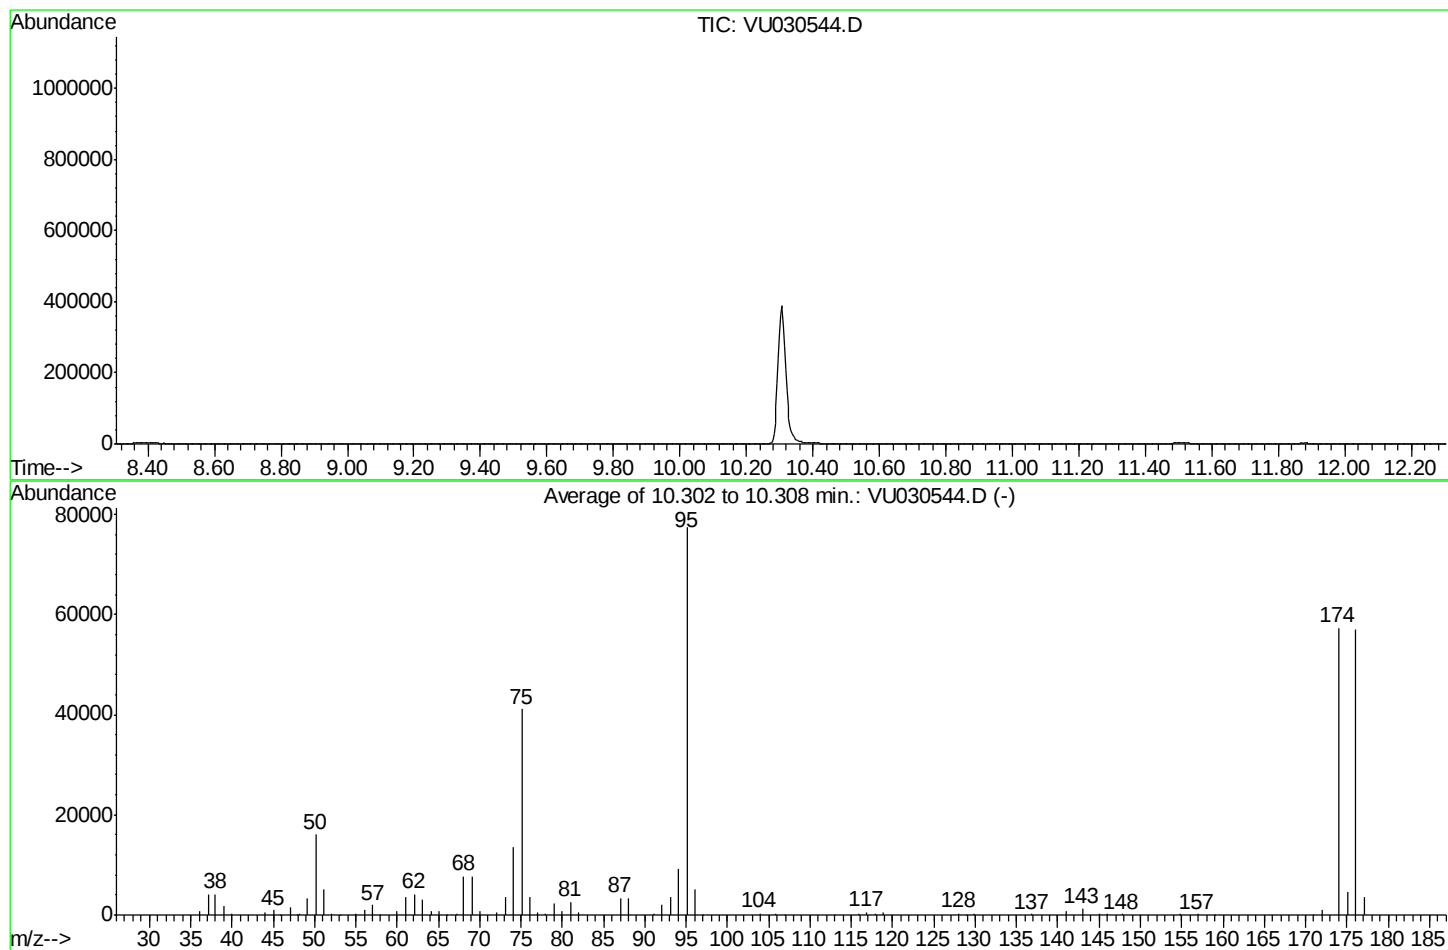

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2854

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.8	16088	PASS
75	95	30	80	53.1	41090	PASS
95	95	100	100	100.0	77405	PASS
96	95	5	9	6.5	5057	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	74.1	57325	PASS
175	174	5	9	8.1	4636	PASS
176	174	95	101	99.6	57098	PASS
177	176	5	9	6.4	3629	PASS

Scan 2854 (10.266 min): VU030544.D
BFB47

m/z	Abundance
40.00	314.0
44.00	577.0

Instrument :
MSVOA_U
ClientSampleId :
BFB47

m/z	Abundance
36.00	762.0
37.10	3812.0
38.00	4007.0
39.00	1554.0
40.10	475.0
44.00	1107.0
45.00	817.0
45.80	100.0
47.00	1470.0
48.10	470.0
49.10	3283.0
50.10	16400.0
51.00	4889.0
52.10	172.0
53.10	121.0
55.00	233.0
56.10	1111.0
57.10	1976.0
57.90	164.0
60.00	686.0
61.00	3597.0
62.10	4040.0
63.10	3162.0
64.10	832.0
65.00	837.0
66.00	101.0
67.20	226.0
68.00	8066.0
69.10	7746.0
70.00	705.0
72.00	578.0
73.10	3593.0
74.10	12832.0
75.10	40888.0
76.10	3241.0
77.00	429.0
77.90	403.0
79.00	2182.0
80.00	787.0
81.00	2630.0
82.00	545.0
87.10	3486.0
88.00	3342.0
91.00	233.0
92.00	2261.0
93.10	3706.0
94.10	8917.0
95.10	77328.0
96.10	5009.0
104.00	353.0
105.80	340.0
107.00	132.0
116.00	213.0
116.90	609.0
117.90	317.0
118.90	420.0
128.00	277.0
128.90	114.0
129.90	215.0
136.90	189.0
141.00	820.0
143.00	1211.0
145.00	266.0
146.00	124.0
147.80	238.0
154.80	132.0
156.90	183.0
159.00	128.0
170.90	127.0
172.00	1067.0
174.00	58808.0
175.10	4721.0
176.00	57392.0
177.10	3641.0

Instrument :
MSVOA_U
ClientSampleId :
BFB47

m/z	Abundance
36.00	823.0
37.10	4132.0
38.00	4369.0
39.00	1802.0
40.00	480.0
44.00	1163.0
45.10	973.0
45.90	113.0
47.10	1526.0
48.10	400.0
49.10	3510.0
50.10	16752.0
51.00	5294.0
52.10	182.0
53.10	134.0
55.00	237.0
56.10	1177.0
57.10	2017.0
58.10	132.0
60.00	670.0
61.10	3636.0
62.10	4404.0
63.10	3151.0
64.10	771.0
65.10	929.0
66.00	107.0
67.20	280.0
68.00	7915.0
69.10	7941.0
70.00	697.0
72.00	643.0
73.10	3587.0
74.10	13880.0
75.10	42128.0
76.10	3668.0
76.90	381.0
77.80	379.0
79.00	2247.0
80.00	834.0
81.00	2750.0
81.90	589.0
87.10	3468.0
88.00	3311.0
91.10	268.0
92.00	2141.0
93.10	3682.0
94.10	9560.0
95.10	79904.0
96.10	5193.0
97.00	126.0
103.90	329.0
105.80	343.0
107.00	135.0
115.90	244.0
116.90	621.0
117.90	331.0
118.90	596.0
128.00	281.0
129.90	270.0
136.90	191.0
141.00	812.0
143.00	1269.0
145.10	298.0
145.90	157.0
147.80	242.0
154.80	150.0
156.90	180.0
171.00	105.0
172.00	1064.0
174.00	58920.0
175.10	4838.0
176.00	58856.0
177.00	3759.0

Instrument :
MSVOA_U
ClientSampleId :
BFB47

m/z	Abundance
36.00	841.0
37.10	4005.0
38.00	3968.0
39.00	1828.0
40.00	510.0
44.00	1088.0
45.10	925.0
45.90	134.0
47.10	1474.0
47.90	371.0
49.10	3459.0
50.10	15113.0
51.10	4946.0
52.10	204.0
54.90	224.0
56.10	1160.0
57.00	1916.0
60.00	629.0
61.10	3450.0
62.10	4163.0
63.10	2897.0
64.00	693.0
65.10	925.0
67.20	289.0
68.10	7370.0
69.10	7327.0
70.00	641.0
72.00	656.0
73.00	3245.0
74.10	13611.0
75.10	40256.0
76.10	3572.0
76.90	408.0
78.00	387.0
79.00	2154.0
80.00	758.0
81.00	2518.0
81.90	562.0
87.00	3089.0
88.00	3021.0
91.00	286.0
92.00	1990.0
93.10	3371.0
94.10	8993.0
95.10	74984.0
96.10	4969.0
97.00	158.0
103.90	292.0
105.90	259.0
106.90	122.0
112.90	100.0
115.90	239.0
116.90	513.0
117.90	273.0
118.90	616.0
128.00	259.0
129.90	279.0
136.90	149.0
141.00	702.0
143.00	1201.0
145.10	276.0
145.90	143.0
147.80	191.0
154.90	179.0
157.00	123.0
171.10	130.0
172.00	943.0
174.00	54248.0
175.10	4350.0
176.00	55048.0
177.00	3488.0

Instrument :
MSVOA_U
ClientSampleId :
BFB47