

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU033021\
 Data File : VU042838.D
 Acq On : 30 Mar 2021 14:46
 Operator : SY/MD
 Sample : VIBLK20
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK20

Quant Time: Mar 31 02:10:54 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Mar 31 02:07:34 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.259	114	73794	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.427	117	73955	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.822	152	35620	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.604	65	19970	4.06	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery = 81.20%			
7) Chloroethane-d5	1.919	69	18213	4.89	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery = 97.80%			
11) 1,1-Dichloroethene-d2	2.575	63	34871	3.14	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery = 62.80%			
20) 2-Butanone-d5	4.649	46	65230	40.38	ug/L	0.00
Spiked Amount 50.000	Range 40 - 130		Recovery = 80.76%			
24) Chloroform-d	5.073	84	47807	4.91	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery = 98.20%			
26) 1,2-Dichloroethane-d4	5.713	65	29663	4.96	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery = 99.20%			
32) Benzene-d6	5.739	84	83091	4.58	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery = 91.60%			
36) 1,2-Dichloropropane-d6	6.703	67	28215	4.82	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery = 96.40%			
41) Toluene-d8	7.906	98	74660	4.22	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery = 84.40%			
43) trans-1,3-Dichloroprop...	8.192	79	11064	4.05	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery = 81.00%			
46) 2-Hexanone-d5	8.648	63	61312	46.86	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery = 93.72%			
57) 1,1,2,2-Tetrachloroeth...	10.767	84	24768	4.75	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery = 95.00%			
64) 1,2-Dichlorobenzene-d4	12.201	152	31548	4.89	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery = 97.80%			
Target Compounds						Qvalue
16) Methylene chloride	3.054	84	1031	0.17	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU033021\
Data File : VU042838.D
Acq On : 30 Mar 2021 14:46
Operator : SY/MD
Sample : VIBLK20
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK20

Quant Time: Mar 31 02:10:54 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Mar 31 02:07:34 2021
Response via : Initial Calibration

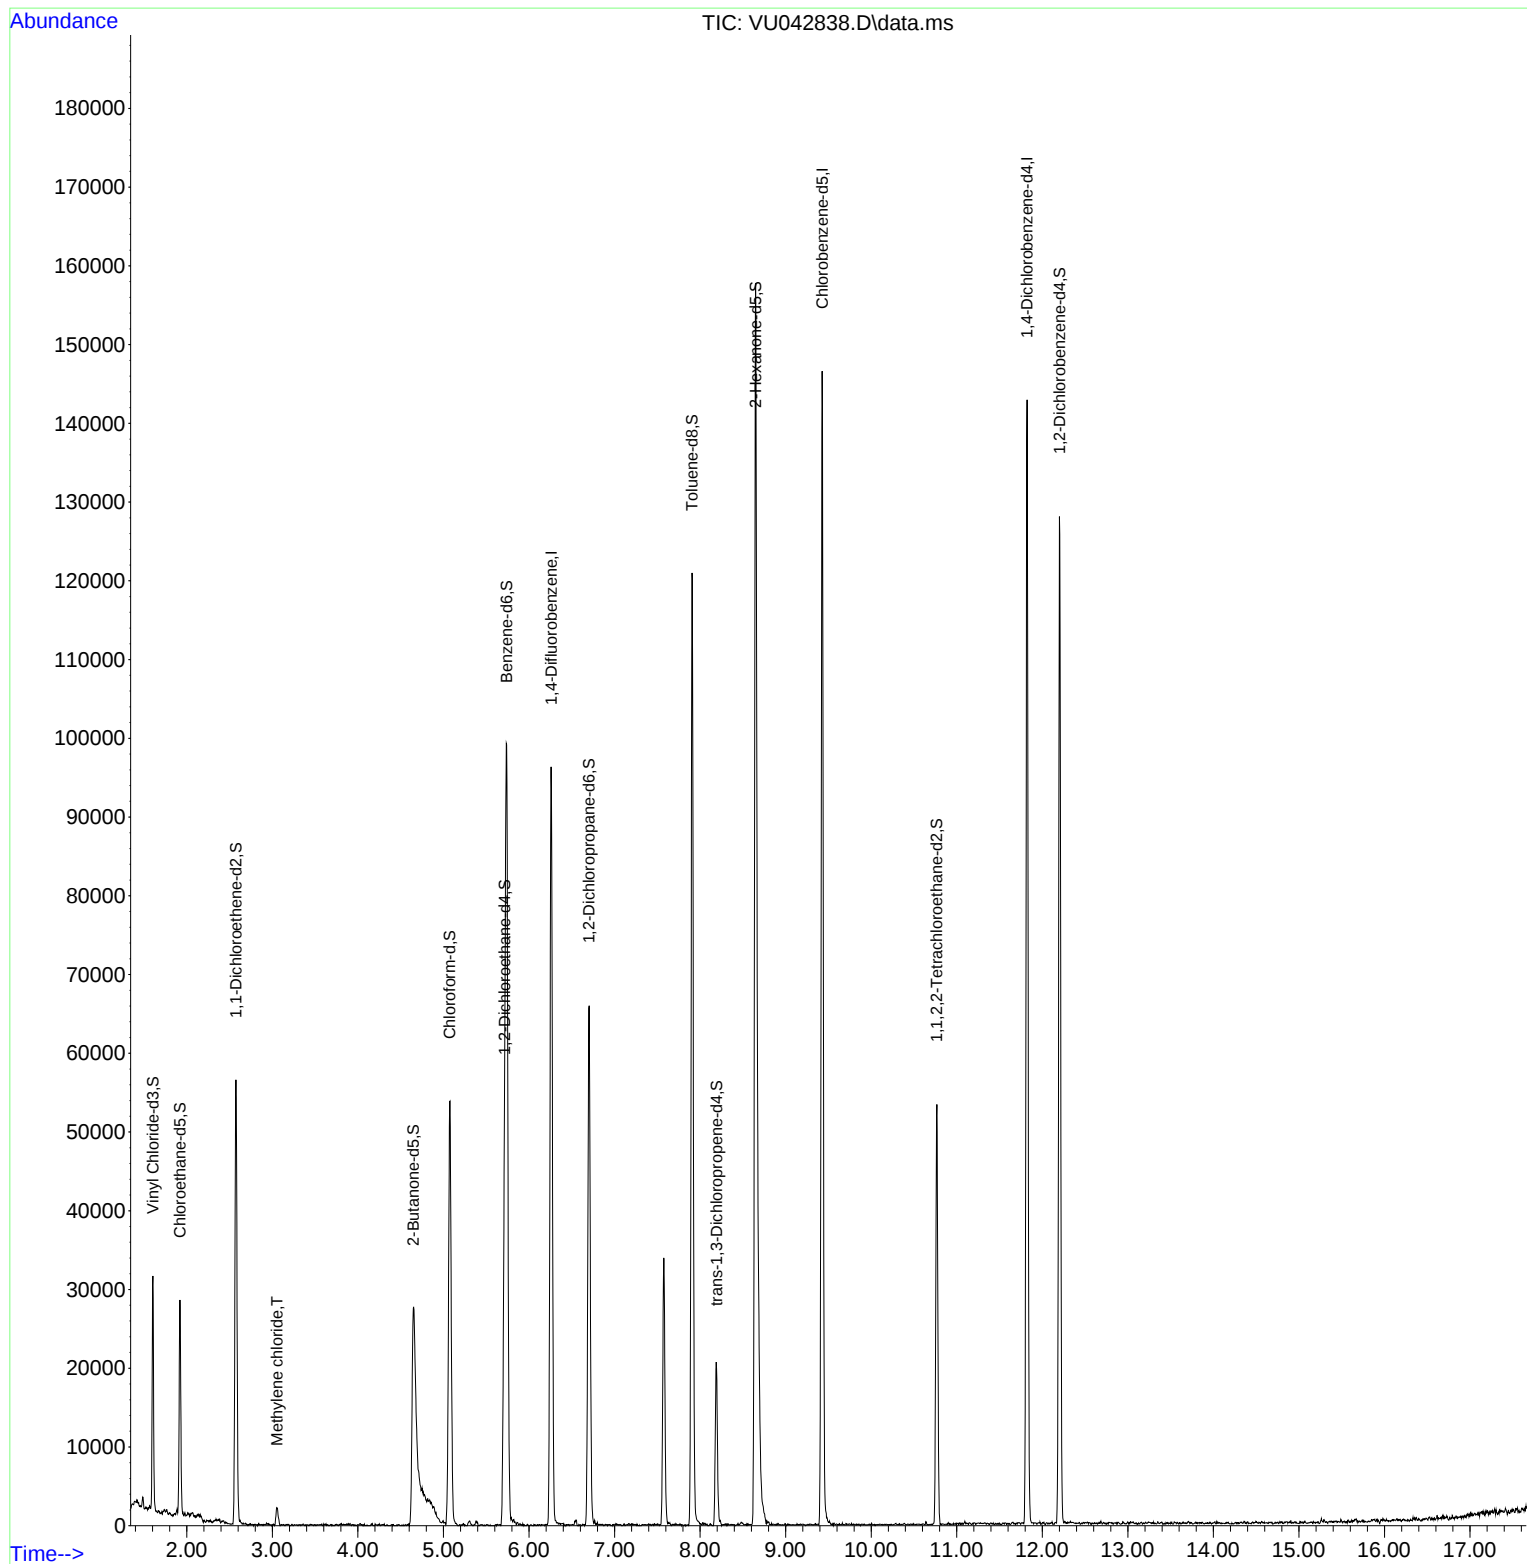

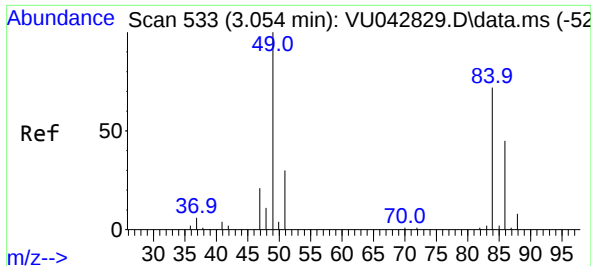

#16
Methylene chloride
Concen: 0.17 ug/L
RT: 3.054 min Scan# 533
Delta R.T. -0.000 min
Lab File: VU042838.D
Acq: 30 Mar 2021 14:46

Instrument :
MSVOA_U
ClientSampleId :
VIBLK20

Tgt Ion:	84	Resp:	1031
Ion	Ratio	Lower	Upper
84	100		
86	56.2	44.1	81.9
49	135.8	95.0	176.4

