


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU033021\
Data File : VU042828.D
Acq On : 30 Mar 2021 09:30
Operator : SY/MD
Sample : BFB30
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB30

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SOMUTR030221WMA.M
Title : TRACE VOA SOM01.0
Last Update : Wed Mar 31 02:07:34 2021

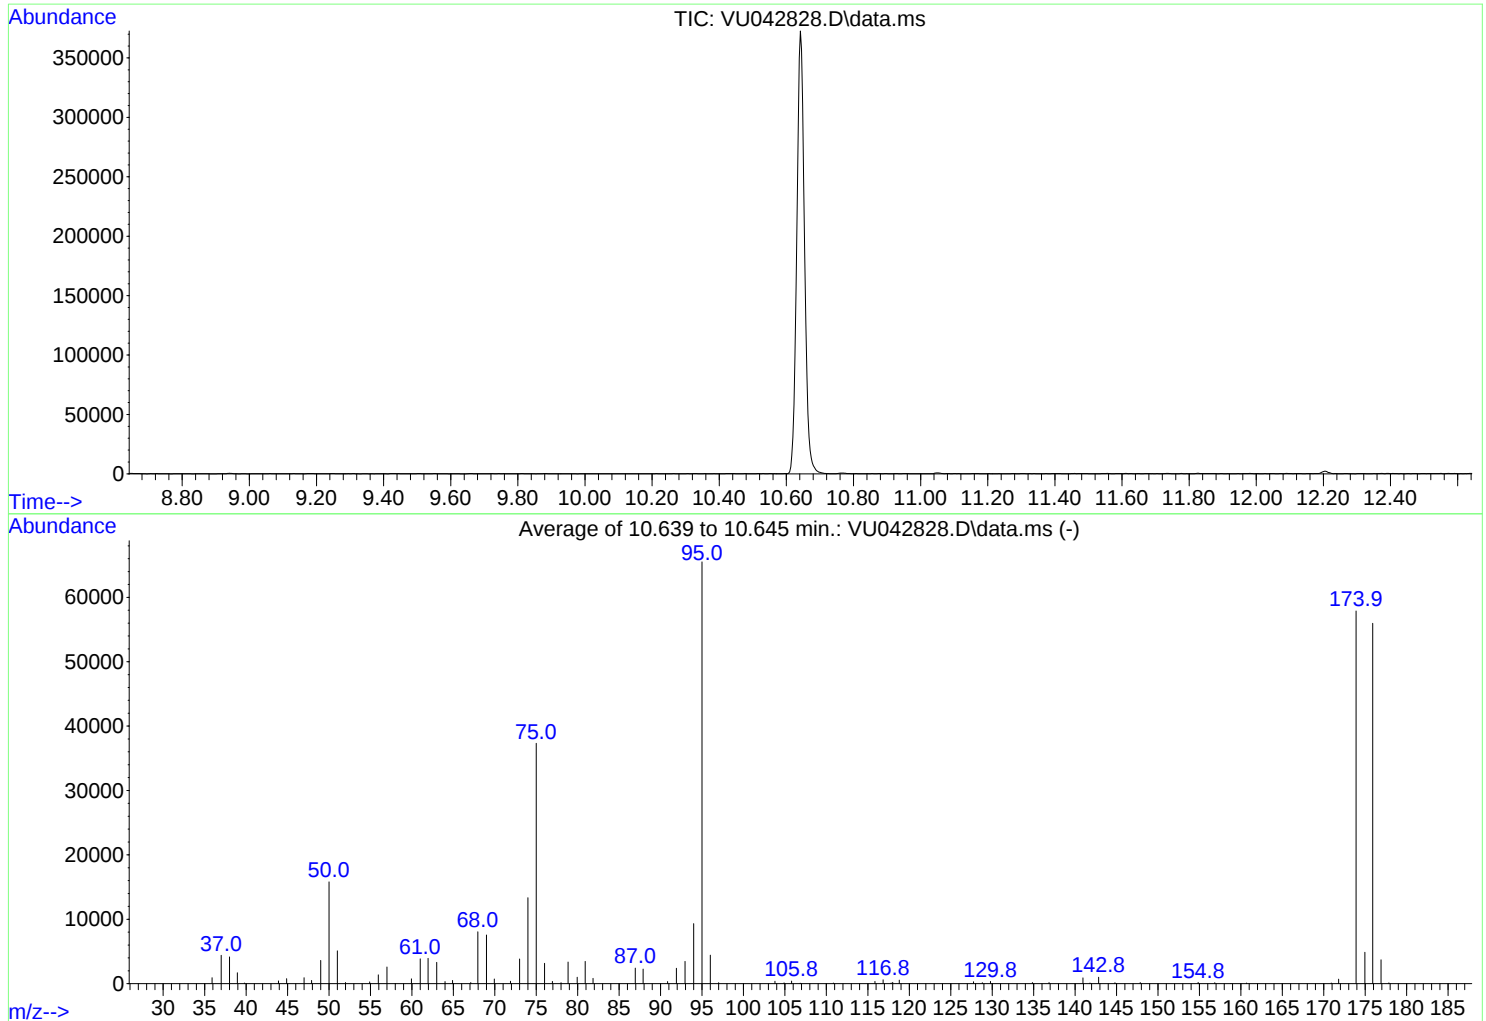

AutoFind: Scans 2892, 2893, 2894; Background Corrected with Scan 2879

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	24.1	15807	PASS
75	95	30	80	57.0	37325	PASS
95	95	100	100	100.0	65515	PASS
96	95	5	9	6.7	4420	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	88.3	57872	PASS
175	174	5	9	8.4	4882	PASS
176	174	95	101	96.7	55968	PASS
177	176	5	9	6.6	3714	PASS

m/z	Abundance
43.90	240.0

Instrument :
MSVOA_U
ClientSampleId :
BFB30

m/z	Abundance
35.90	930.0
37.00	4609.0
38.00	4180.0
38.90	1671.0
39.80	124.0
43.90	700.0
44.90	739.0
47.00	1003.0
47.90	469.0
49.00	3514.0
50.00	15981.0
51.00	5099.0
52.00	174.0
54.90	311.0
56.00	1405.0
57.00	2647.0
58.00	106.0
60.00	754.0
61.00	3842.0
61.90	3908.0
63.00	3484.0
64.00	286.0
64.90	492.0
67.10	277.0
68.00	8062.0
69.00	7325.0
70.00	798.0
71.90	341.0
73.00	3738.0
74.00	13104.0
75.00	36528.0
76.00	3021.0
77.00	317.0
78.00	140.0
78.90	3370.0
79.90	1043.0
80.90	3436.0
81.80	735.0
87.00	2418.0
87.90	2266.0
90.90	323.0
91.90	2472.0
93.00	3331.0
94.00	8988.0
95.00	63408.0
96.00	4156.0
97.00	171.0
103.80	388.0
104.80	115.0
105.80	383.0
110.80	116.0
115.90	357.0
116.90	600.0
117.80	288.0
118.80	564.0
127.80	273.0
128.80	137.0
129.80	341.0
134.80	155.0
136.90	171.0
140.90	841.0
142.90	1003.0
144.80	146.0
147.80	163.0
154.80	181.0
156.80	129.0
160.70	165.0
171.80	772.0
173.90	54936.0
174.90	4563.0
175.90	53264.0
176.90	3508.0
177.80	128.0

Instrument :
MSVOA_U
ClientSampleId :
BFB30

m/z	Abundance
35.90	945.0
37.00	4539.0
38.00	4335.0
39.00	1748.0
39.80	119.0
43.90	676.0
44.90	799.0
47.00	950.0
47.90	529.0
49.00	3712.0
50.00	16367.0
51.00	5318.0
52.00	185.0
54.90	291.0
56.00	1399.0
57.00	2681.0
59.90	772.0
61.00	3976.0
62.00	4077.0
63.00	3425.0
64.00	337.0
64.90	541.0
67.10	244.0
67.90	8362.0
69.00	7754.0
70.00	744.0
71.90	412.0
73.00	3992.0
74.00	13804.0
75.00	38544.0
76.00	3252.0
76.90	342.0
78.00	149.0
78.80	3465.0
79.90	1040.0
80.90	3538.0
81.80	826.0
86.90	2426.0
87.90	2338.0
90.90	341.0
91.90	2464.0
93.00	3584.0
94.00	9660.0
95.00	67936.0
96.00	4603.0
97.00	141.0
103.80	406.0
104.90	120.0
105.80	412.0
106.80	104.0
110.80	107.0
115.80	360.0
116.80	620.0
118.00	283.0
118.80	588.0
127.80	322.0
128.80	166.0
129.80	351.0
134.80	179.0
136.90	165.0
140.90	900.0
141.80	137.0
142.90	1020.0
144.80	166.0
147.90	174.0
154.80	186.0
156.80	166.0
160.70	151.0
170.90	115.0
171.80	737.0
173.90	60056.0
175.00	5058.0
175.90	57912.0
176.90	3870.0
177.90	113.0

Instrument :
MSVOA_U
ClientSampleId :
BFB30

m/z	Abundance
35.90	850.0
37.00	4026.0
38.00	3956.0
39.00	1676.0
39.80	101.0
43.90	650.0
44.90	753.0
47.00	778.0
47.90	522.0
49.00	3555.0
50.00	15073.0
51.00	4886.0
52.00	186.0
54.90	242.0
55.90	1263.0
57.00	2413.0
59.90	725.0
61.00	3720.0
62.00	3817.0
63.00	3027.0
64.00	386.0
64.90	493.0
67.90	7774.0
69.00	7596.0
69.90	629.0
71.90	393.0
73.00	3774.0
74.00	13167.0
75.00	36904.0
76.00	3225.0
76.90	420.0
78.00	160.0
78.80	3214.0
80.00	900.0
80.90	3380.0
81.90	896.0
86.90	2366.0
87.90	2207.0
90.80	343.0
91.90	2222.0
92.90	3424.0
94.00	9285.0
95.00	65200.0
96.00	4500.0
97.00	107.0
103.80	355.0
105.00	150.0
105.80	396.0
106.90	115.0
110.90	102.0
115.80	336.0
116.80	596.0
118.00	311.0
118.80	505.0
127.70	339.0
128.80	160.0
129.80	347.0
134.90	178.0
136.80	165.0
141.00	942.0
141.80	153.0
142.80	950.0
144.80	171.0
147.90	156.0
154.90	197.0
156.90	175.0
158.80	107.0
170.90	170.0
171.80	615.0
173.90	58624.0
175.00	5026.0
175.90	56728.0
176.90	3764.0
177.90	106.0

Instrument :
MSVOA_U
ClientSampleId :
BFB30